

Quantitation Report (QT Reviewed)


Instrument :
BNA_E
ClientSampled :
C0ZZ1

Manual Integrations
APPROVED

Sohil
8/18/2017 7:08:33 PM

Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
Data File : BE093864.D
Acq On : 17 Aug 2017 14:24
Operator : SJ/JU
Sample : I4693-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Aug 17 19:41:23 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 02:52:40 2017
Response via : Initial Calibration

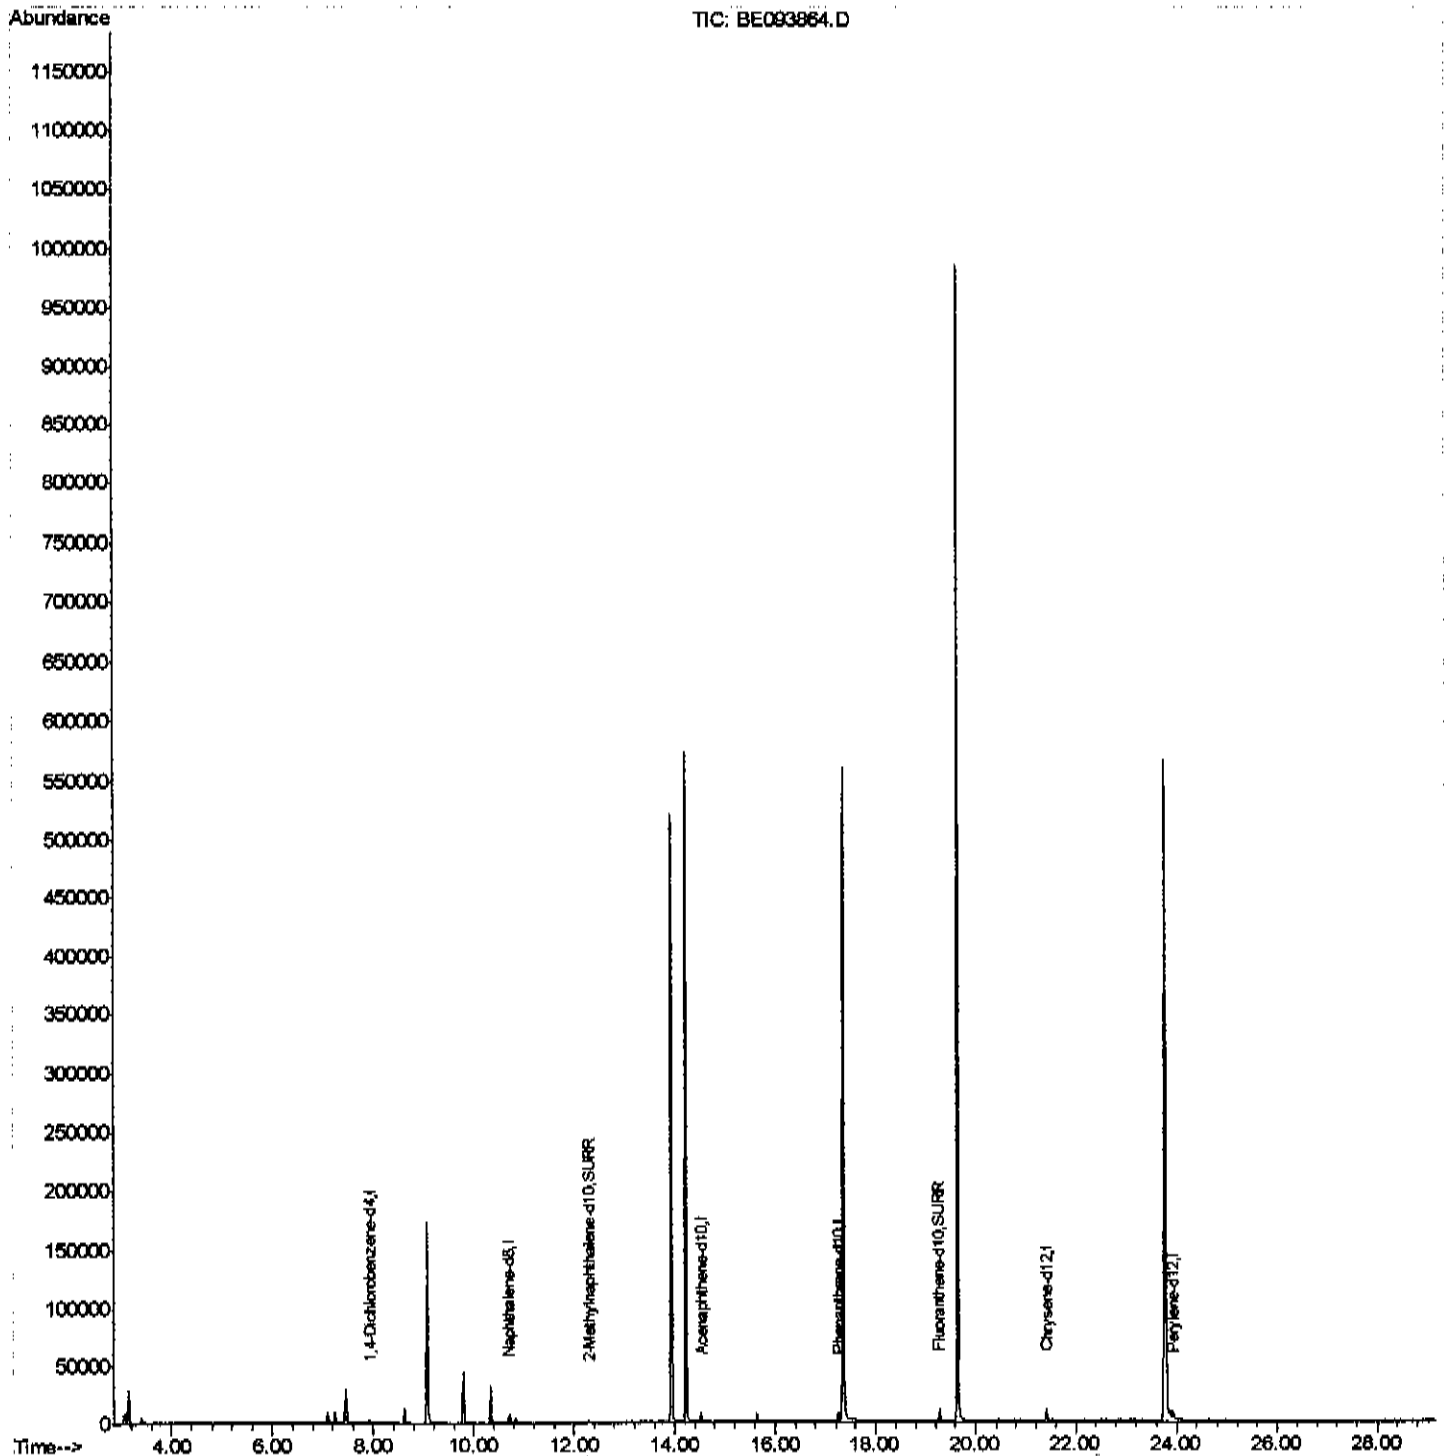

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093864.D
 Acq On : 17 Aug 2017 14:24
 Operator : SJ/JU
 Sample : I4693-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0ZZ1

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:33 PM

Quant Time: Aug 17 18:05:00 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 02:52:40 2017
 Response via : Initial Calibration

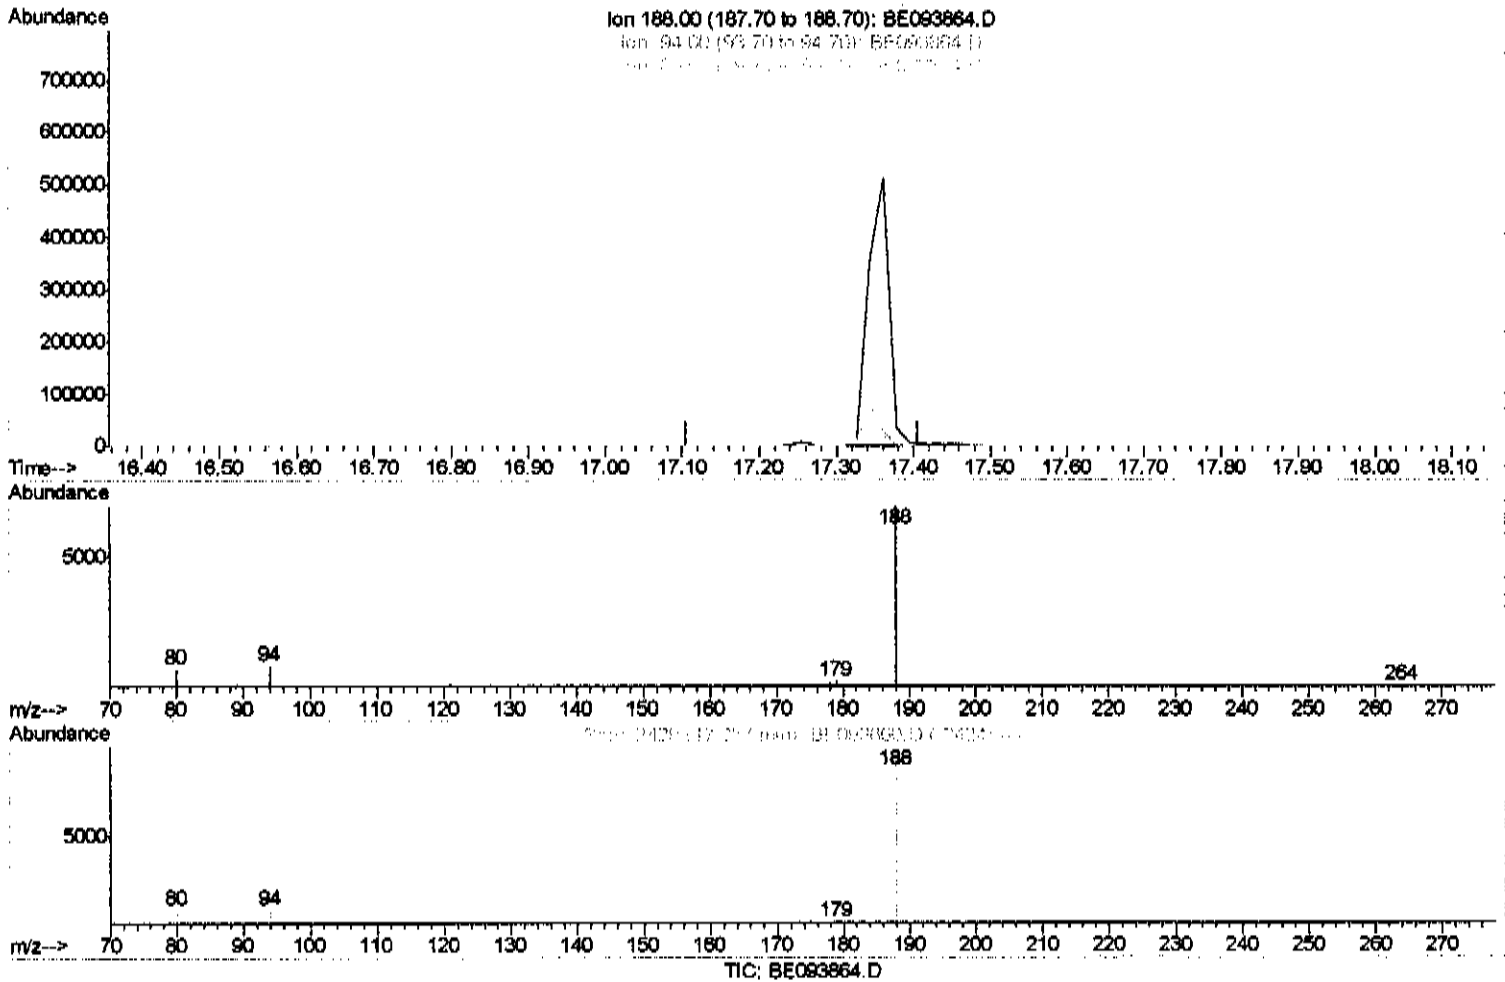

(10) Phenanthrene-d10 (I)
 17.256min (-17.256) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00%
80.00	11.80	0.00%
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093864.D
 Acq On : 17 Aug 2017 14:24
 Operator : SJ/JU
 Sample : I4693-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0ZZ1

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:33 PM

Quant Time: Aug 17 18:05:00 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 02:52:40 2017
 Response via : Initial Calibration

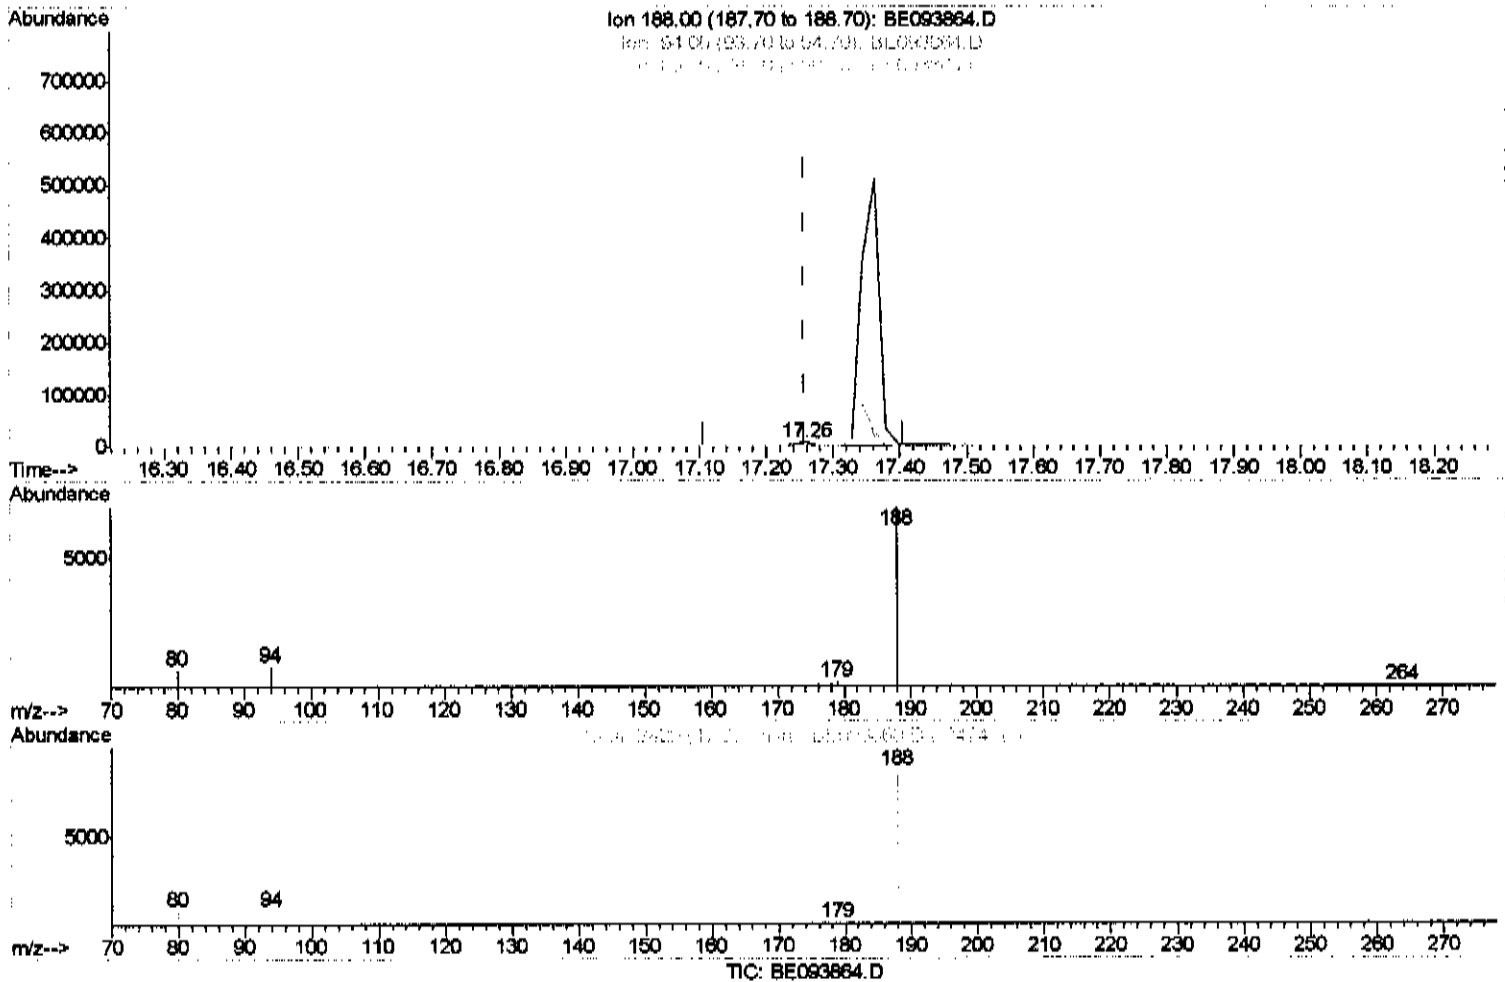

(10) Phenanthrene-d10 (I)

17.257min (+0.001) 0.40ng/ul m

response 10696

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.87
80.00	11.80	10.01
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093864.D
 Acq On : 17 Aug 2017 14:24
 Operator : SJ/JU
 Sample : I4693-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0ZZ1

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:33 PM

Quant Time: Aug 17 19:39:38 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 02:52:40 2017
 Response via : Initial Calibration

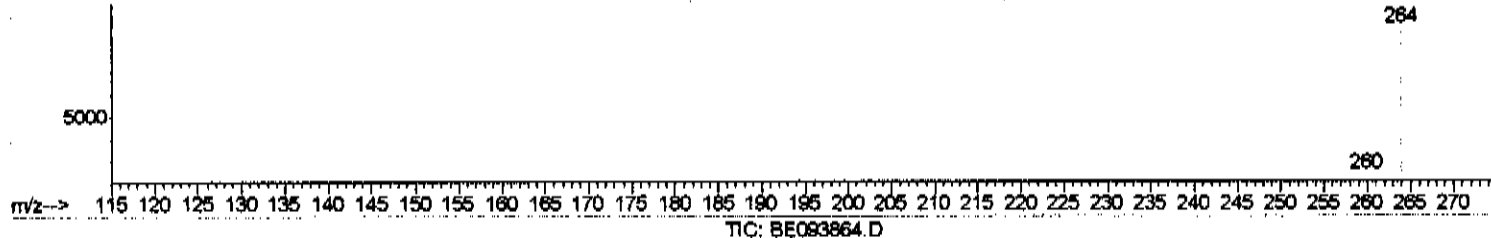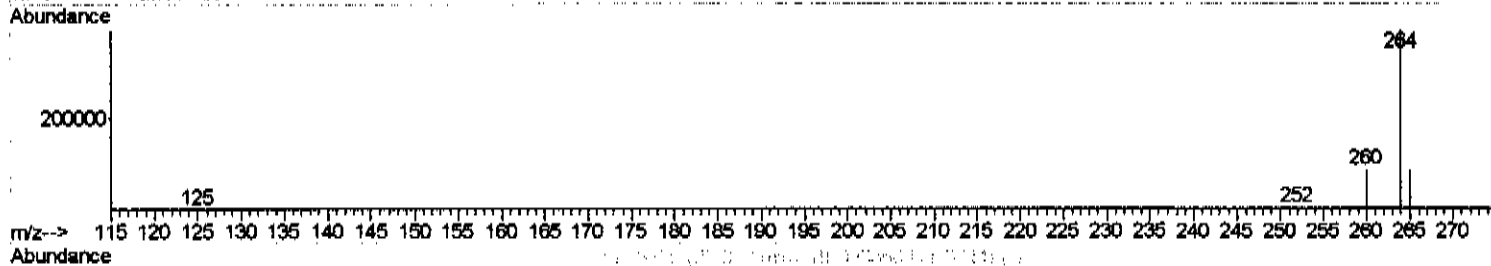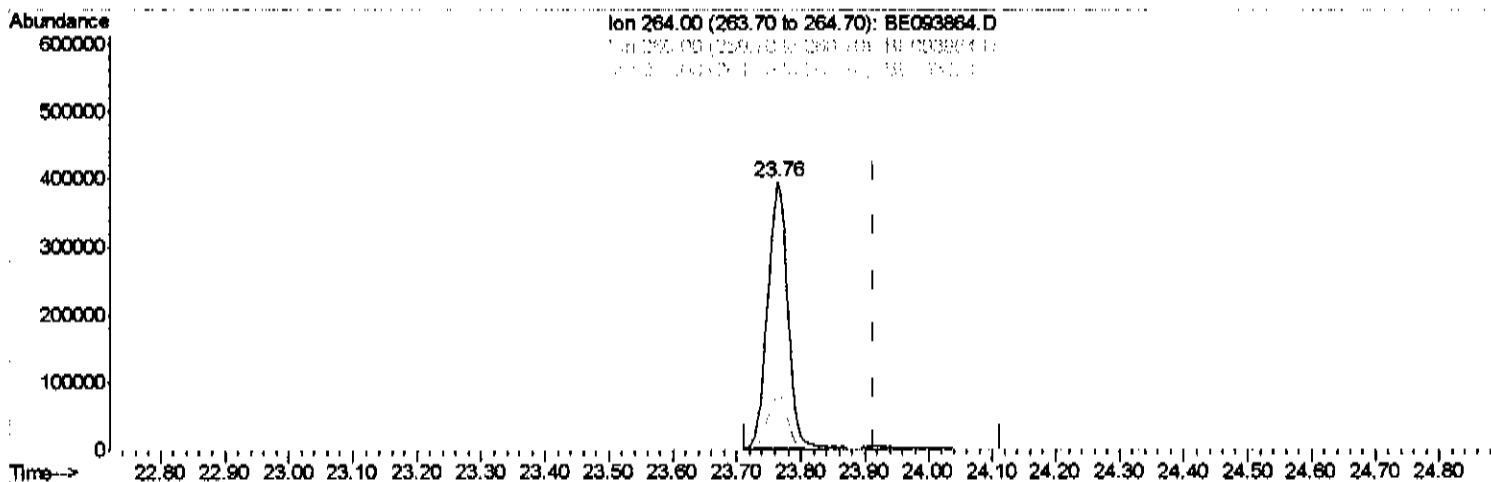

(20) Perylene-d12 (I)

23.784min (-0.151) 0.40ng/ul

response 839596

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.44#
265.00	103.50	21.27#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093864.D
 Acq On : 17 Aug 2017 14:24
 Operator : SJ/JU
 Sample : I4693-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0ZZ1

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:33 PM

Quant Time: Aug 17 19:39:38 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 02:52:40 2017
 Response via : Initial Calibration

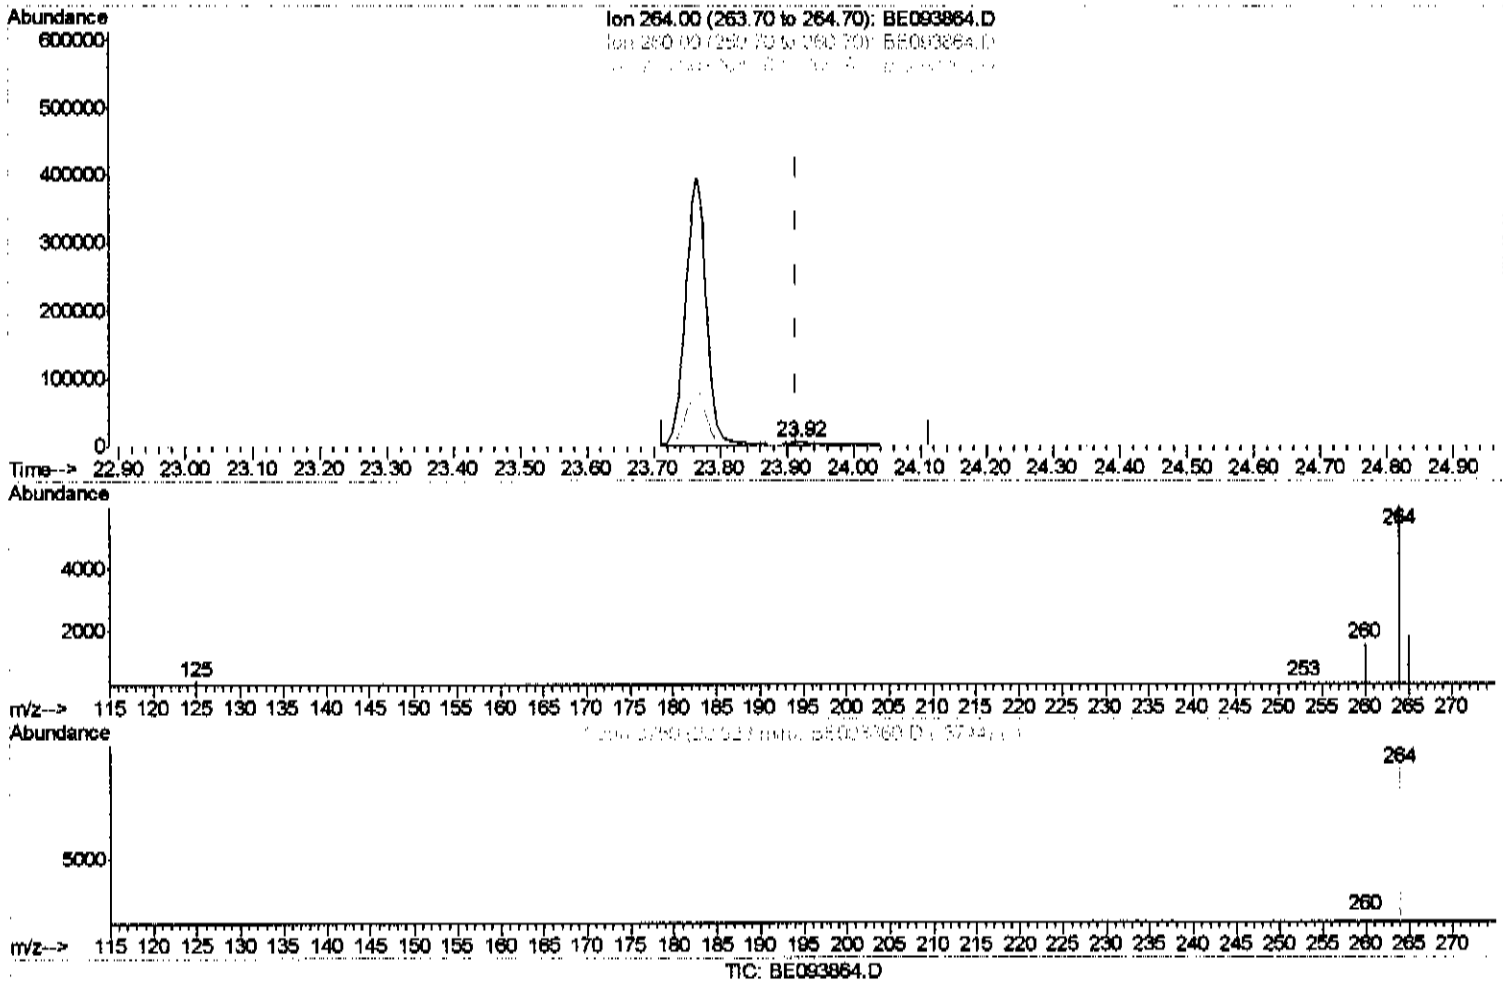

(20) Perylene-d12 (I)

23.918min (+0.004) 0.40ng/ul m

response 7720

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	28.10
265.00	103.50	30.39%
0.00	0.00	0.00

SJ
 8/18/17

Quantitation Report (QT Reviewed)

Instrument :
BNA_E
ClientSampled :
C0ZZ1

Manual Integrations
APPROVED

Sohil
8/18/2017 7:08:33 PM

Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
Data File : BE093864.D
Acq On : 17 Aug 2017 14:24
Operator : SJ/JU
Sample : I4693-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Aug 17 19:41:23 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 02:52:40 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	1582	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	8285	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	5026	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	10696m	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	10262	0.40	ng/ul	0.00
20) Perylene-d12	23.92	264	7720m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.29	152	4537	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	12206	0.36	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed