

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampled :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:06:20 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

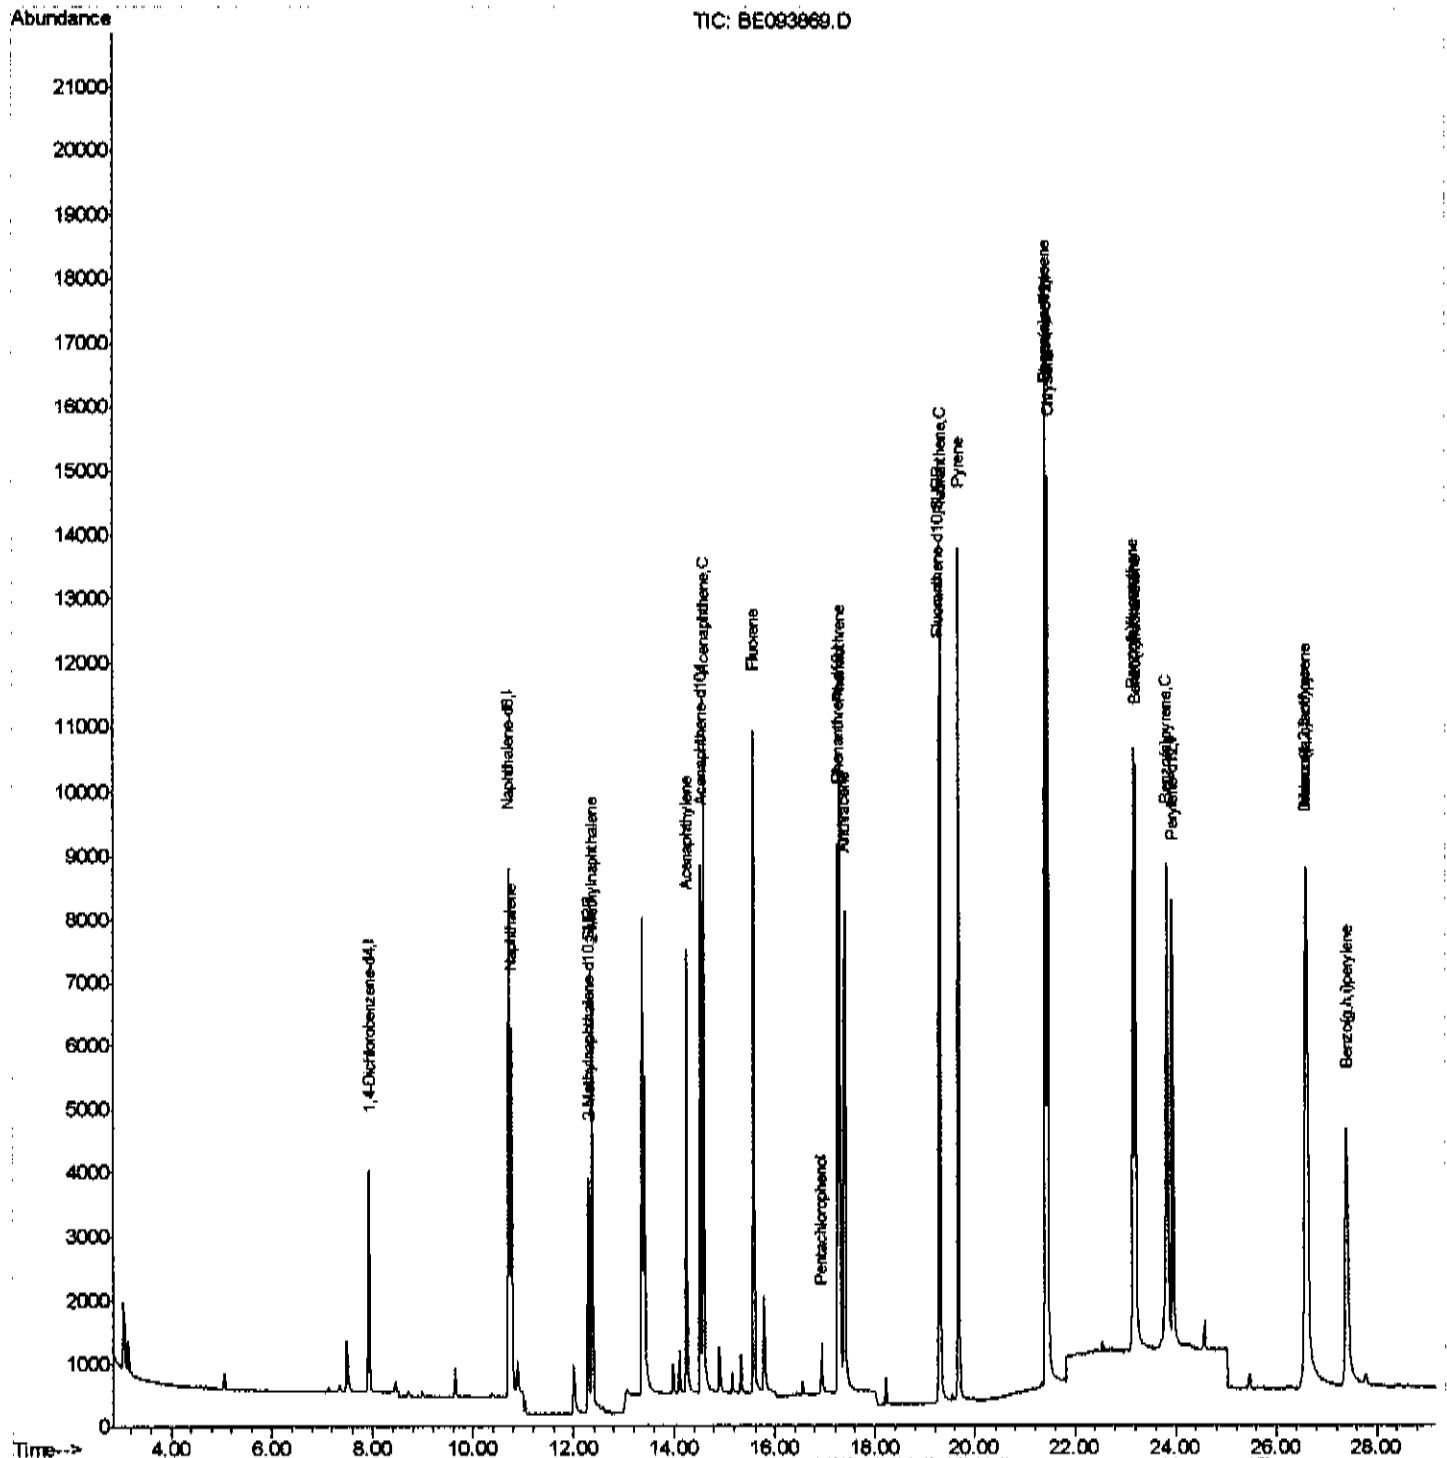

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:02:03 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

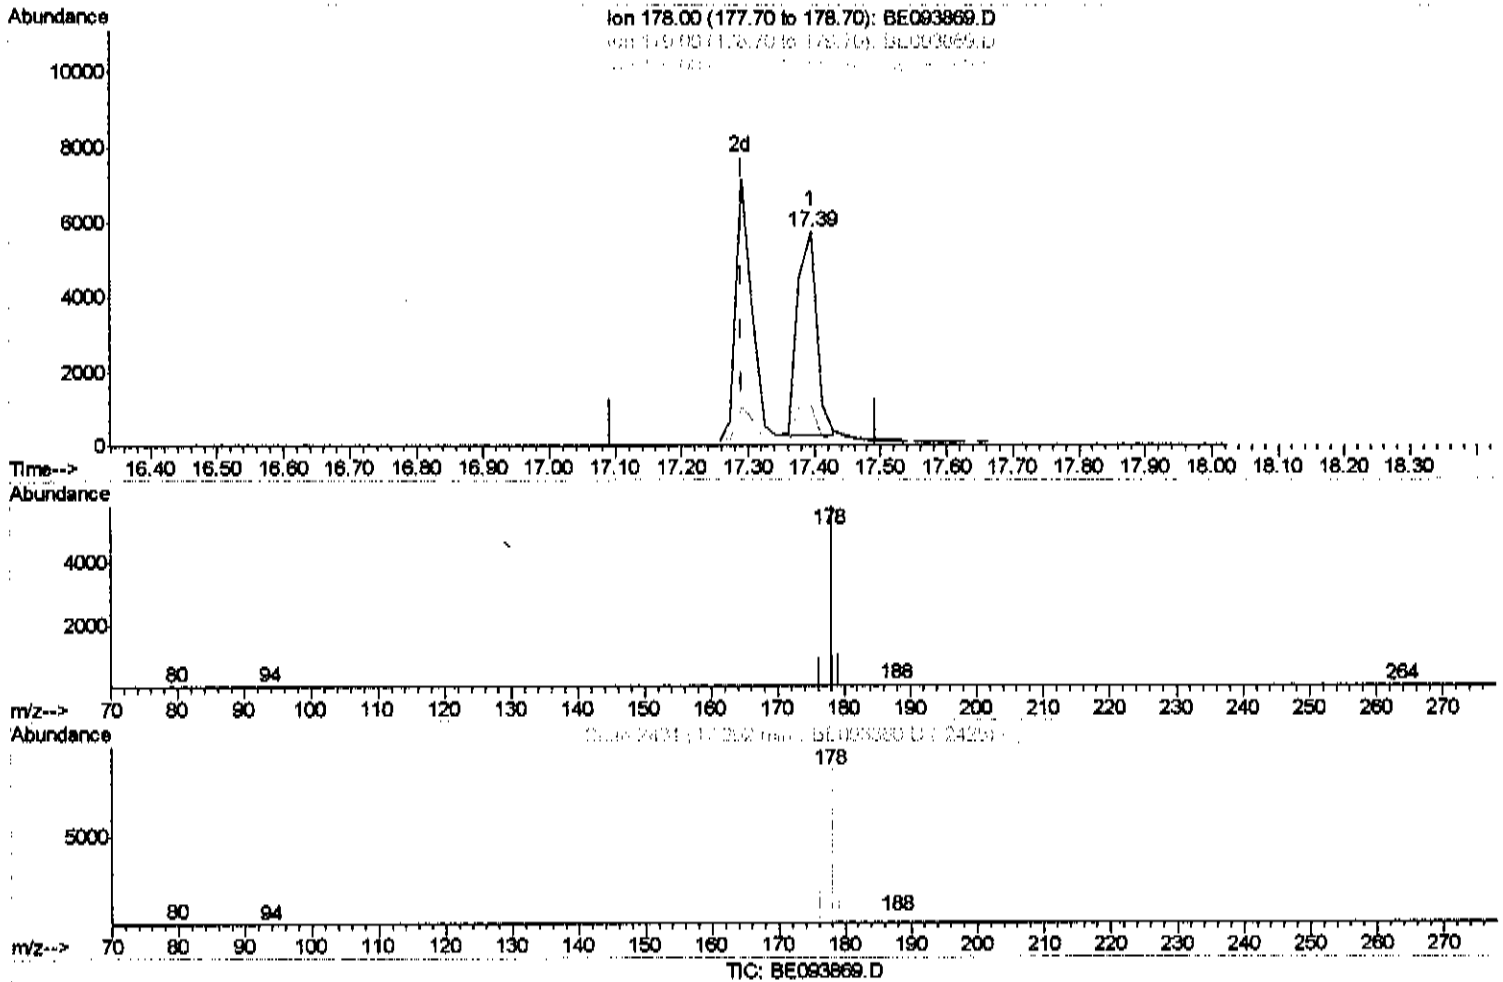

(12) Phenanthrene

17.394min (+0.102) 0.34ng/ul

response 11202

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	18.54
176.00	17.00	16.45
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleID :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:02:03 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

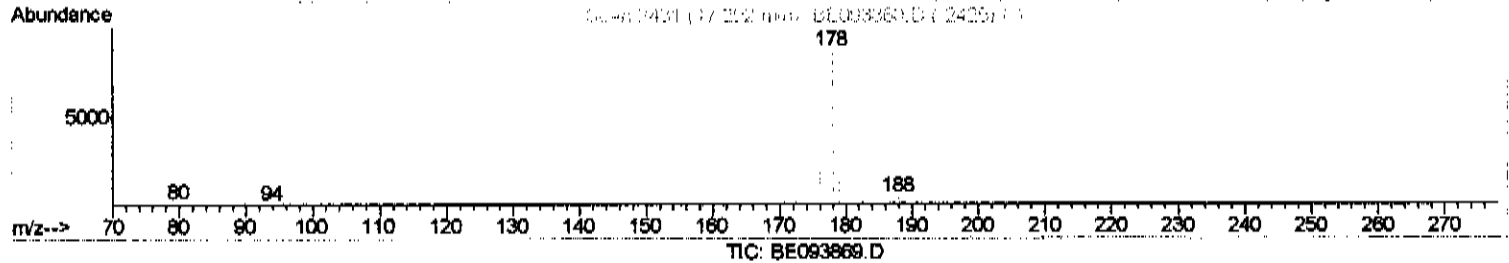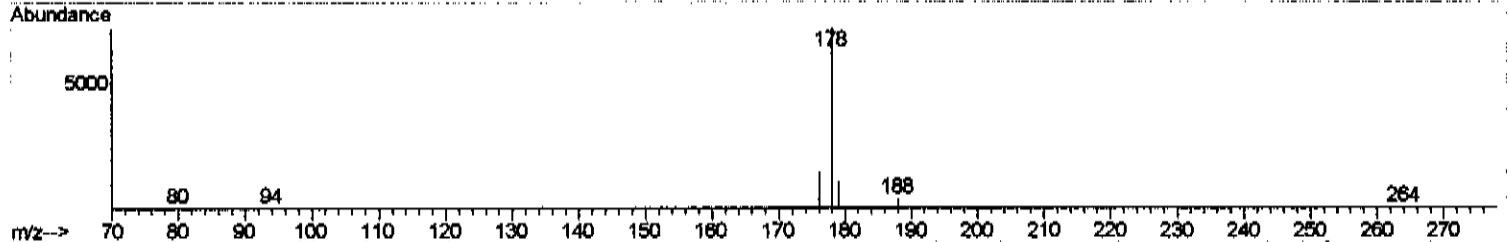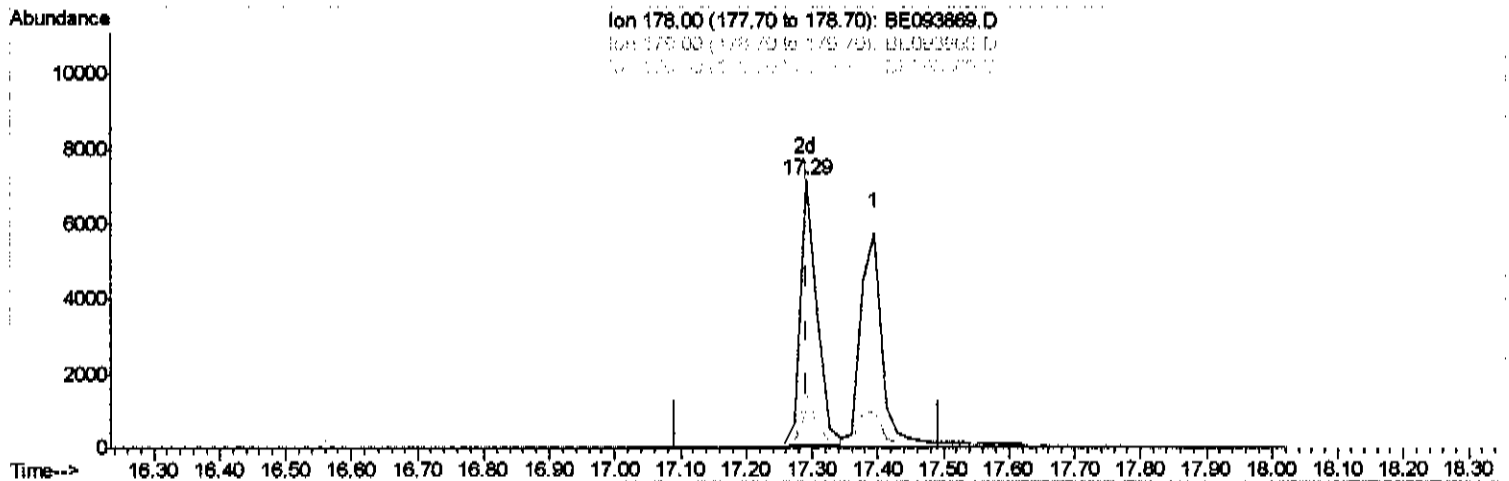

(12) Phenanthrene

17.290min (-0.002) 0.38ng/ul m *SJ/JU 8/18/17*

response 12362

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	14.72#
178.00	17.00	20.64#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:02:03 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

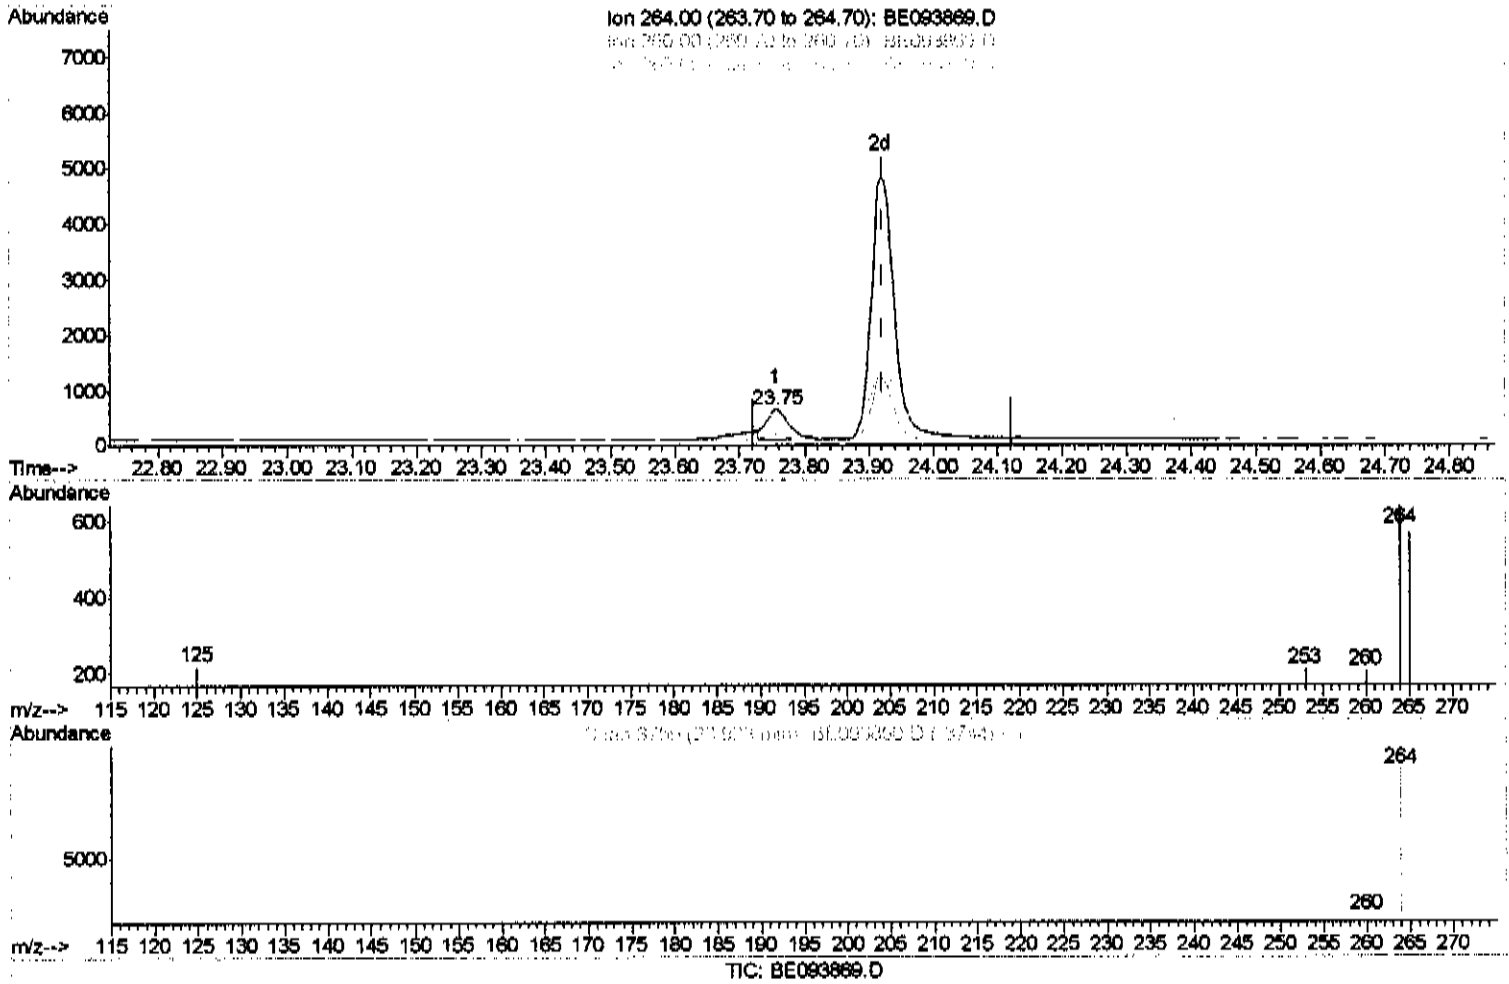

(20) Perylene-d12 (I)

23.755min (-0.168) 0.40ng/ul

response 1235

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	32.14
265.00	103.50	88.46
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:02:03 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

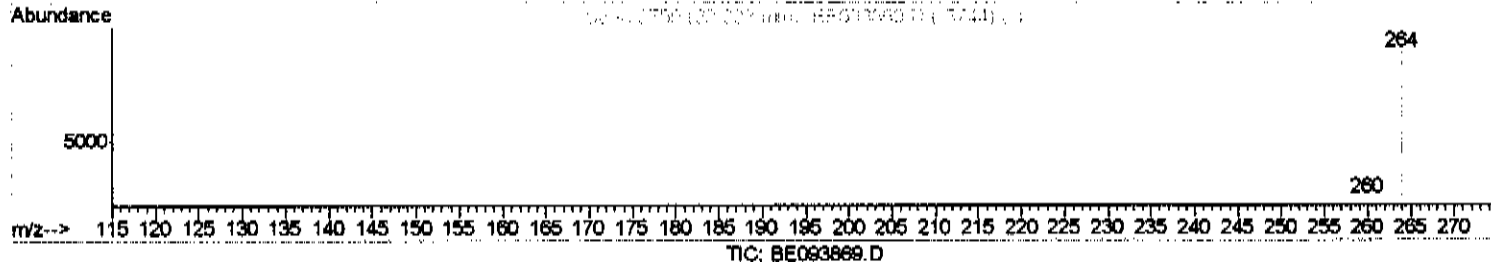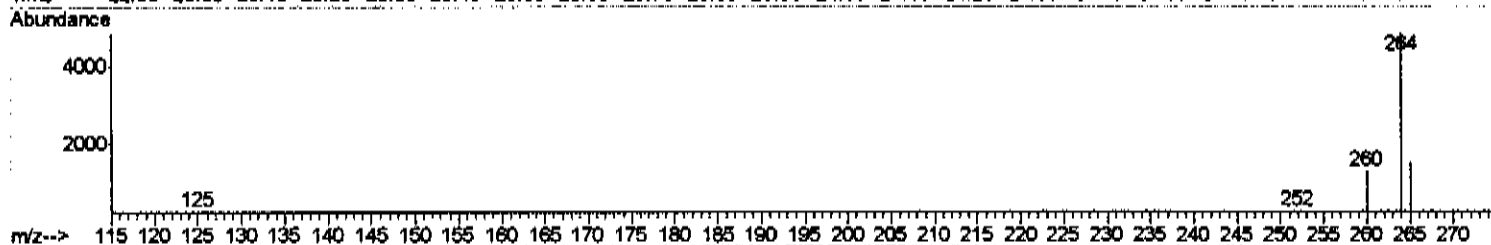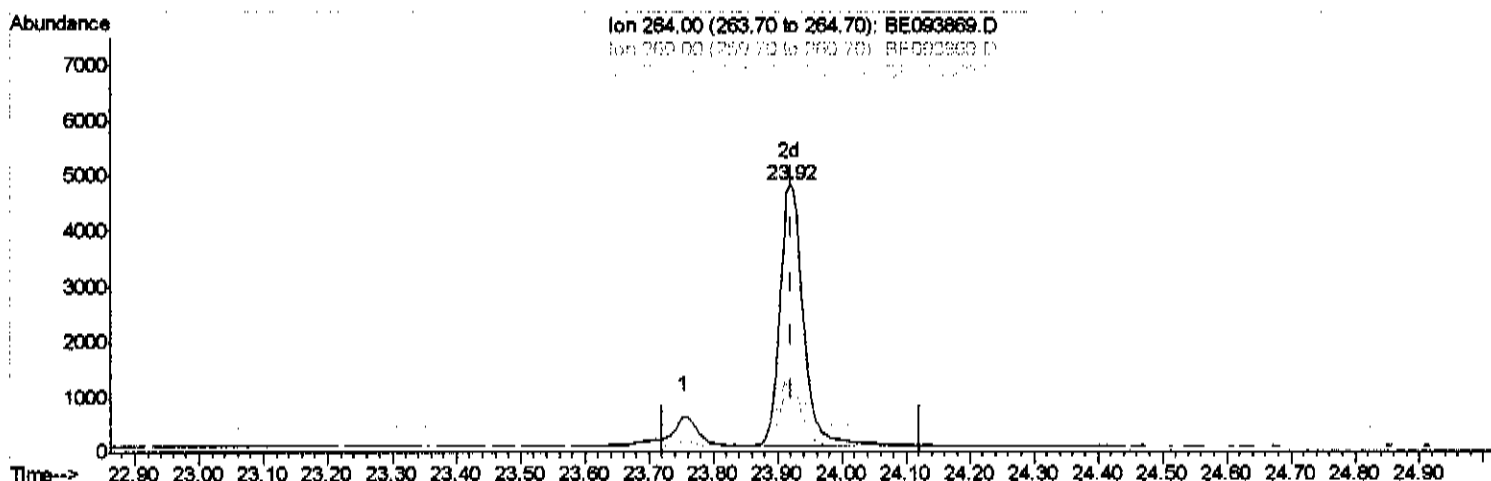

(20) Perylene-d12 (I)

23.919min (-0.004) 0.40ng/ul m *SJ*
 response 11892

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.12
266.00	103.50	31.03%
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:03:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

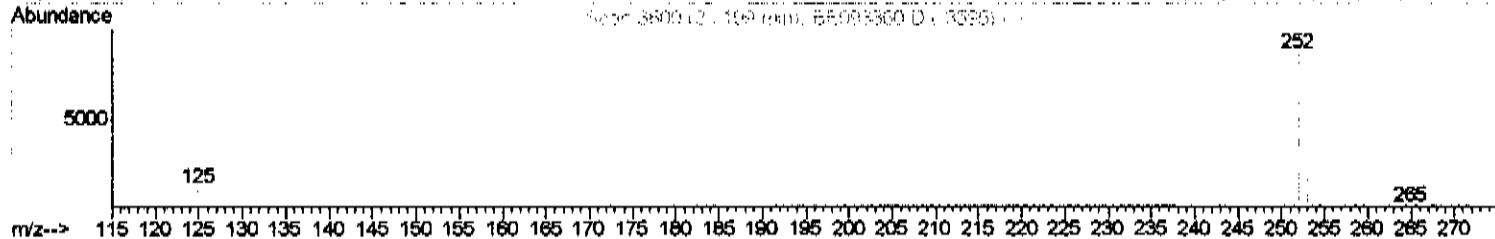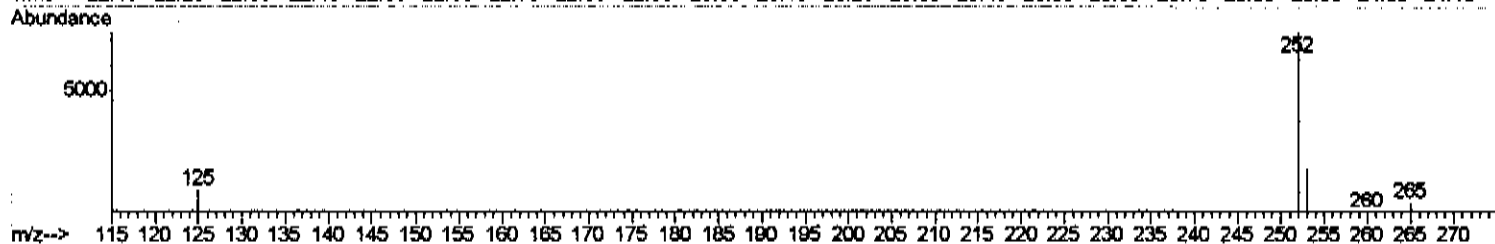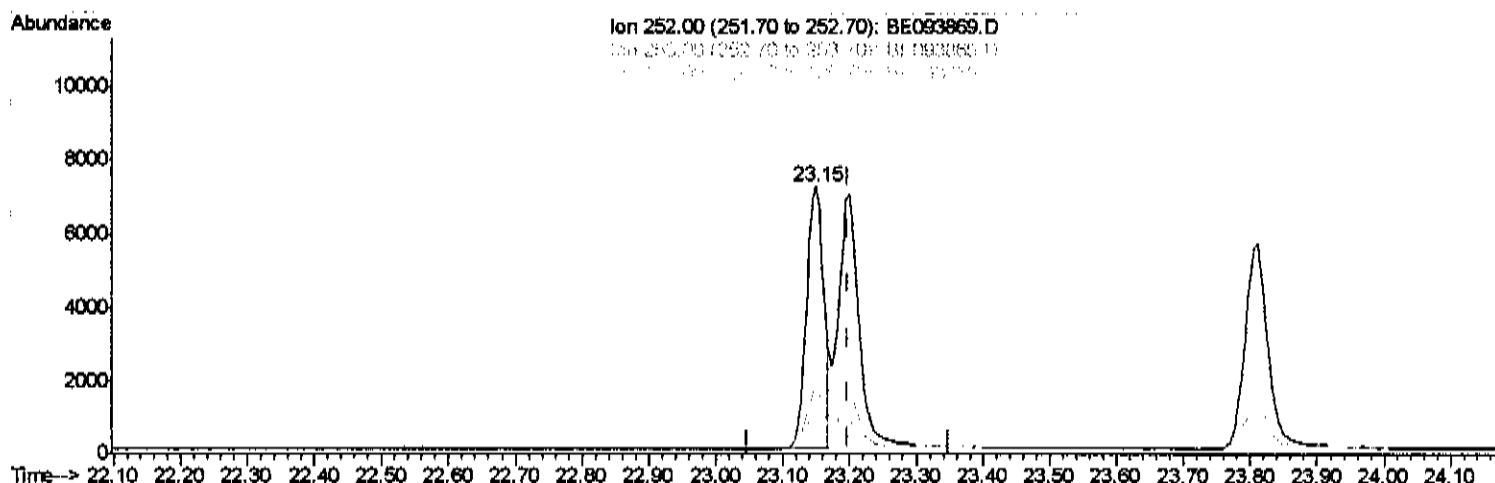

TIC: BE093869.D

(22) Benzo(k)fluoranthene

23.149min (-0.050) 0.38ng/ul

response 12879

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	23.97#
125.00	17.10	13.20#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleID :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:03:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

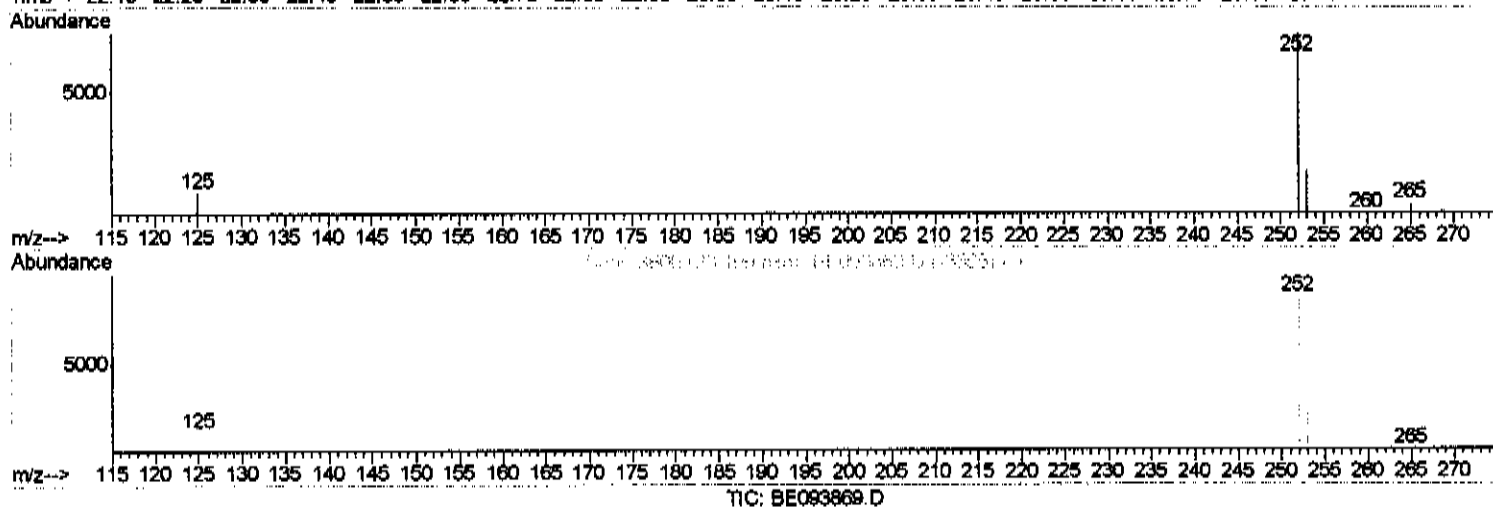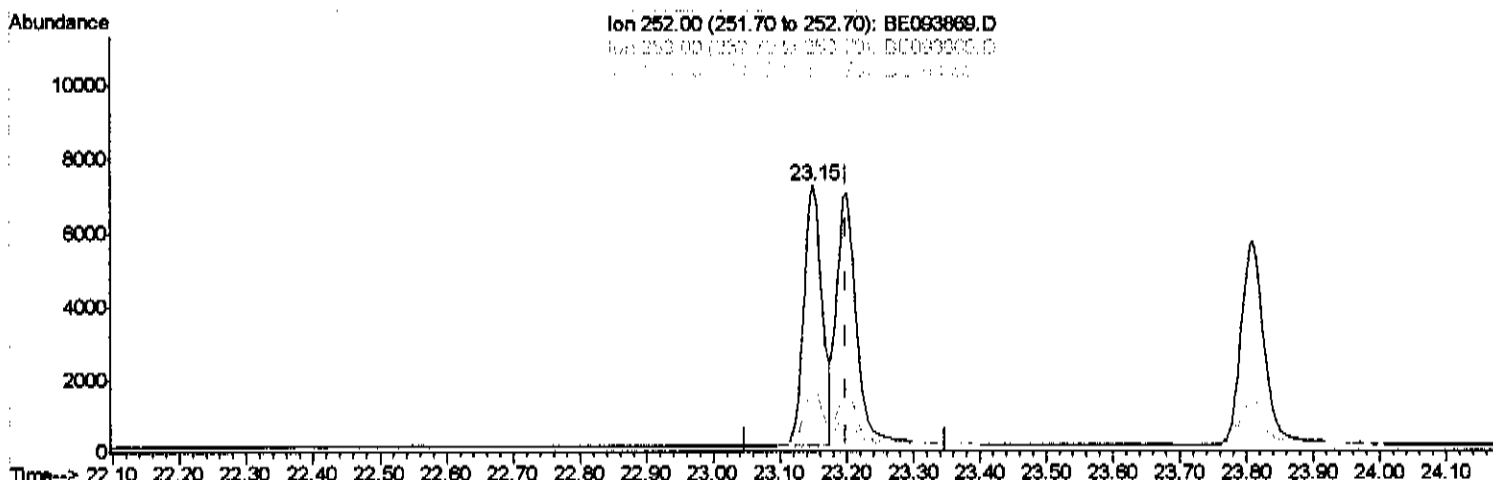

(22) Benzo(k)fluoranthene

23.149min (-0.050) 0.37ng/ul m

response 13585

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	23.97%
125.00	17.10	13.20%
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDC00.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SST0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:03:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

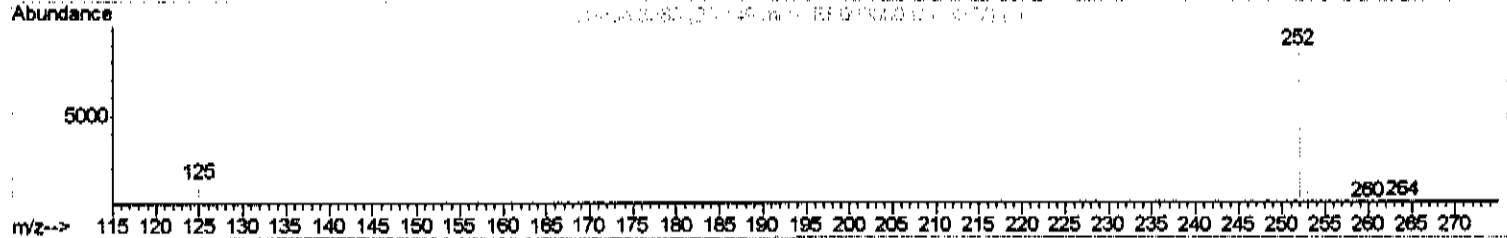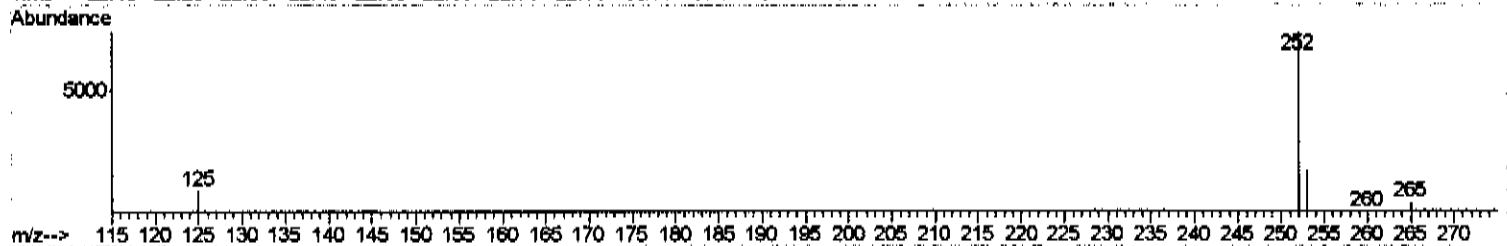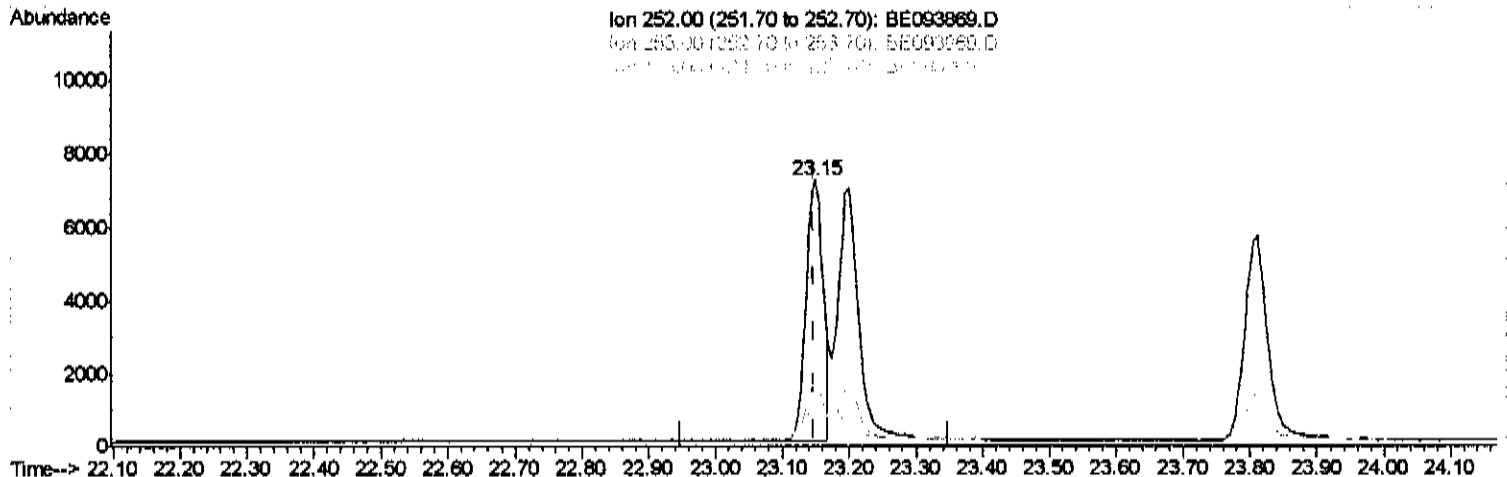

TIC: BE093869.D

(21) Benzo(b)fluoranthene
 23.149min (+0.001) 0.35ng/ul
 response 12879

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	23.97
125.00	17.50	13.20
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleID :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:03:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

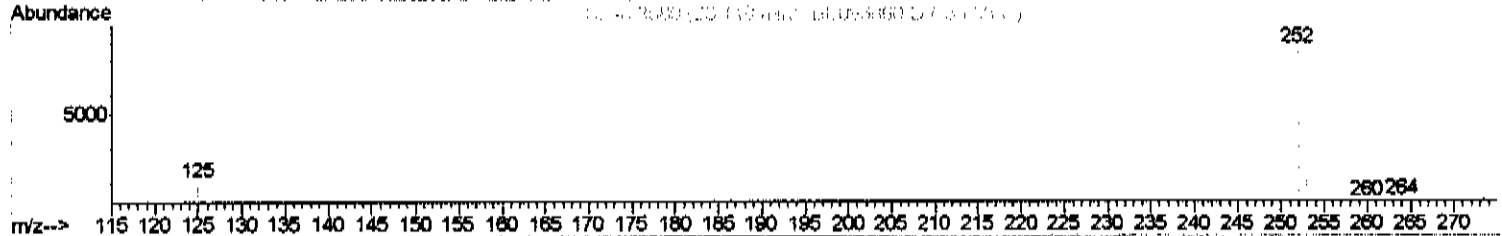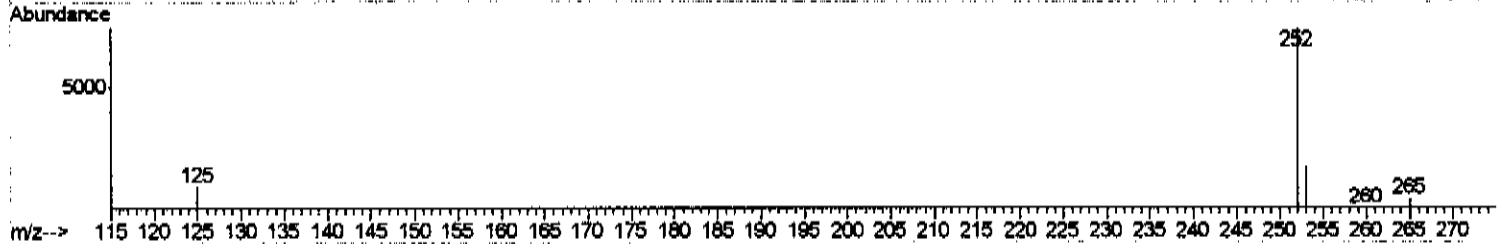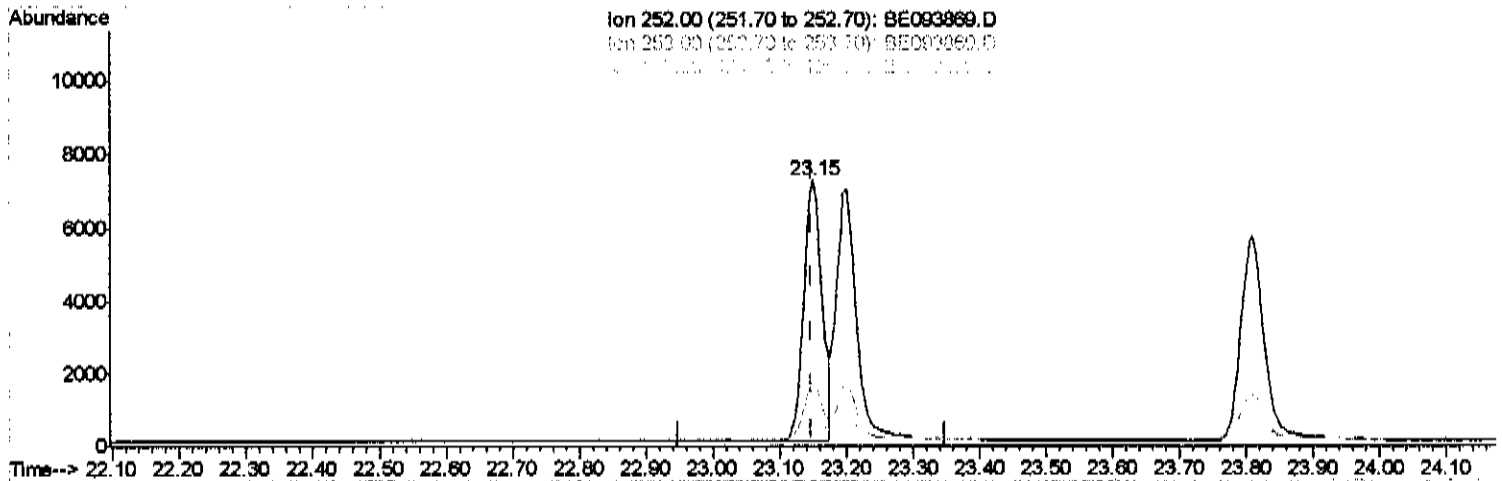

TIC: BE093869.D

(21) Benzo(b)fluoranthene

23.149min (+0.001) 0.37ng/ul m

response 13541

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	23.97
125.00	17.50	13.20
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:03:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

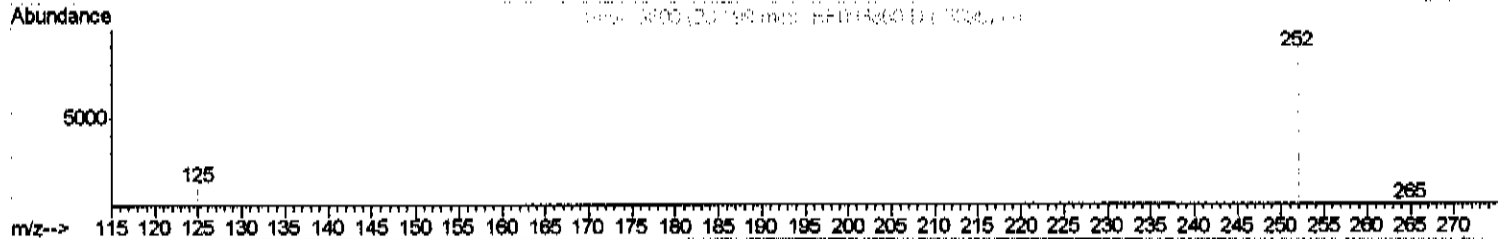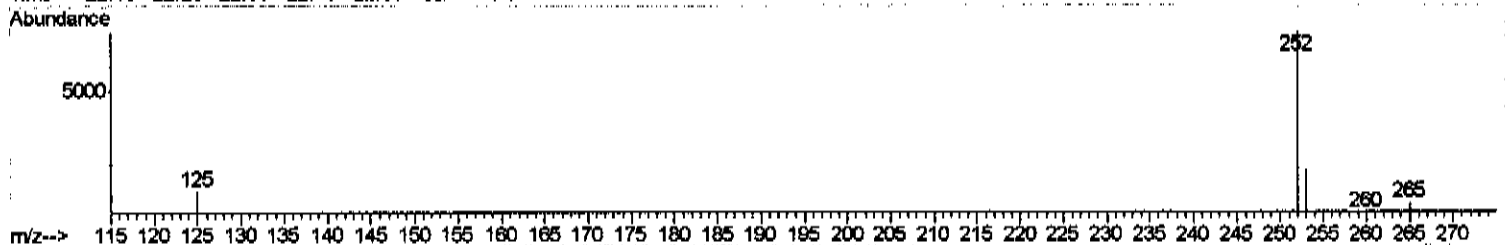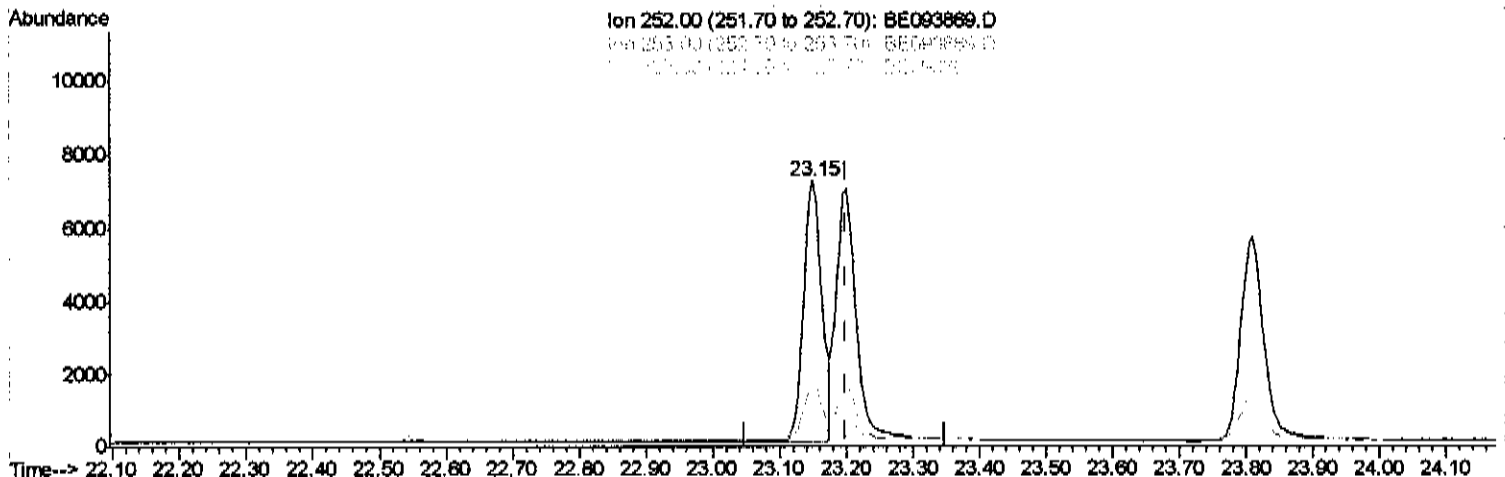

TIC: BE093869.D

(22) Benzo(k)fluoranthene

23.149min (-0.050) 0.37ng/ul m

response 13585

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	23.97%
125.00	17.10	13.20%
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:03:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

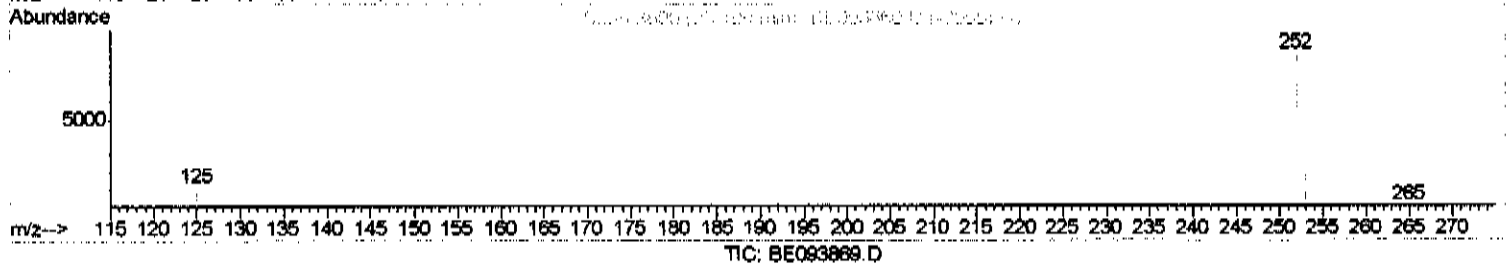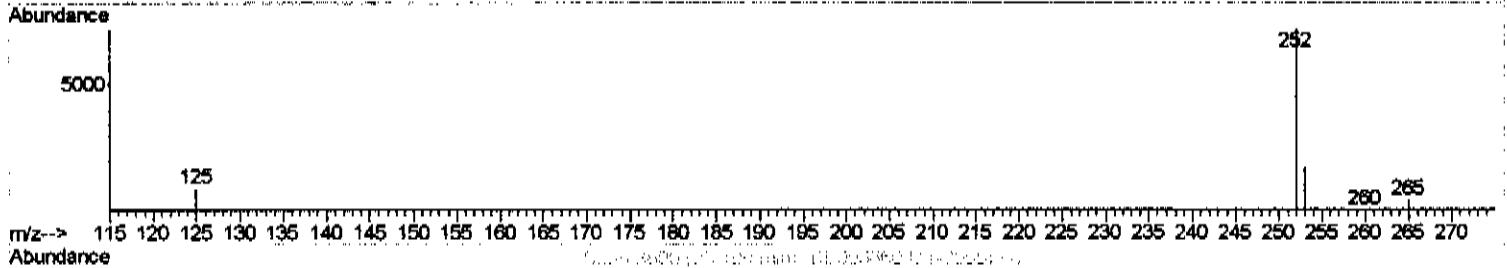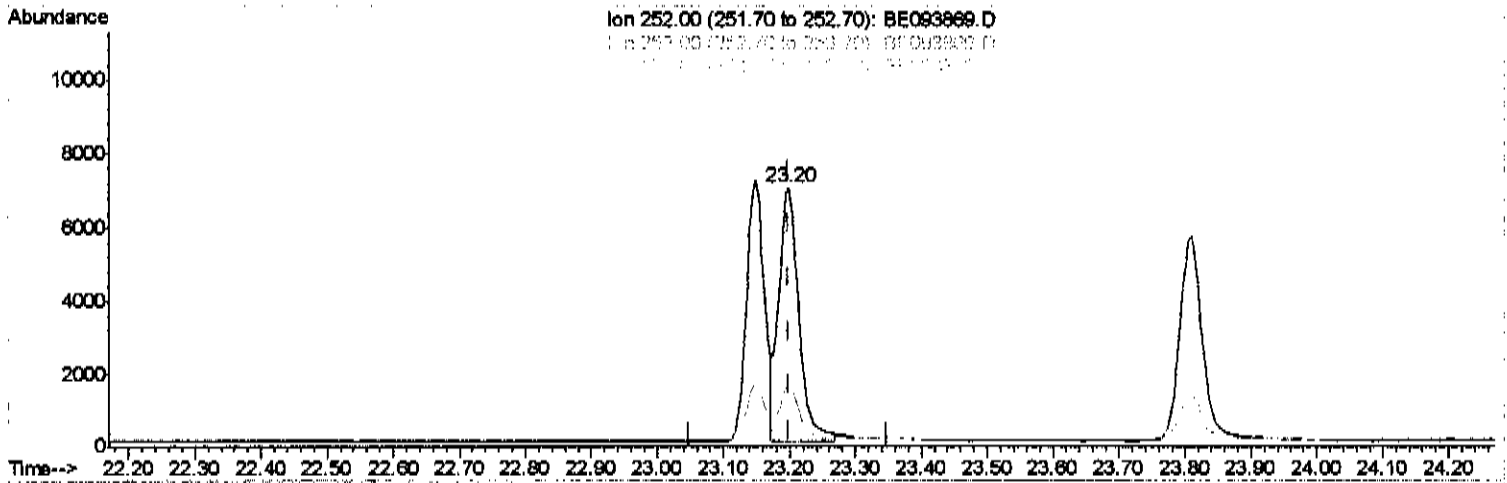

(22) Benzo(k)fluoranthene

23.199min (+0.001) 0.40ng/ul m

response 14581

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	24.55
125.00	17.10	13.11#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleID :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:03:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

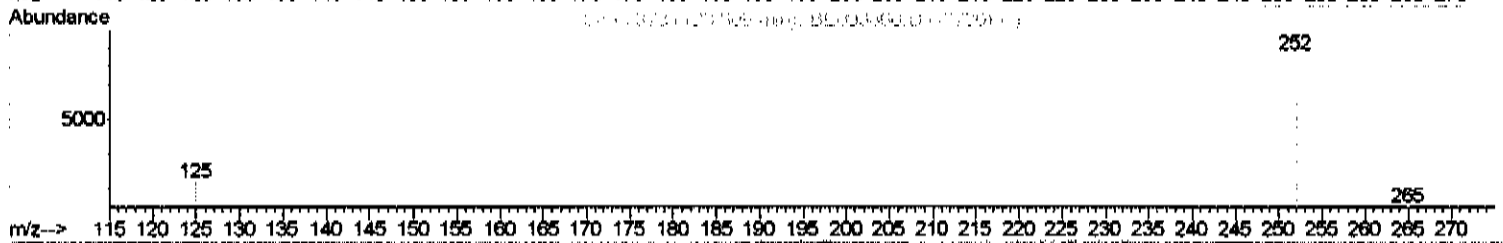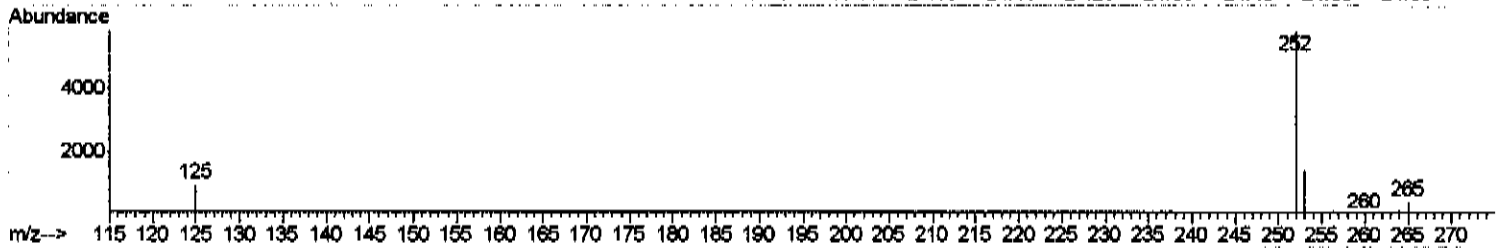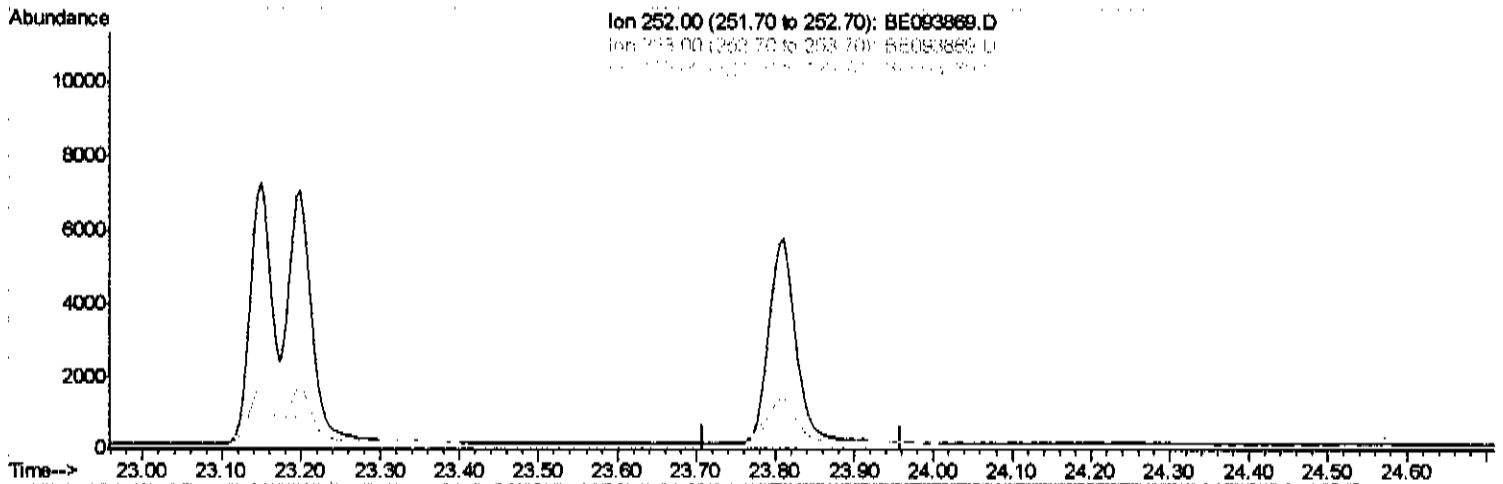

TIC: BE093869.D

(23) Benzo(a)pyrene (C)

23.809min (-23.809) 0.00ng/ul

response 0

Ion	Exp%	Act%
252.00	100	0.00
253.00	35.60	0.00%
125.00	22.60	0.00%
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:03:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

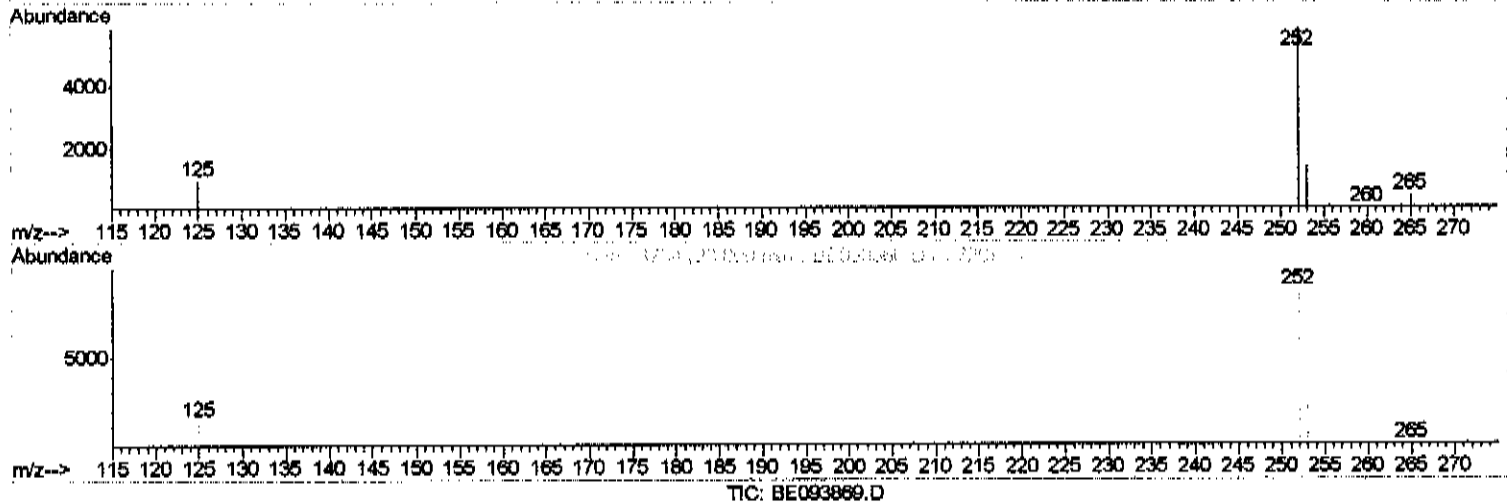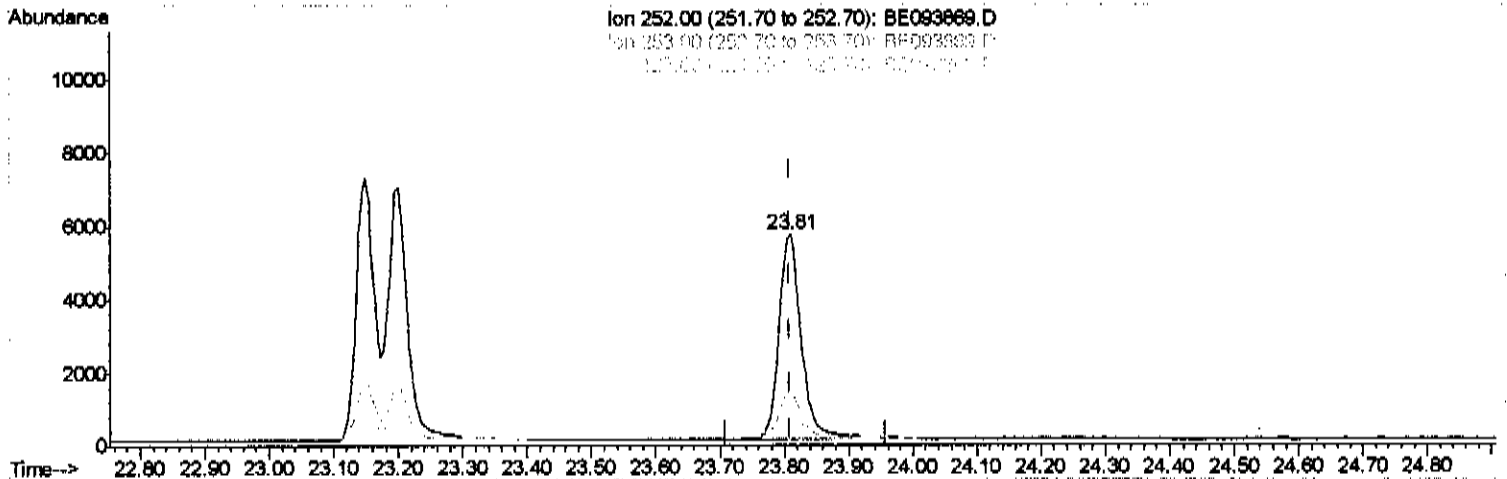

(23) Benzo(a)pyrene (C)

23.810min (+0.001) 0.39ng/ul m

response 13538

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	24.63#
125.00	22.60	16.78#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampled :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:03:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

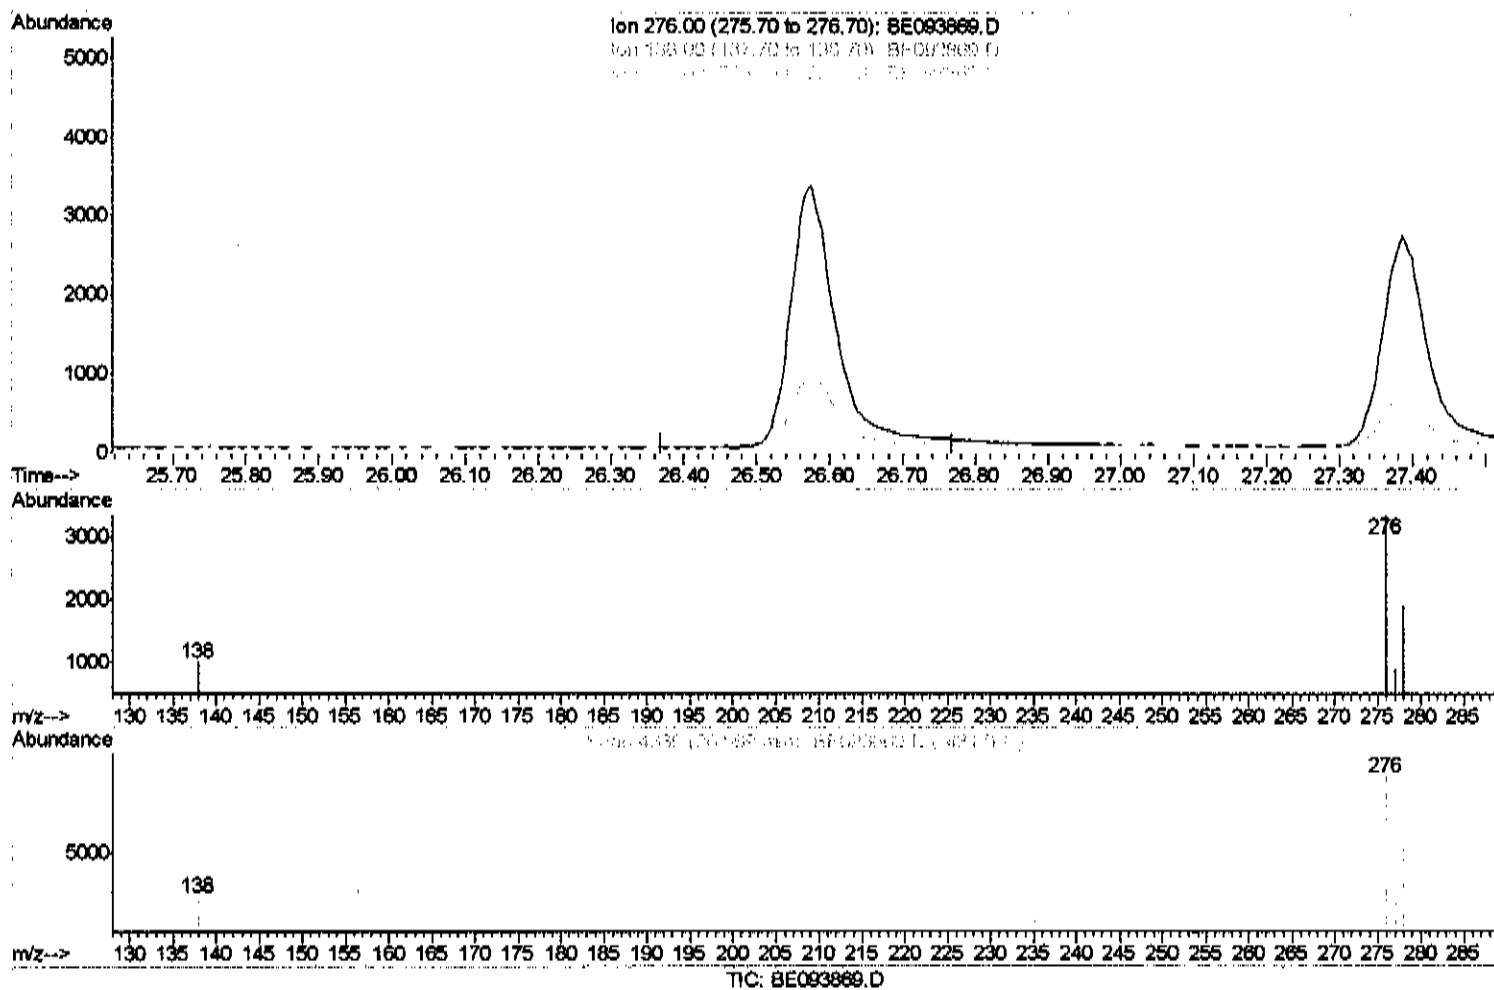

(24) Indeno(1,2,3-cd)pyrene

26.569min (-26.569) 0.00ng/ul

response 0

Ion	Exp%	Act%
276.00	100	0.00
138.00	35.00	0.00#
227.00	10.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDC00.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampled :
 SSTDO.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:03:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

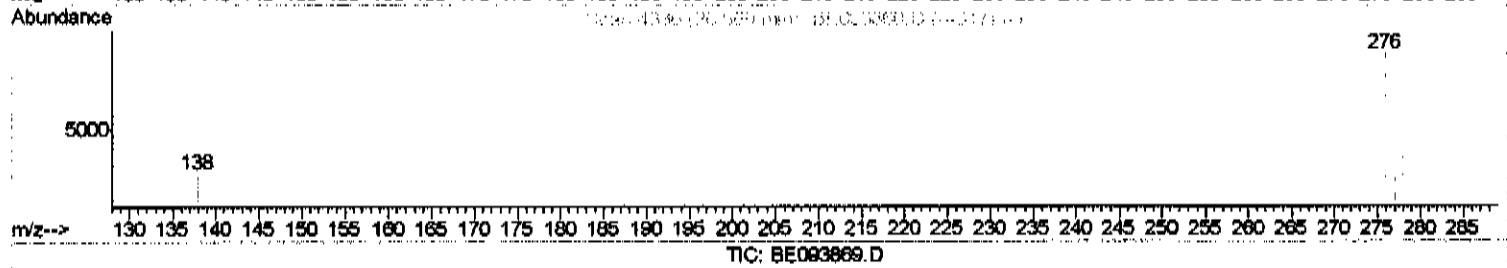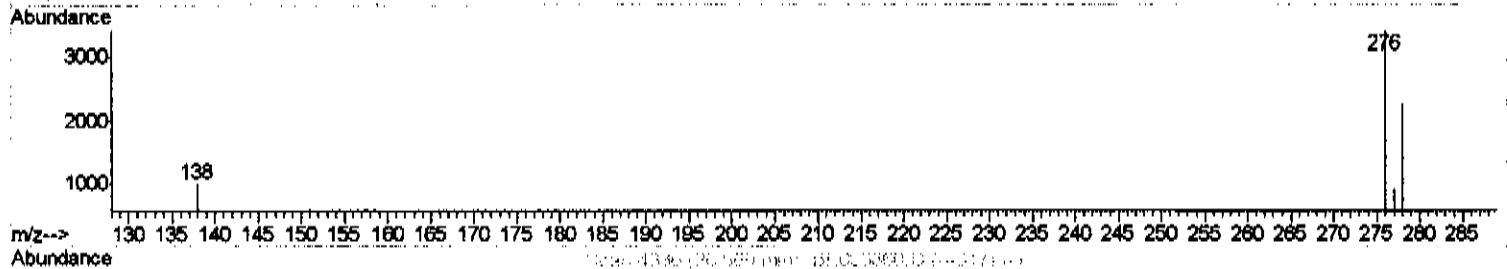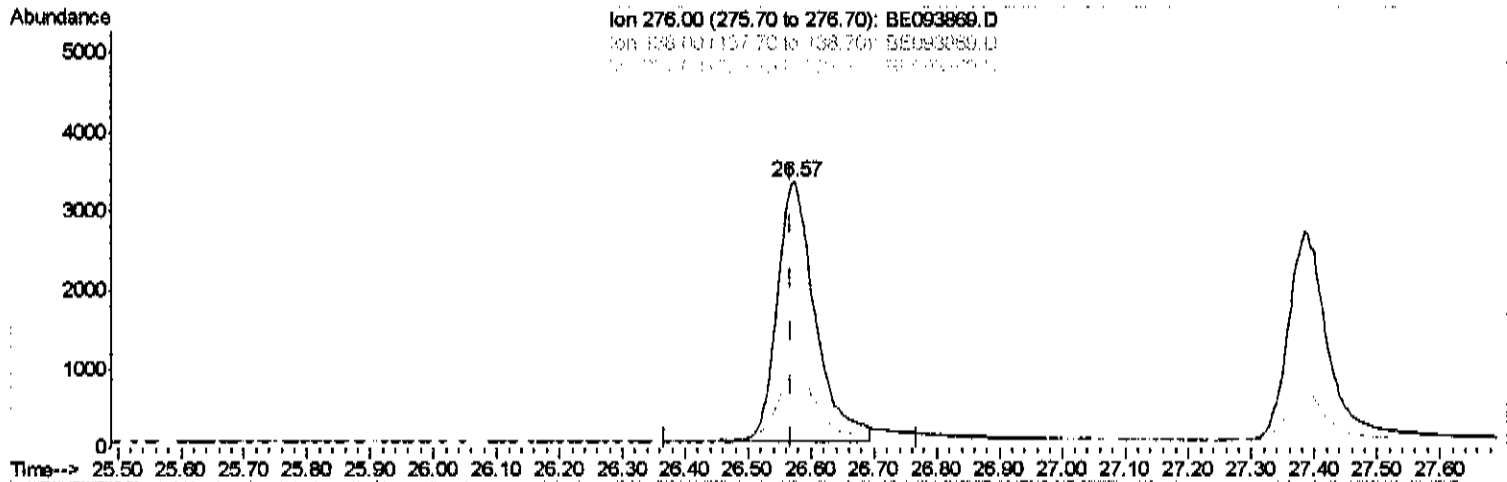

(24) Indeno(1,2,3-cd)pyrene

26.574min (+0.005) 0.36ng/ul m *[Signature]*

response 13866

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	0.00%
227.00	10.00	0.00%
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleID :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:03:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

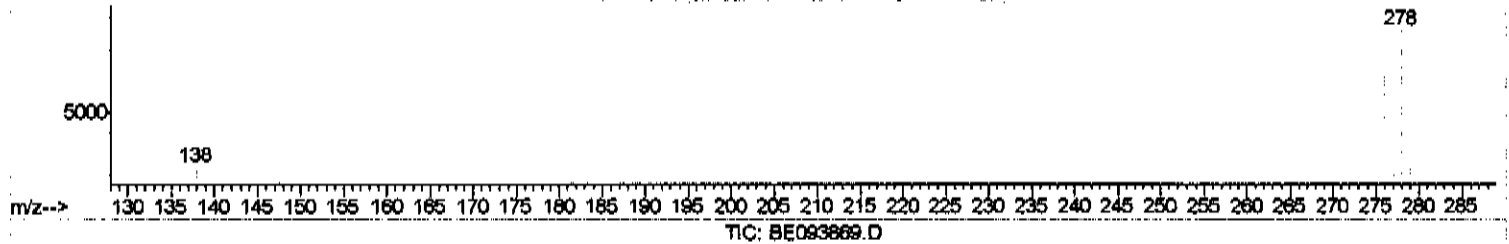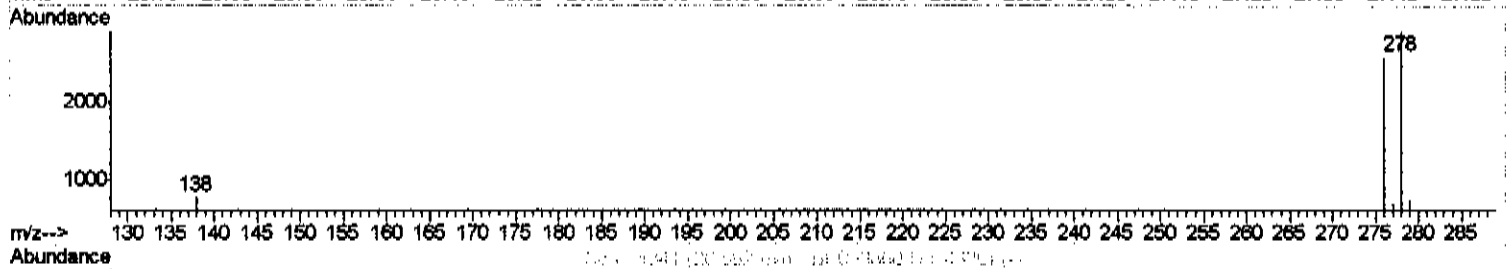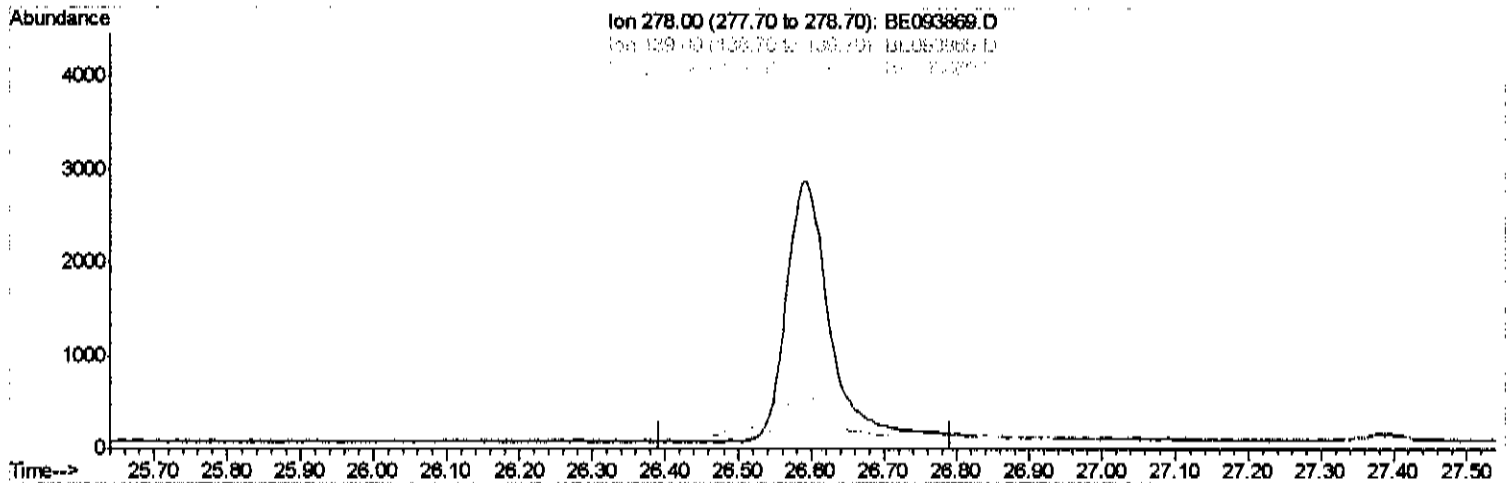

(25) Dibenzo(a,h)anthracene

26.592min (-26.592) 0.00ng/ul

response 0

Ion	Exp%	Act%
278.00	100	0.00
139.00	21.70	0.00#
279.00	32.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampled :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:03:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

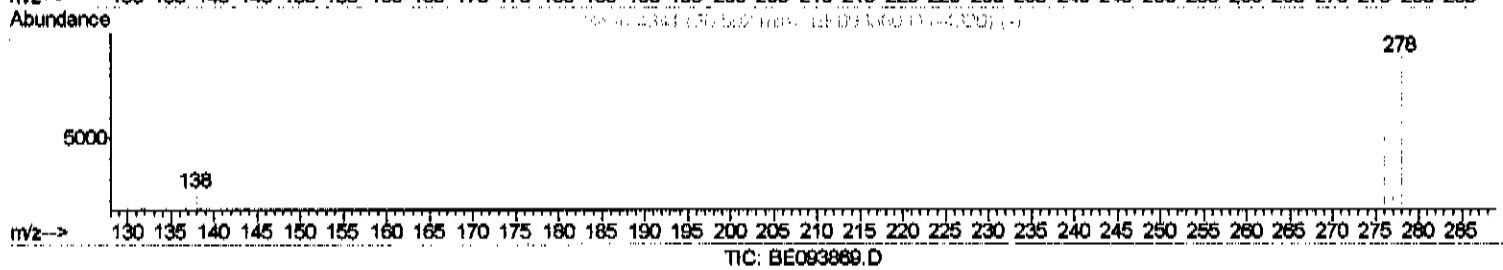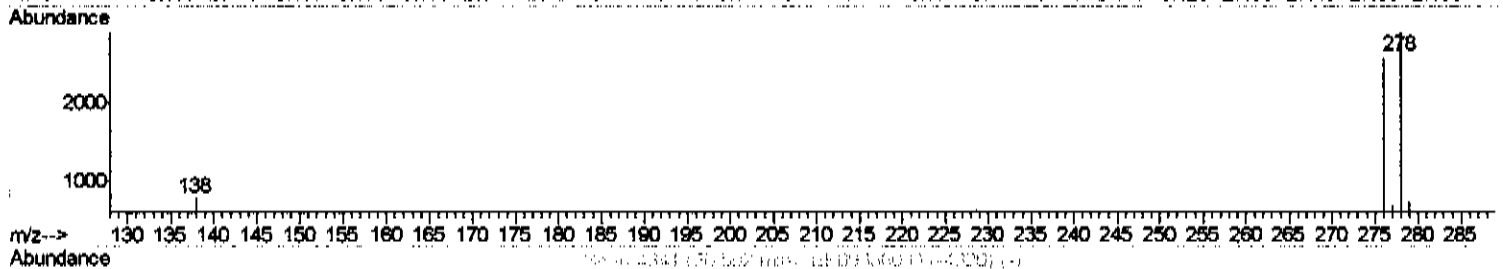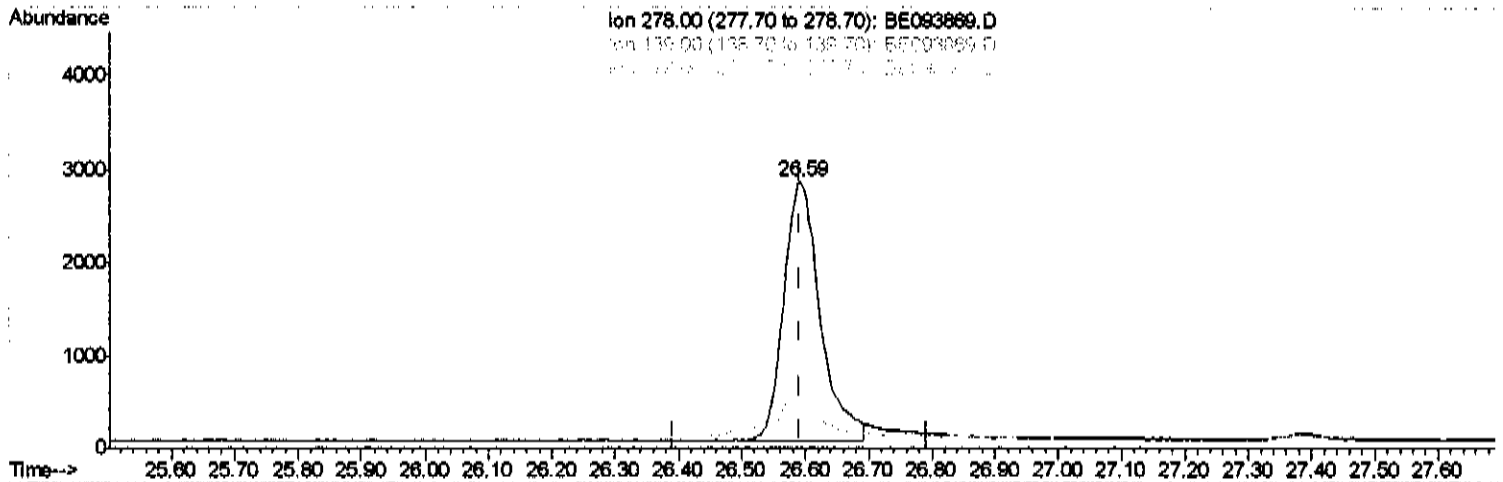

(25) Dibenzo(a,h)anthracene

26.592min (+0.000) 0.35ng/ul m

response 11192

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	21.41
279.00	32.40	25.93
0.00	0.00	0.00

Handwritten: 8/18/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDC00.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampled :
 SSTDO.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:03:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

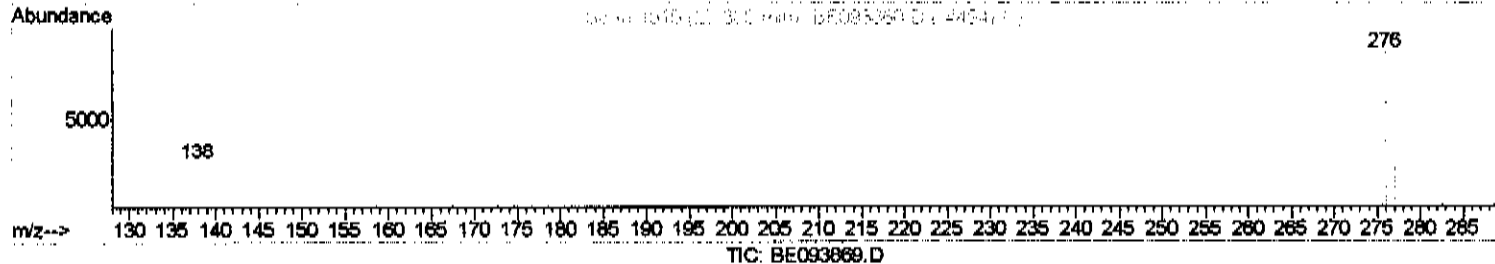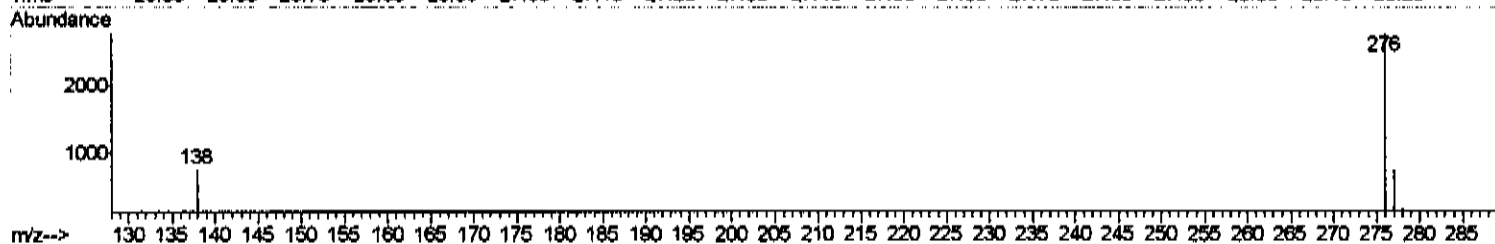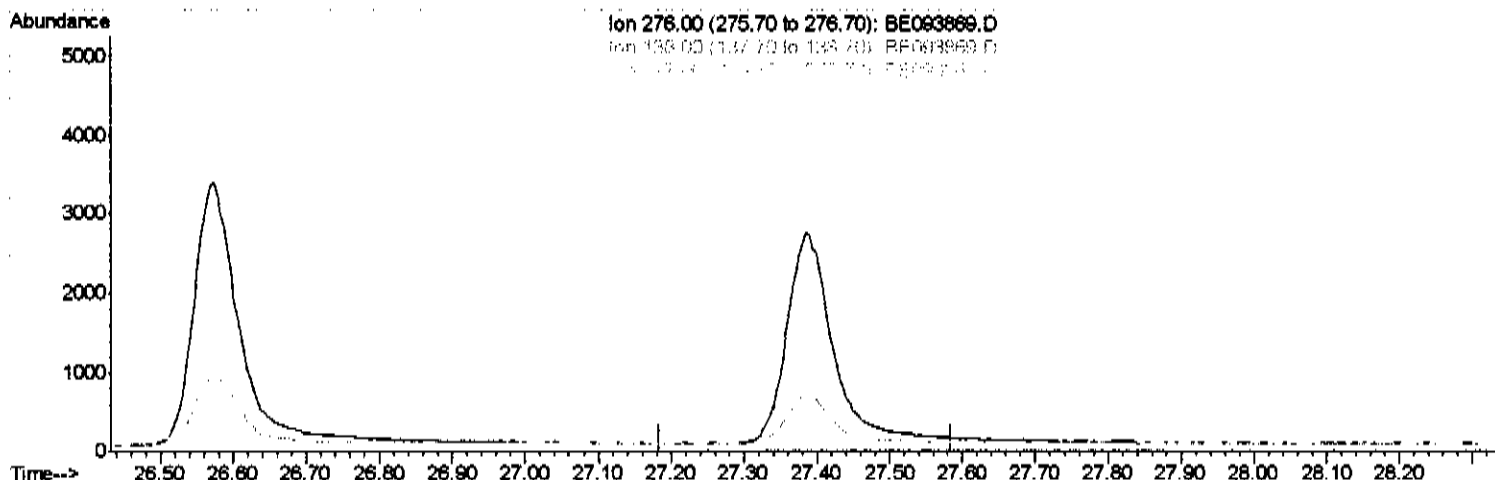

(26) Benzo(g,h,i)perylene
 27.385min (-27.385) 0.00ng/ul
 response 0

Ion	Exp%	Act%
276.00	100	0.00
138.00	27.30	0.00#
277.00	25.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
 Data File : BE093869.D
 Acq On : 17 Aug 2017 17:29
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTD0.413

Manual Integrations
 APPROVED

Sohil
 8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:03:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

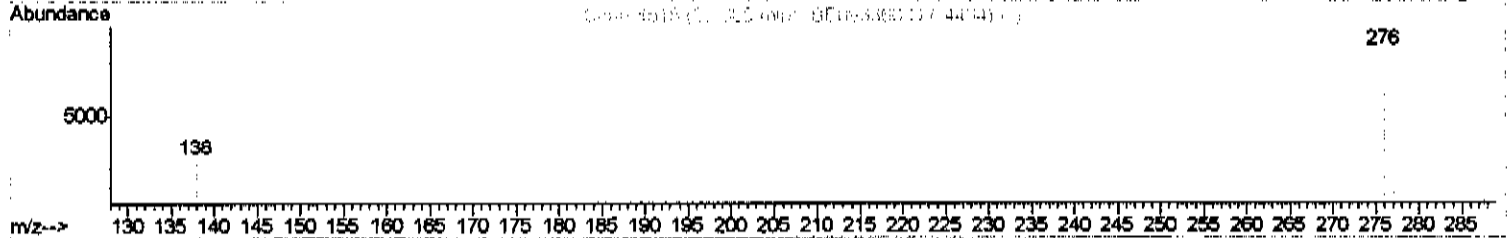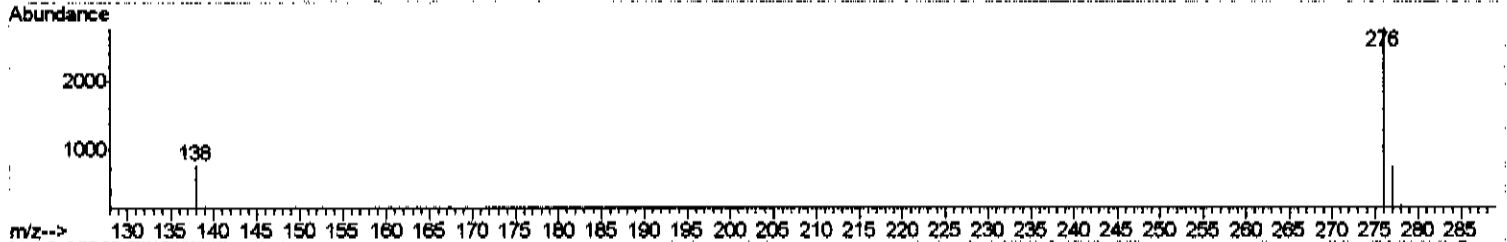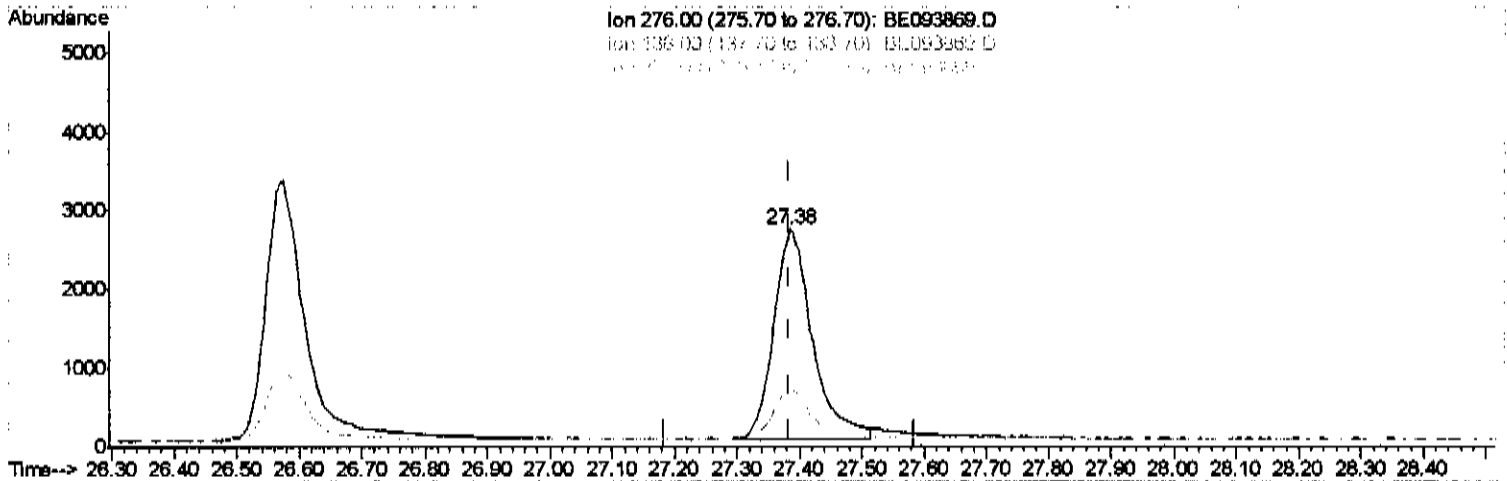

TIC: BE093869.D

(26) Benzo(g,h,i)perylene

27.385min (+0.000) 0.35ng/ul m

response 11555

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	27.59
277.00	25.60	26.87
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Instrument :
BNA_E
LabSampleId :
SSTD0.413

Data Path : Z:\HPCHEM1\BNA_E\Data\BE081717\
Data File : BE093869.D
Acq On : 17 Aug 2017 17:29
Operator : SJ/JU
Sample : SSTDCCC0.4EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Manual Integrations
APPROVED

Sohil
8/18/2017 7:08:42 PM

Quant Time: Aug 17 20:06:20 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 19:06:13 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	1903	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	9835	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	5411	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	12069	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	13280	0.40	ng/ul	0.00
20) Perylene-d12	23.92	264	11892m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.29	152	6083	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	13870	0.36	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.75	128	9437	0.394	ng/ul#	92
5) 2-Methylnaphthalene	12.36	142	6406	0.367	ng/ul	98
7) Acenaphthylene	14.24	152	9502	0.420	ng/ul	97
8) Acenaphthene	14.59	153	6866	0.386	ng/ul	99
9) Fluorene	15.57	166	7724	0.343	ng/ul#	93
11) Pentachlorophenol	16.93	266	786	0.395	ng/ul	96
12) Phenanthrene	17.29	178	12362m	0.376	ng/ul	95
13) Anthracene	17.39	178	12348	0.386	ng/ul	93
15) Fluoranthene	19.31	202	14700	0.358	ng/ul	85
17) Pyrene	19.67	202	15485	0.399	ng/ul#	83
18) Benzo(a)anthracene	21.39	228	14771	0.384	ng/ul#	86
19) Chrysene	21.45	228	14652	0.397	ng/ul	97
21) Benzo(b)fluoranthene	23.15	252	13541m	0.368	ng/ul	94
22) Benzo(k)fluoranthene	23.20	252	14581m	0.402	ng/ul	
23) Benzo(a)pyrene	23.81	252	13538m	0.387	ng/ul	
24) Indeno(1,2,3-cd)pyrene	26.57	276	13866m	0.359	ng/ul	
25) Dibenzo(a,h)anthracene	26.59	278	11192m	0.347	ng/ul	
26) Benzo(g,h,i)perylene	27.38	276	11555m	0.355	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed