

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
 Data File : BE097305.D
 Acq On : 17 Aug 2018 20:21
 Operator : SJ/JU
 Sample : J4424-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 17 23:34:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 17 23:33:44 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1132	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	5847	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	3237	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	490670	0.40	ng/ul	0.10
16) Chrysene-d12	21.17	240	8	0.40	ng/ul	0.19
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-23.22
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	2318	0.25	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
17) Pyrene	19.30	202	20	0.827	ng/ul#	1
18) Benzo(a)anthracene	21.12	228	45	2.269	ng/ul#	1
19) Chrysene	21.20	228	16	0.676	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
Data File : BE097305.D
Acq On : 17 Aug 2018 20:21
Operator : SJ/JU
Sample : J4424-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 17 23:34:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 17 23:33:44 2018
Response via : Initial Calibration




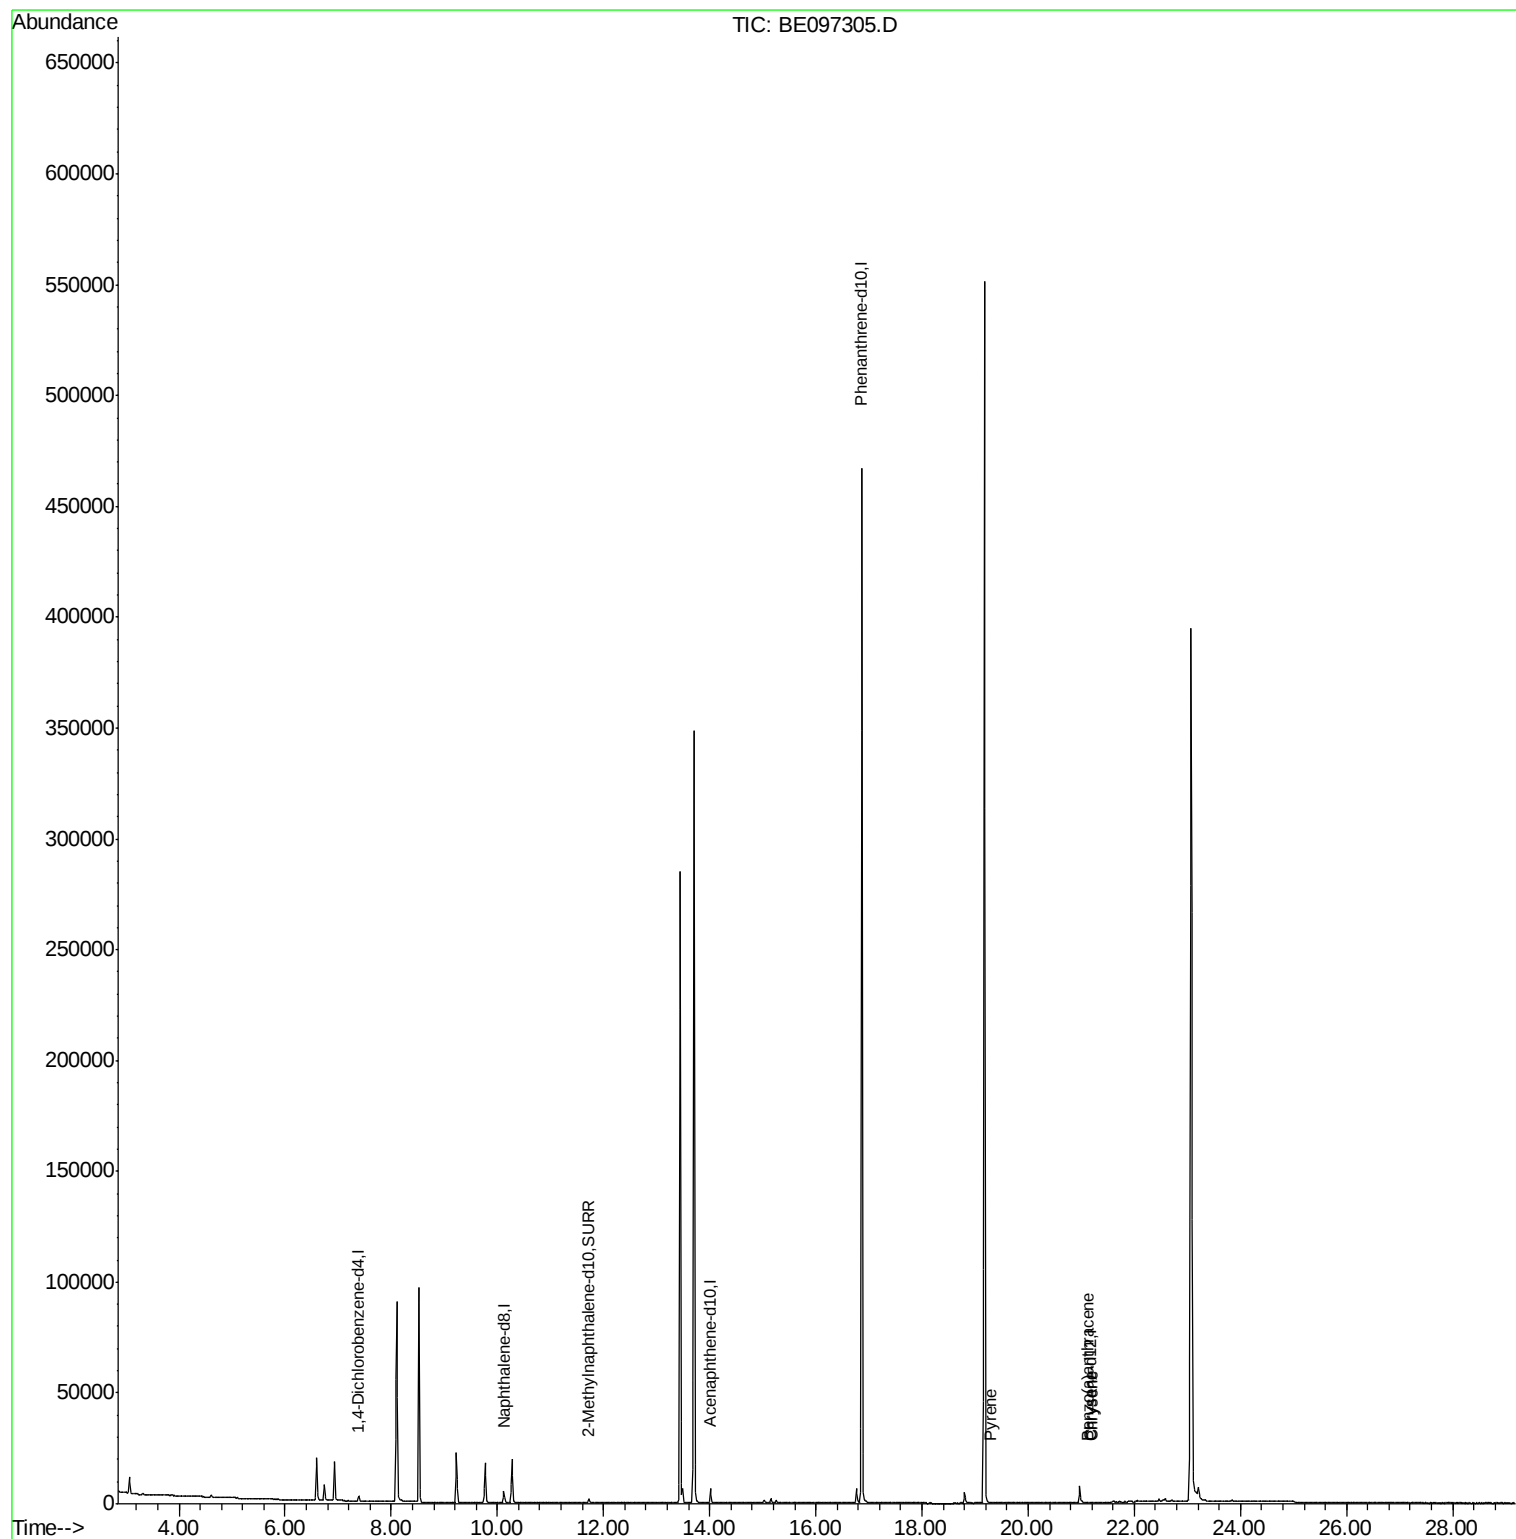


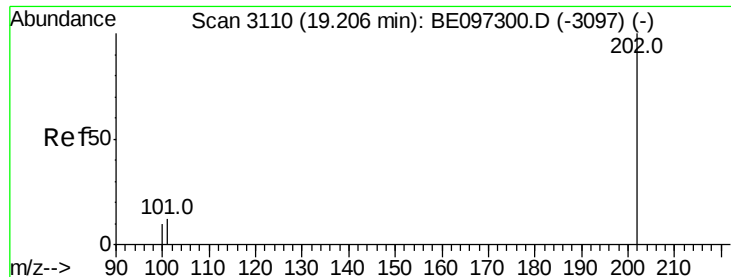

#17
Pvrene
Concen: 0.827 ng/ul
RT: 19.30 min Scan# 3136
Delta R.T. 0.09 min
Lab File: BE097305.D
Acq: 17 Aug 2018 20:21




Instrument :
BNA_E
ClientSampleId :




Tot Ion:202 Resp: 20
Ion Ratio Lower Upper
202 100
101 87.7 18.2 27.4#
100 81.5 15.6 23.4#

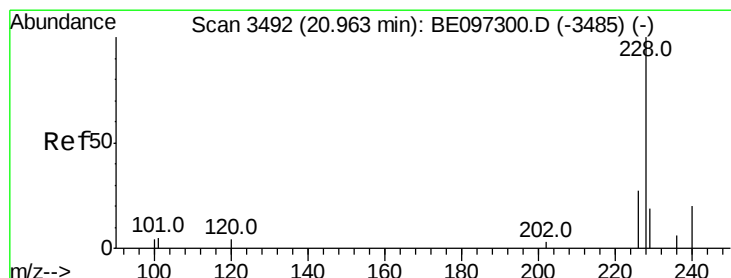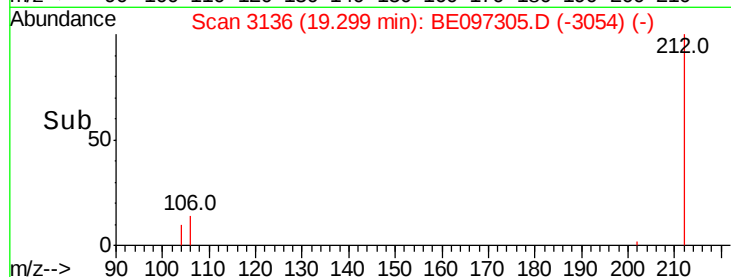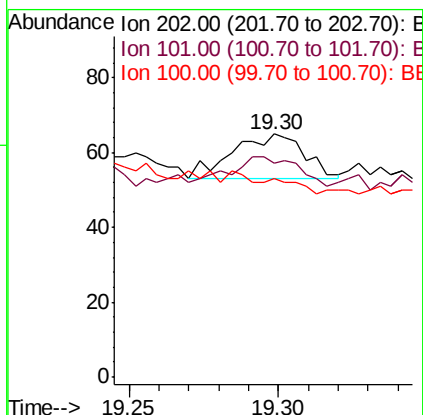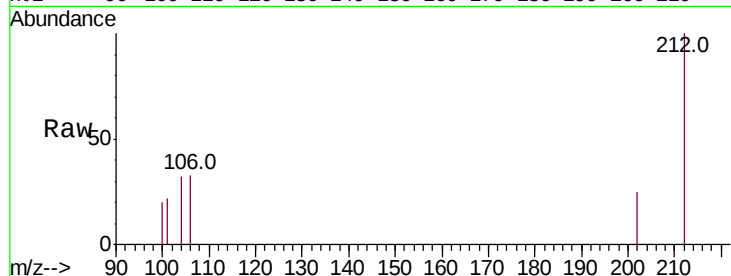

#18
Benzo(a)anthracene
Concen: 2.269 ng/ul
RT: 21.12 min Scan# 3523
Delta R.T. 0.16 min
Lab File: BE097305.D
Acq: 17 Aug 2018 20:21

Tgt Ion:228 Resp: 45
Ion Ratio Lower Upper
228 100
229 94.7 22.8 34.2#
226 93.3 17.0 25.6#

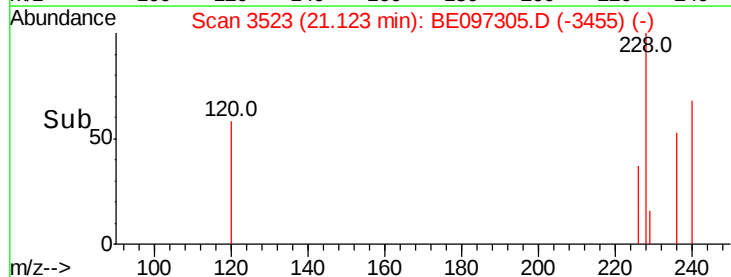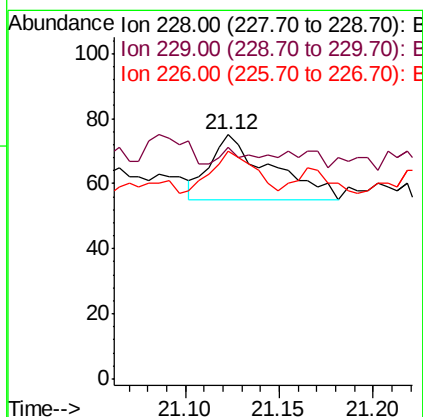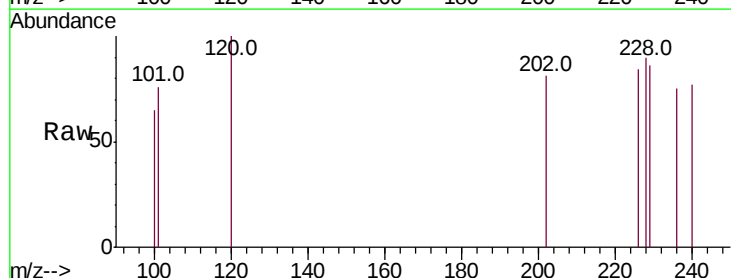

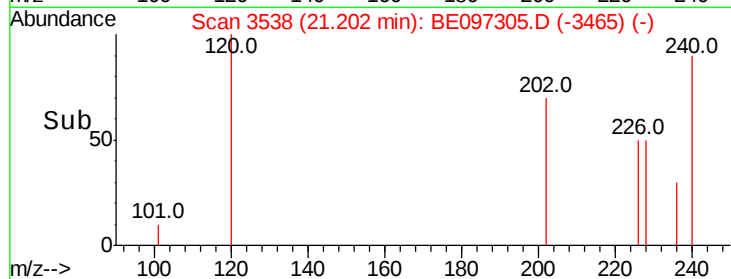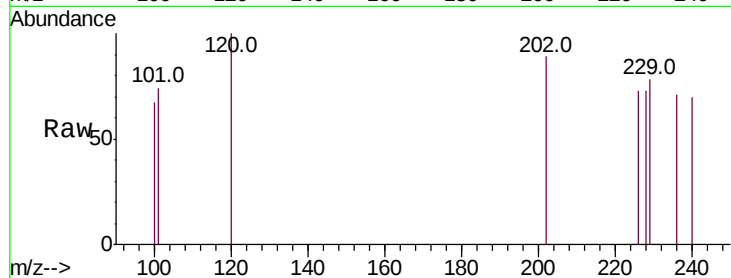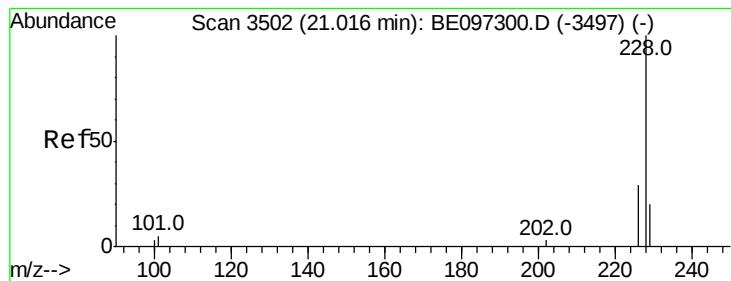

#19

Chrysene

Concen: 0.676 ng/ul

RT: 21.20 min Scan# 3538

Delta R.T. 0.19 min

Lab File: BE097305.D

Acq: 17 Aug 2018 20:21

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 228 Resp: 16

Ion Ratio Lower Upper

228 100

226 100.0 23.4 35.0#

229 106.7 17.7 26.5#

