

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
 Data File : BE097306.D
 Acq On : 17 Aug 2018 21:00
 Operator : SJ/JU
 Sample : PB111072BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 17 23:34:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 17 23:33:44 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1091	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	5786	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	3257	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	553352	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.98
20) Perylene-d12	23.21	264	11902	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	2414	0.26	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.02	166	869	0.075	ng/ul#	22
23) Benzo(a)pyrene	23.07	252	1947	0.065	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
Data File : BE097306.D
Acq On : 17 Aug 2018 21:00
Operator : SJ/JU
Sample : PB111072BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 17 23:34:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 17 23:33:44 2018
Response via : Initial Calibration




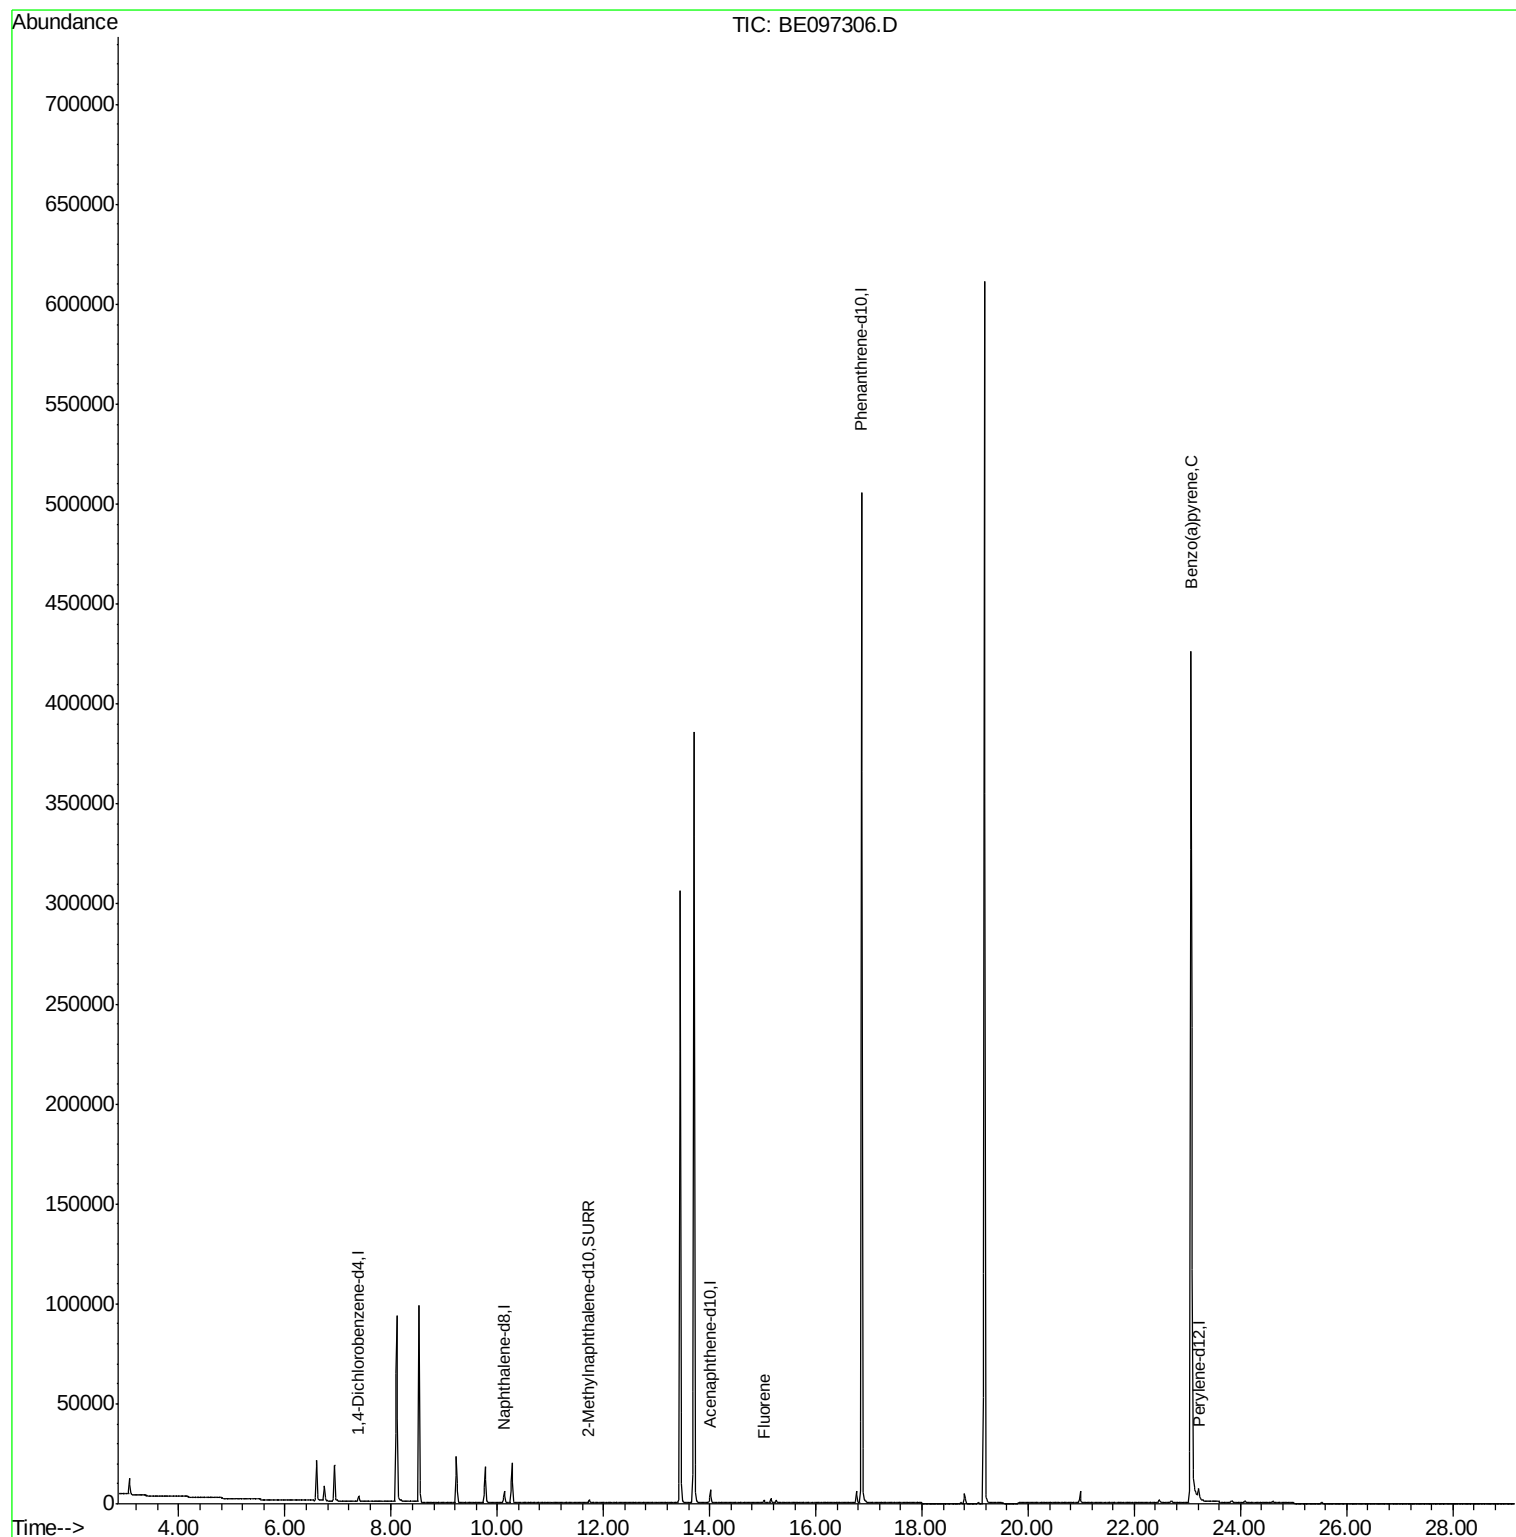


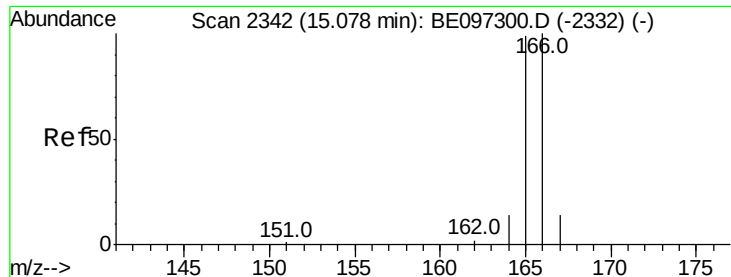

#9
Fluorene
 Concen: 0.075 ng/ul
 RT: 15.02 min Scan# 2332
 Delta R.T. -0.06 min
 Lab File: BE097306.D
 Acq: 17 Aug 2018 21:00

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:166 Resp: 869
 Ion Ratio Lower Upper
 166 100
 165 9.9 73.4 110.2#
 167 35.1 14.6 22.0#

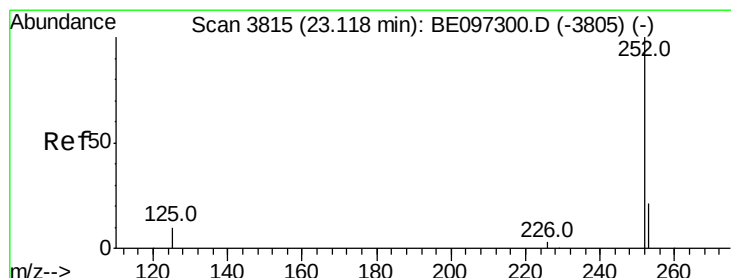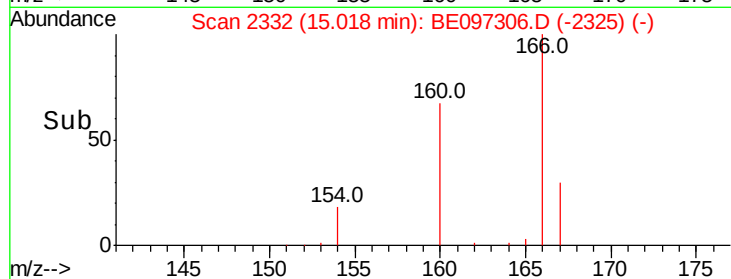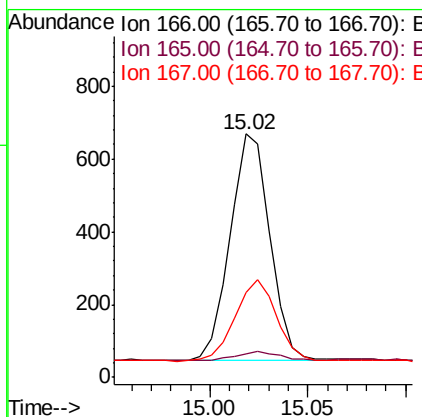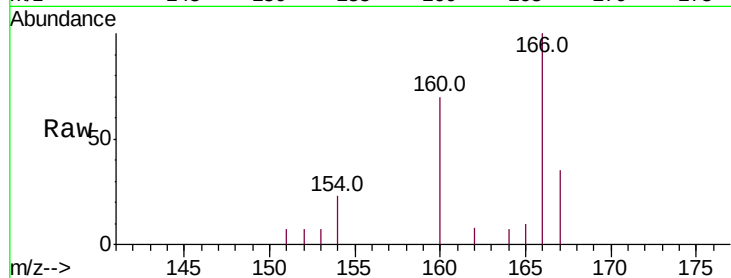

#23
Benzo(a)pyrene
 Concen: 0.065 ng/ul
 RT: 23.07 min Scan# 3808
 Delta R.T. -0.05 min
 Lab File: BE097306.D
 Acq: 17 Aug 2018 21:00

Tgt Ion:252 Resp: 1947
 Ion Ratio Lower Upper
 252 100
 253 36.4 28.5 42.7
 125 25.0 18.1 27.1

