

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
 Data File : BE097307.D
 Acq On : 17 Aug 2018 21:36
 Operator : SJ/JU
 Sample : PB112050BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 17 23:34:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 17 23:33:44 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	979	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	4989	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	2767	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	515423	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.98
20) Perylene-d12	23.21	264	10568	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	2254	0.28	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.02	166	825	0.084	ng/ul#	21
23) Benzo(a)pyrene	23.07	252	1783	0.067	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
Data File : BE097307.D
Acq On : 17 Aug 2018 21:36
Operator : SJ/JU
Sample : PB112050BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 17 23:34:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 17 23:33:44 2018
Response via : Initial Calibration

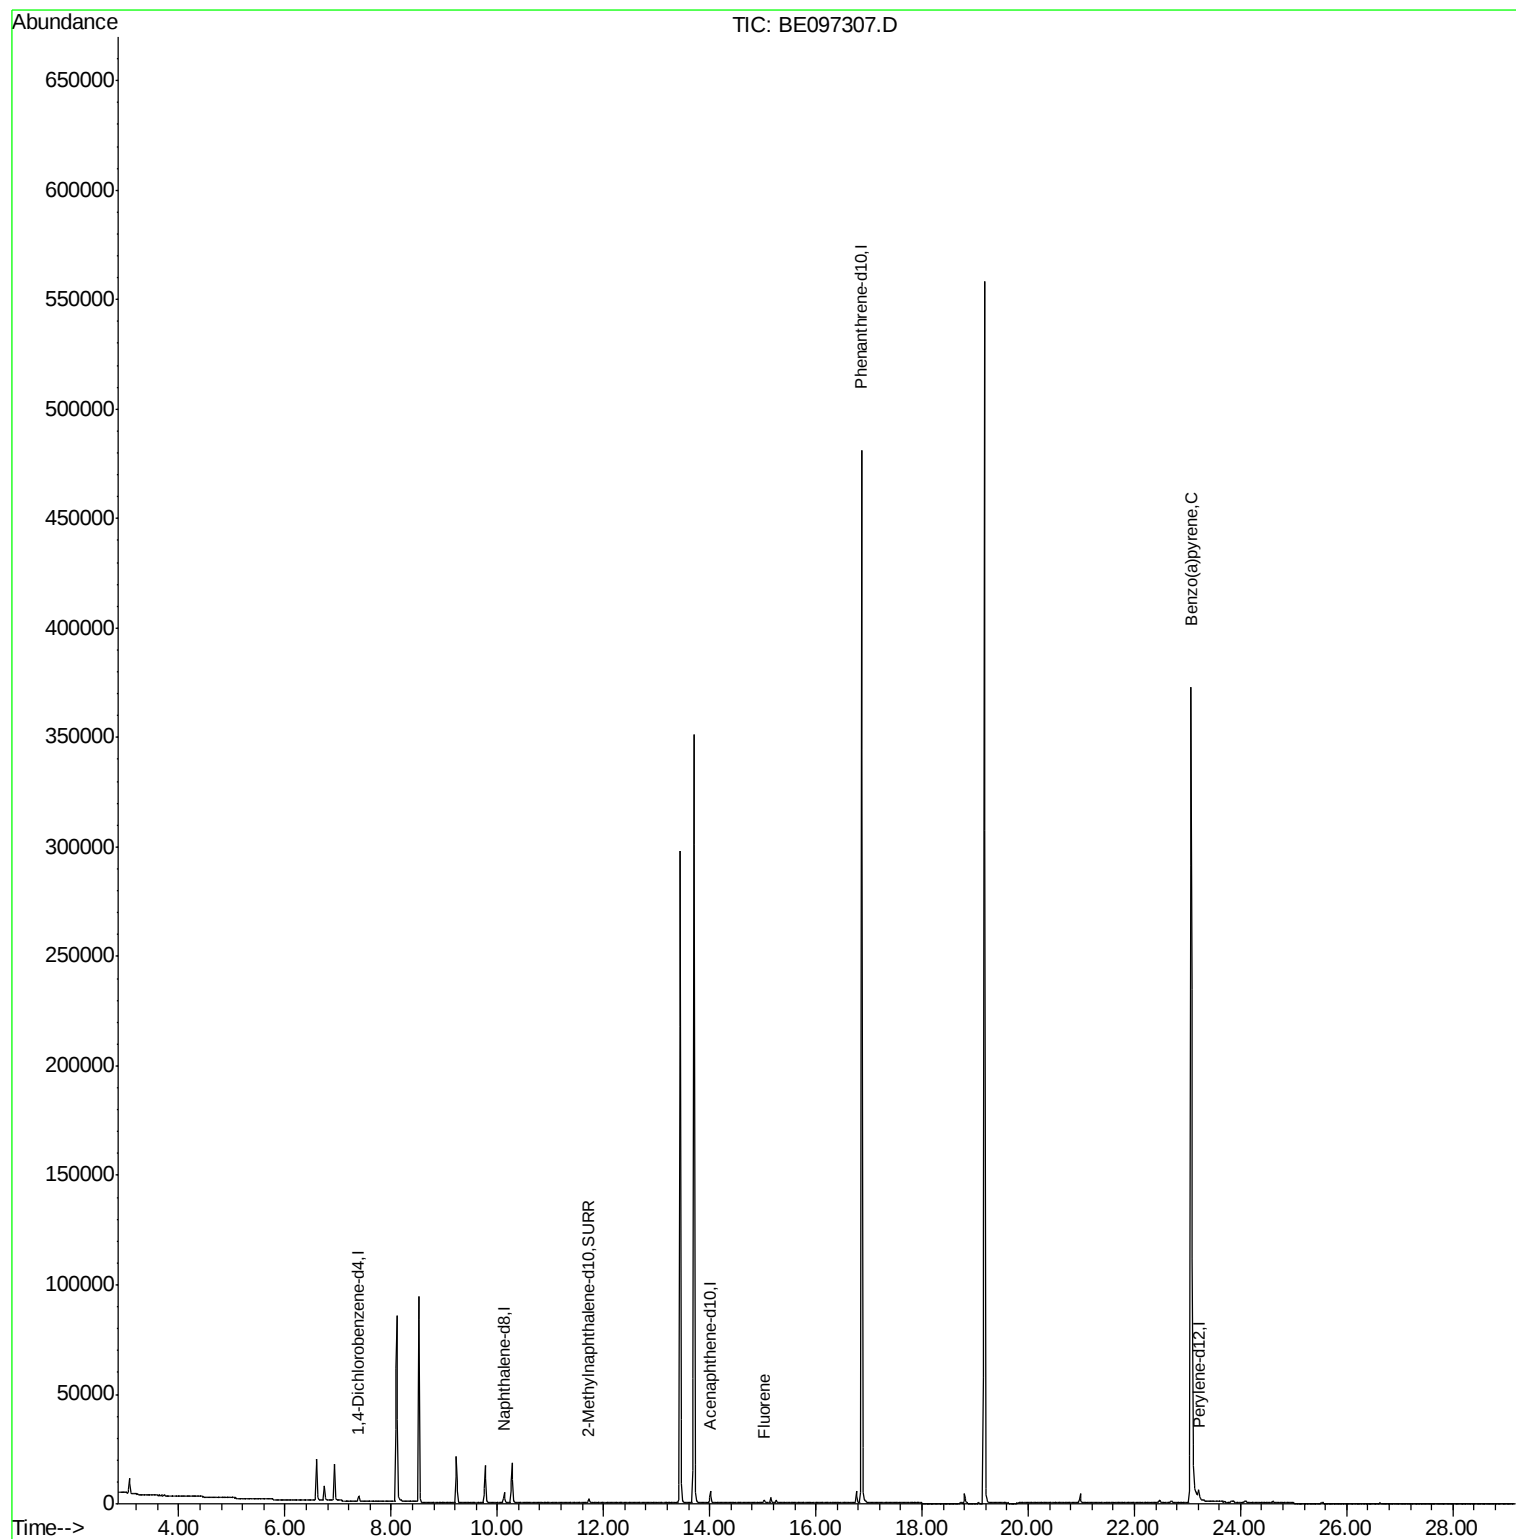

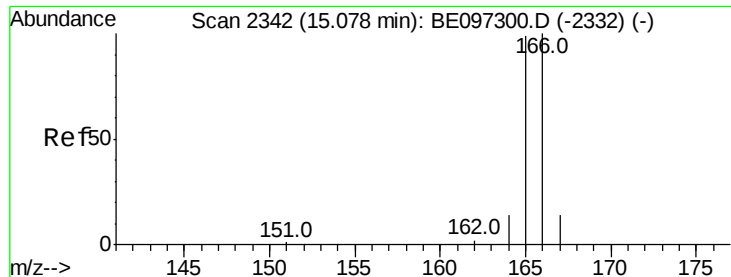

#9

Fluorene

Concen: 0.084 ng/ul

RT: 15.02 min Scan# 2333

Delta R.T. -0.05 min

Lab File: BE097307.D

Acq: 17 Aug 2018 21:36

Instrument :

BNA_E

ClientSampleId :


Tot Ion:166 Resp: 825

Ion Ratio Lower Upper


166 100

165 11.2 73.4 110.2#



167 41.3 14.6 22.0#

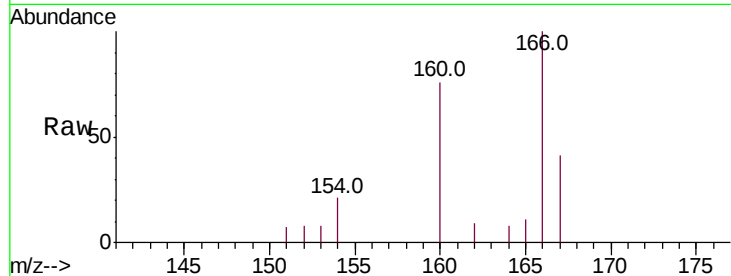

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

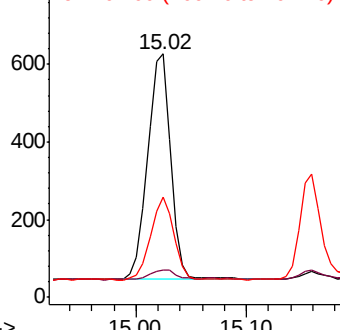

Time-->

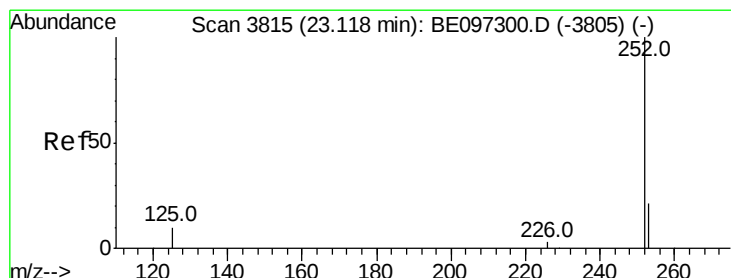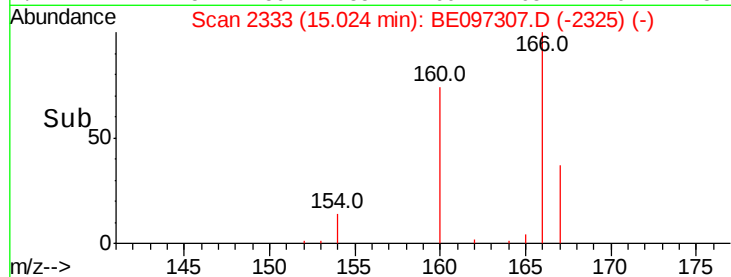

#23

Benzo(a)pyrene

Concen: 0.067 ng/ul

RT: 23.07 min Scan# 3808

Delta R.T. -0.05 min

Lab File: BE097307.D

Acq: 17 Aug 2018 21:36


Tgt Ion:252 Resp: 1783

Ion Ratio Lower Upper


252 100

253 36.5 28.5 42.7

125 25.1 18.1 27.1

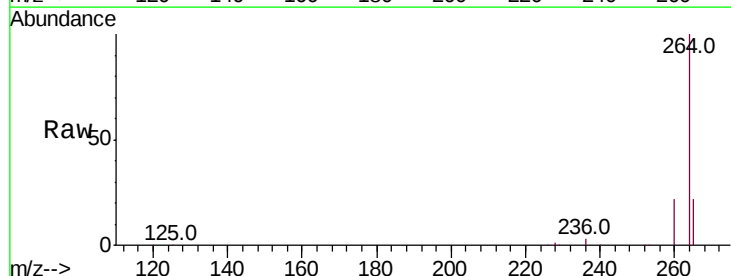

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

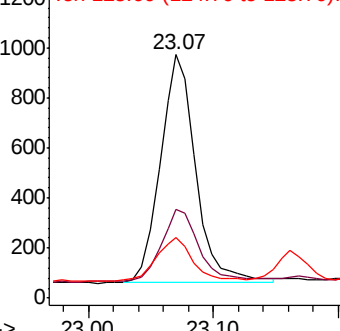

Time-->

