

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
 Data File : BE097321.D
 Acq On : 18 Aug 2018 7:03
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/20/2018 4:15:48 PM

Quant Time: Aug 20 05:13:16 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 18 05:45:47 2018
 Response via : Initial Calibration

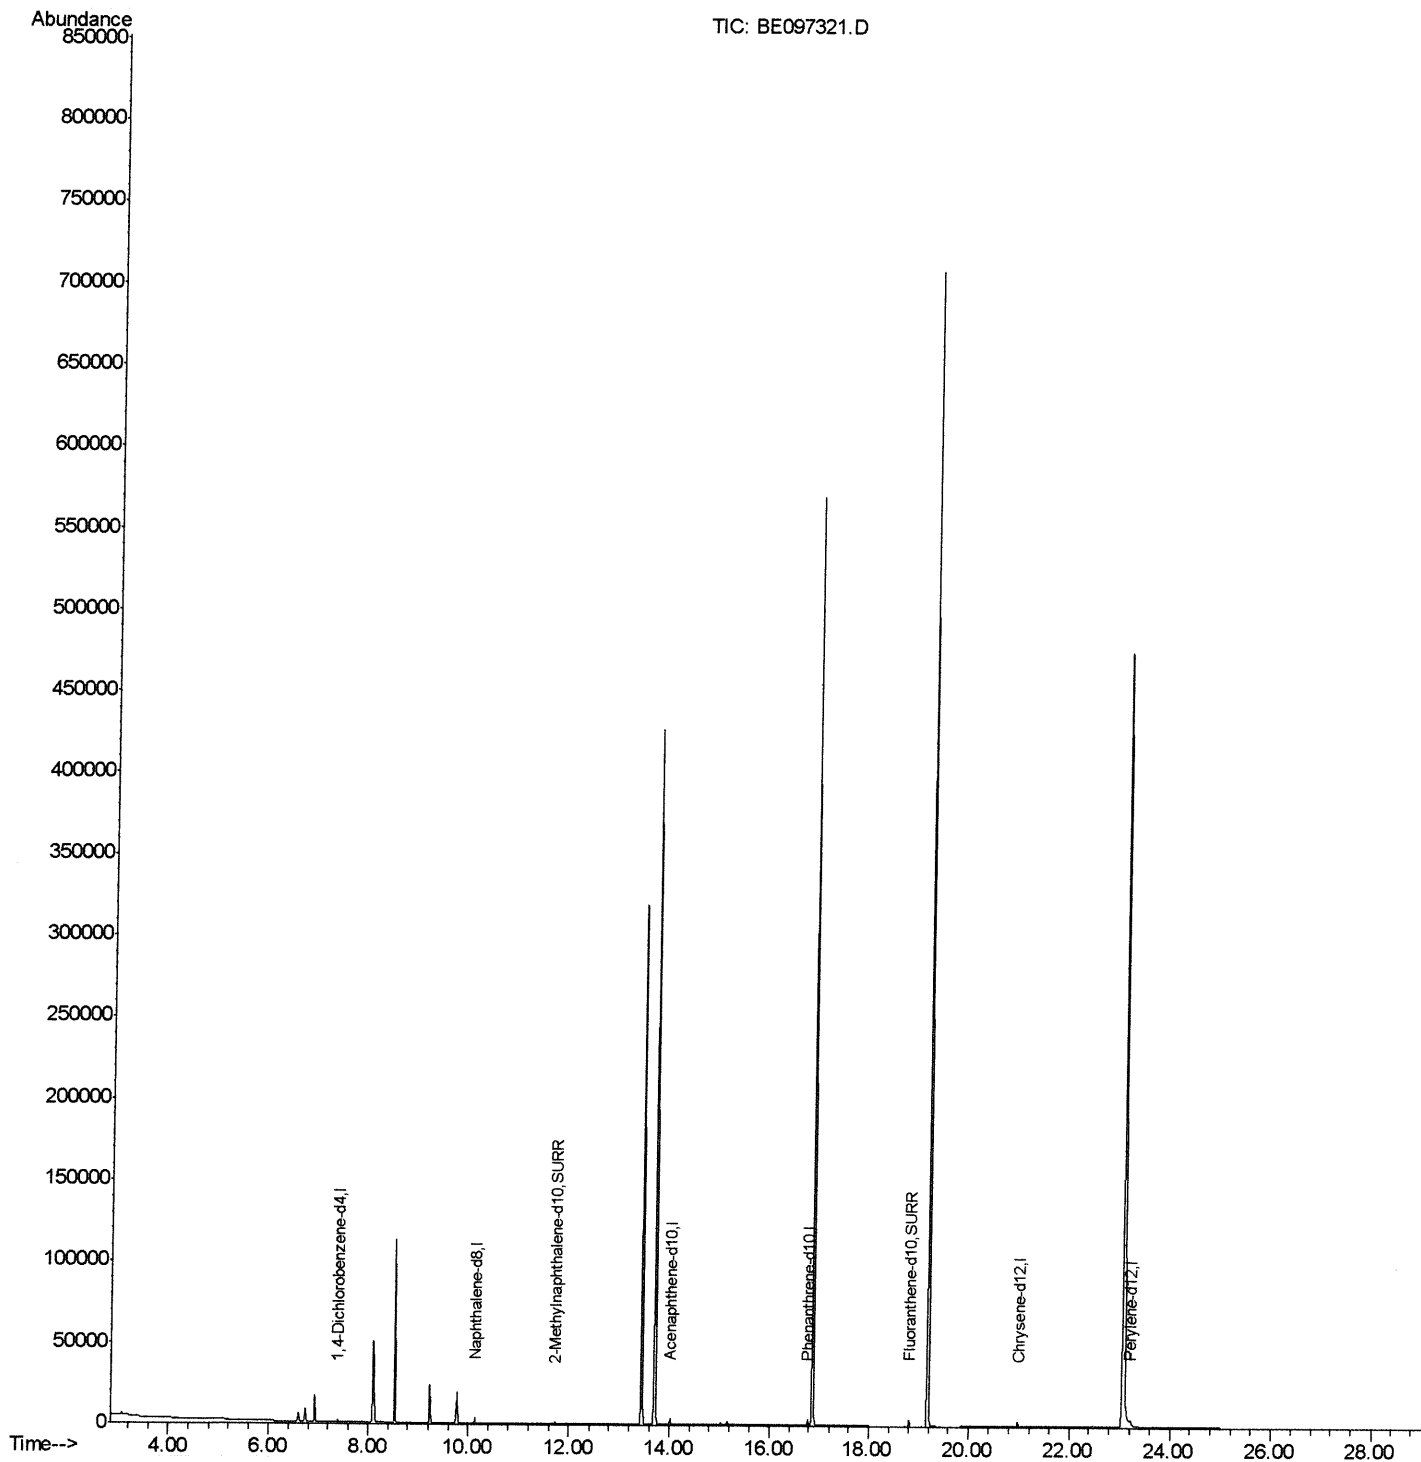

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
 Data File : BE097321.D
 Acq On : 18 Aug 2018 7:03
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/20/2018 4:15:48 PM

Quant Time: Aug 20 04:11:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 18 05:45:47 2018
 Response via : Initial Calibration

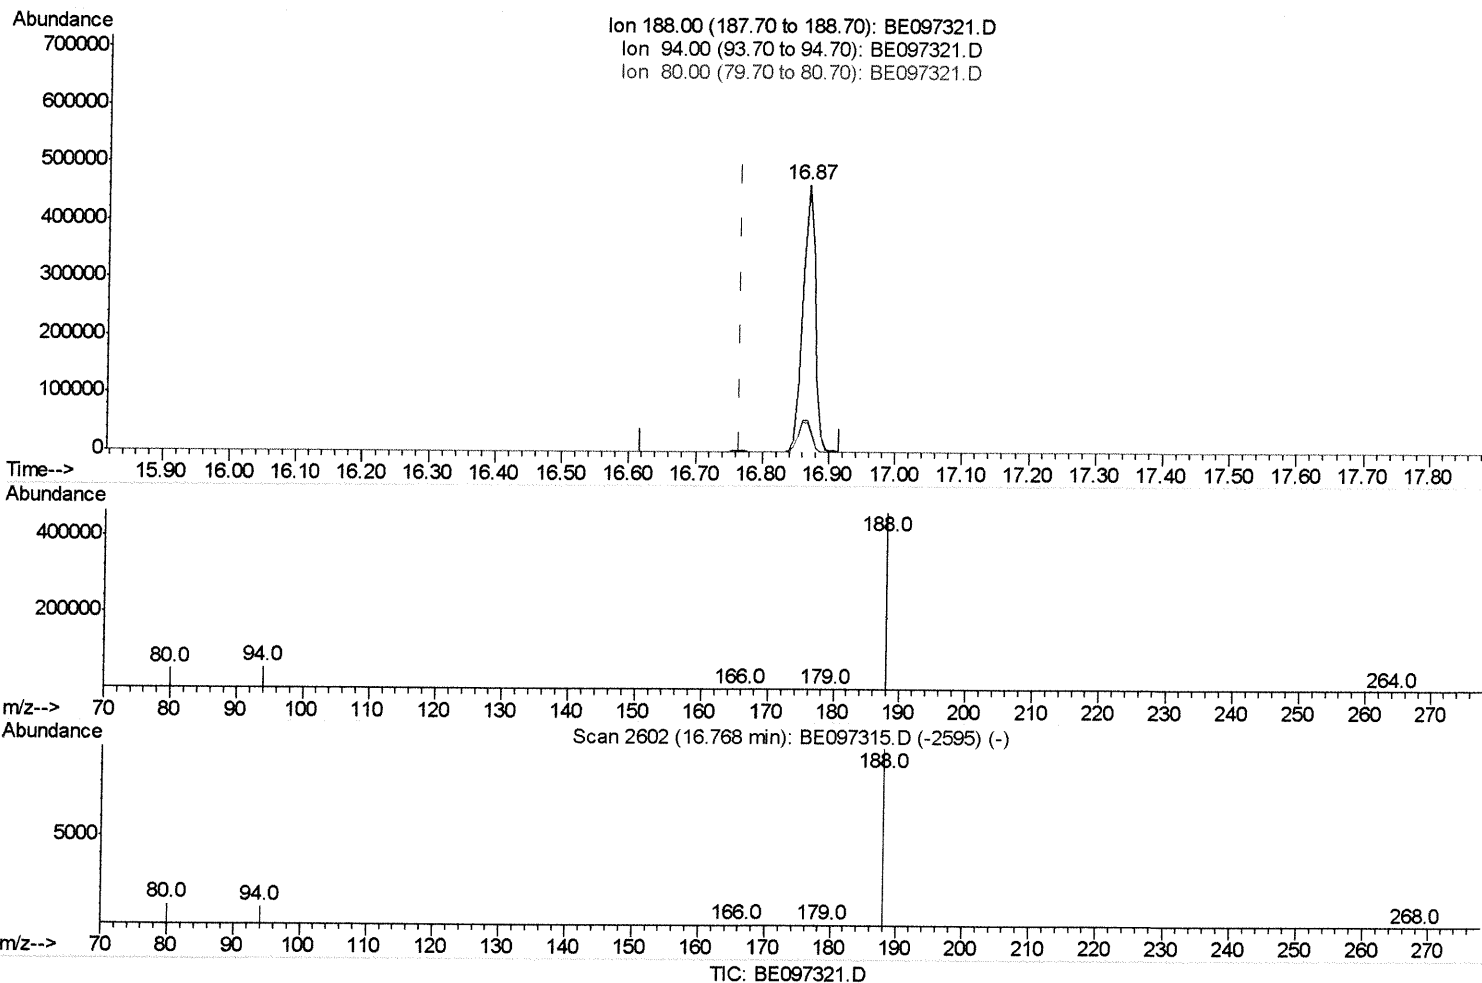

(10) Phenanthrene-d10 (I)

16.867min (+0.099) 0.40ng/ul

response 596515

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.01
80.00	11.80	10.90
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
 Data File : BE097321.D
 Acq On : 18 Aug 2018 7:03
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/20/2018 4:15:48 PM

Quant Time: Aug 20 04:11:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 18 05:45:47 2018
 Response via : Initial Calibration

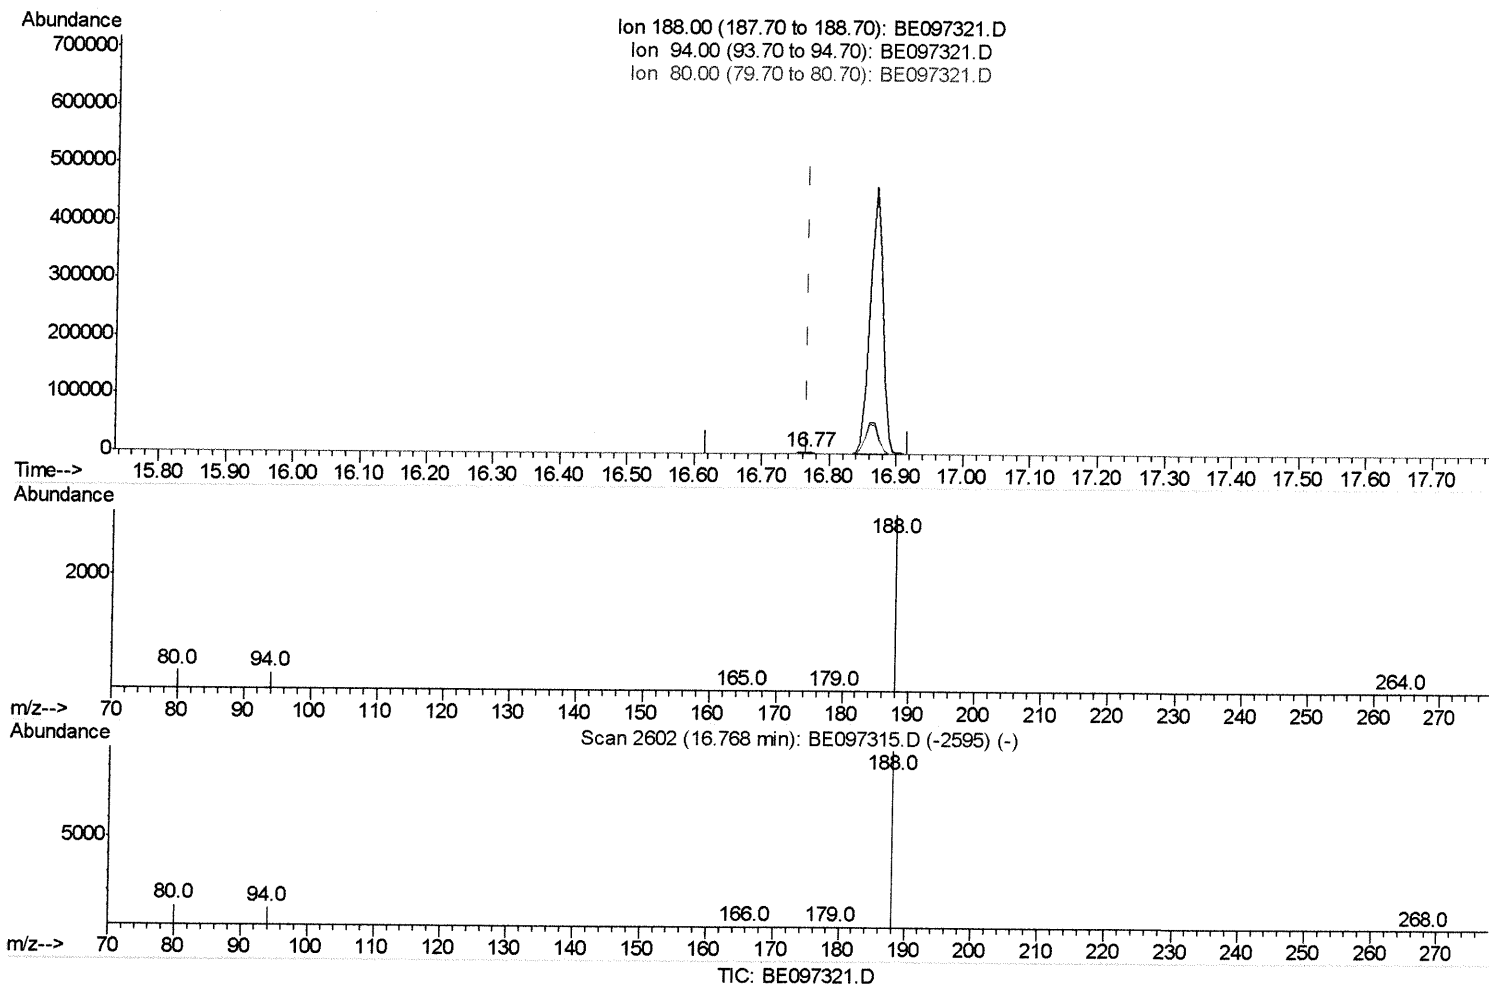

(10) Phenanthrene-d10 (I)

16.768min (+0.000) 0.40ng/ul m

SJ 8/22/18

response 4396

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.48
80.00	11.80	11.42
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
Data File : BE097321.D
Acq On : 18 Aug 2018 7:03
Operator : SJ/JU
Sample : J4422-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AB3

Manual Integrations
APPROVED

Sohil
8/20/2018 4:15:48 PM

Quant Time: Aug 20 05:11:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 18 05:45:47 2018
Response via : Initial Calibration

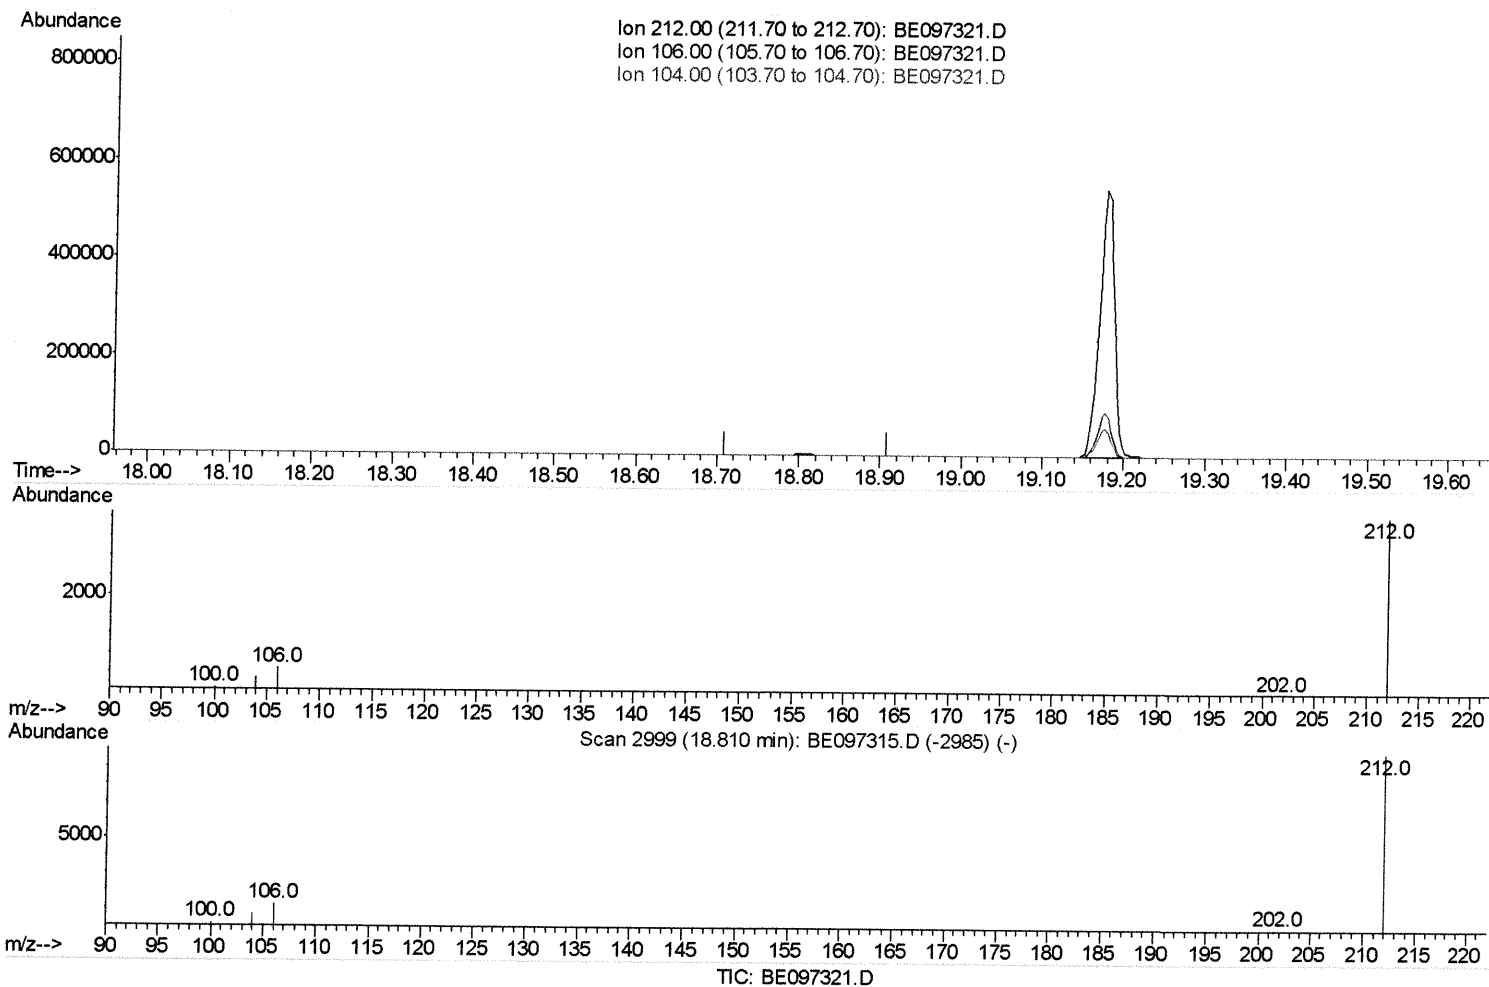

(14) Fluoranthene-d10 (SURR)

18.810min (-18.810) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
 Data File : BE097321.D
 Acq On : 18 Aug 2018 7:03
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/20/2018 4:15:48 PM

Quant Time: Aug 20 05:11:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 18 05:45:47 2018
 Response via : Initial Calibration

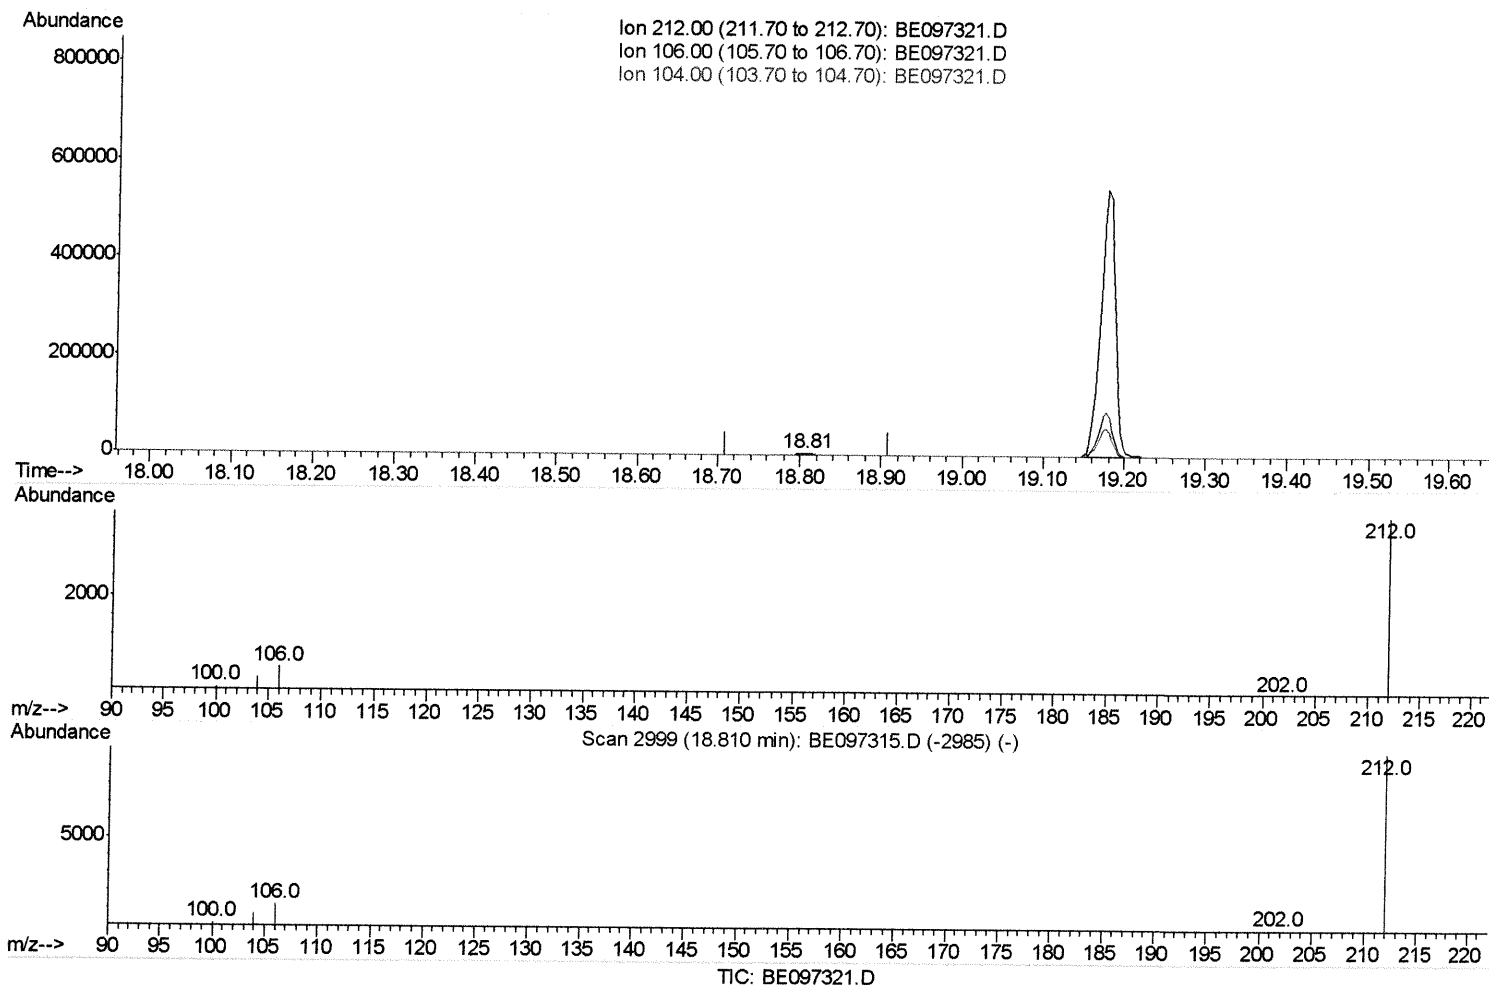

(14) Fluoranthene-d10 (SURR)

18.806min (-0.004) 0.43ng/ul m

SJ 8/22/18

response 5062

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
 Data File : BE097321.D
 Acq On : 18 Aug 2018 7:03
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/20/2018 4:15:48 PM

Quant Time: Aug 20 05:11:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 18 05:45:47 2018
 Response via : Initial Calibration

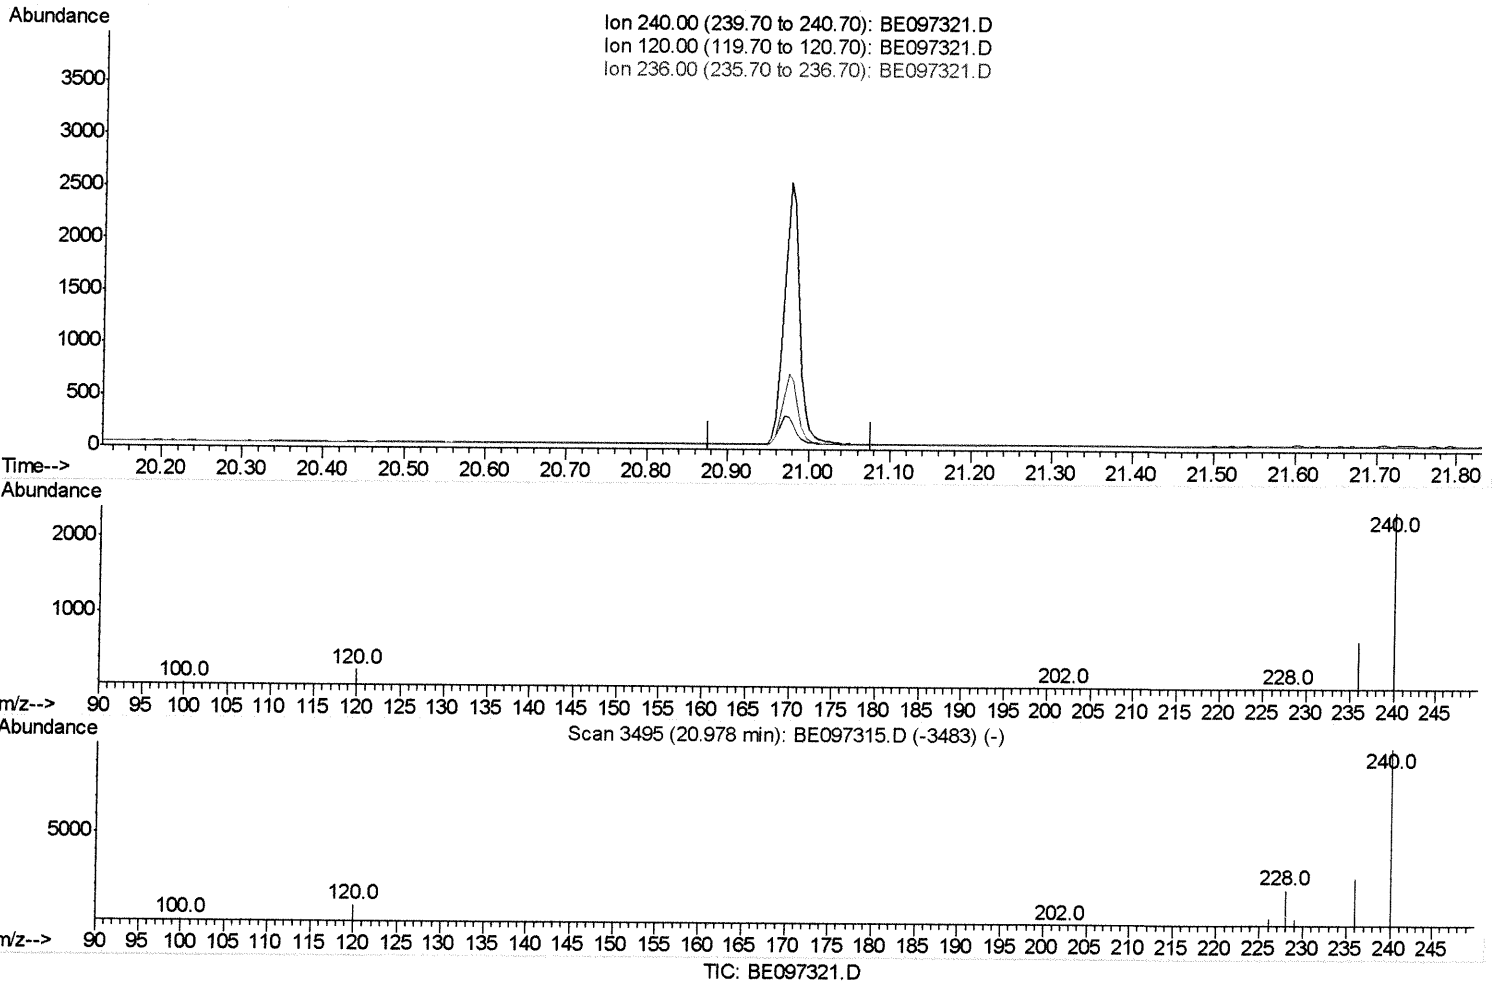

(16) Chrysene-d12 (I)
 20.978min (-20.978) 0.00ng/ul
 response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
 Data File : BE097321.D
 Acq On : 18 Aug 2018 7:03
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/20/2018 4:15:48 PM

Quant Time: Aug 20 05:11:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 18 05:45:47 2018
 Response via : Initial Calibration

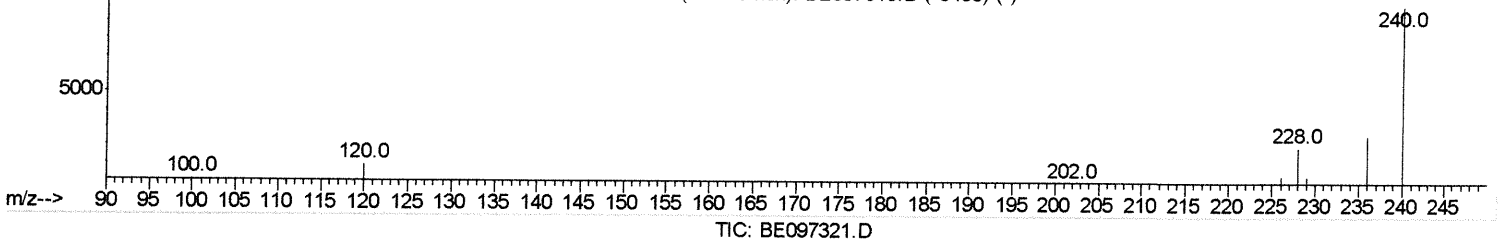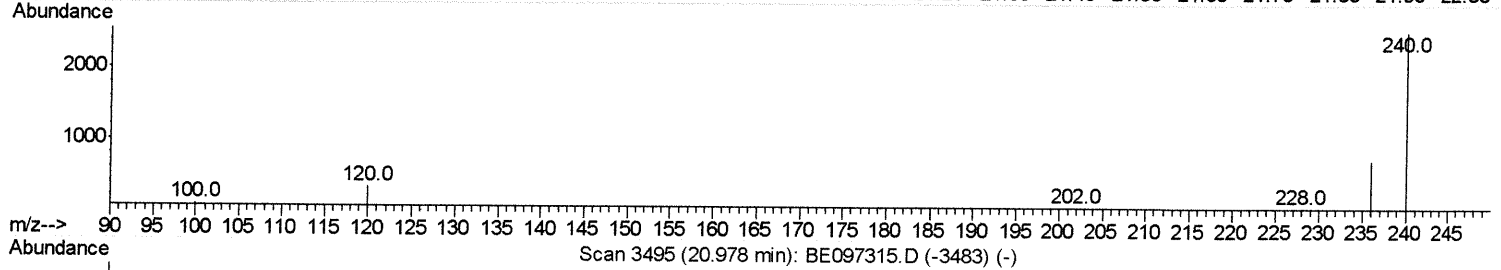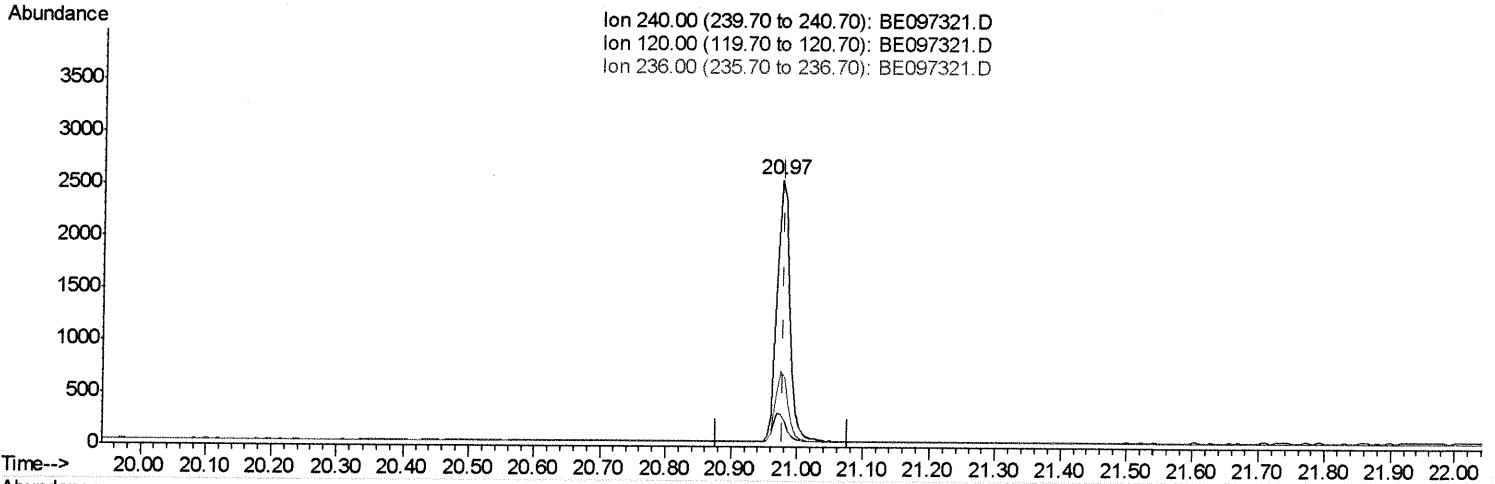

(16) Chrysene-d12 (I)

20.975min (-0.004) 0.40ng/ul m

SJ 8/22/18

response 3358

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	12.40#
236.00	34.90	28.63
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
Data File : BE097321.D
Acq On : 18 Aug 2018 7:03
Operator : SJ/JU
Sample : J4422-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AB3

Manual Integrations
APPROVED

Sohil
8/20/2018 4:15:48 PM

Quant Time: Aug 20 05:12:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 18 05:45:47 2018
Response via : Initial Calibration

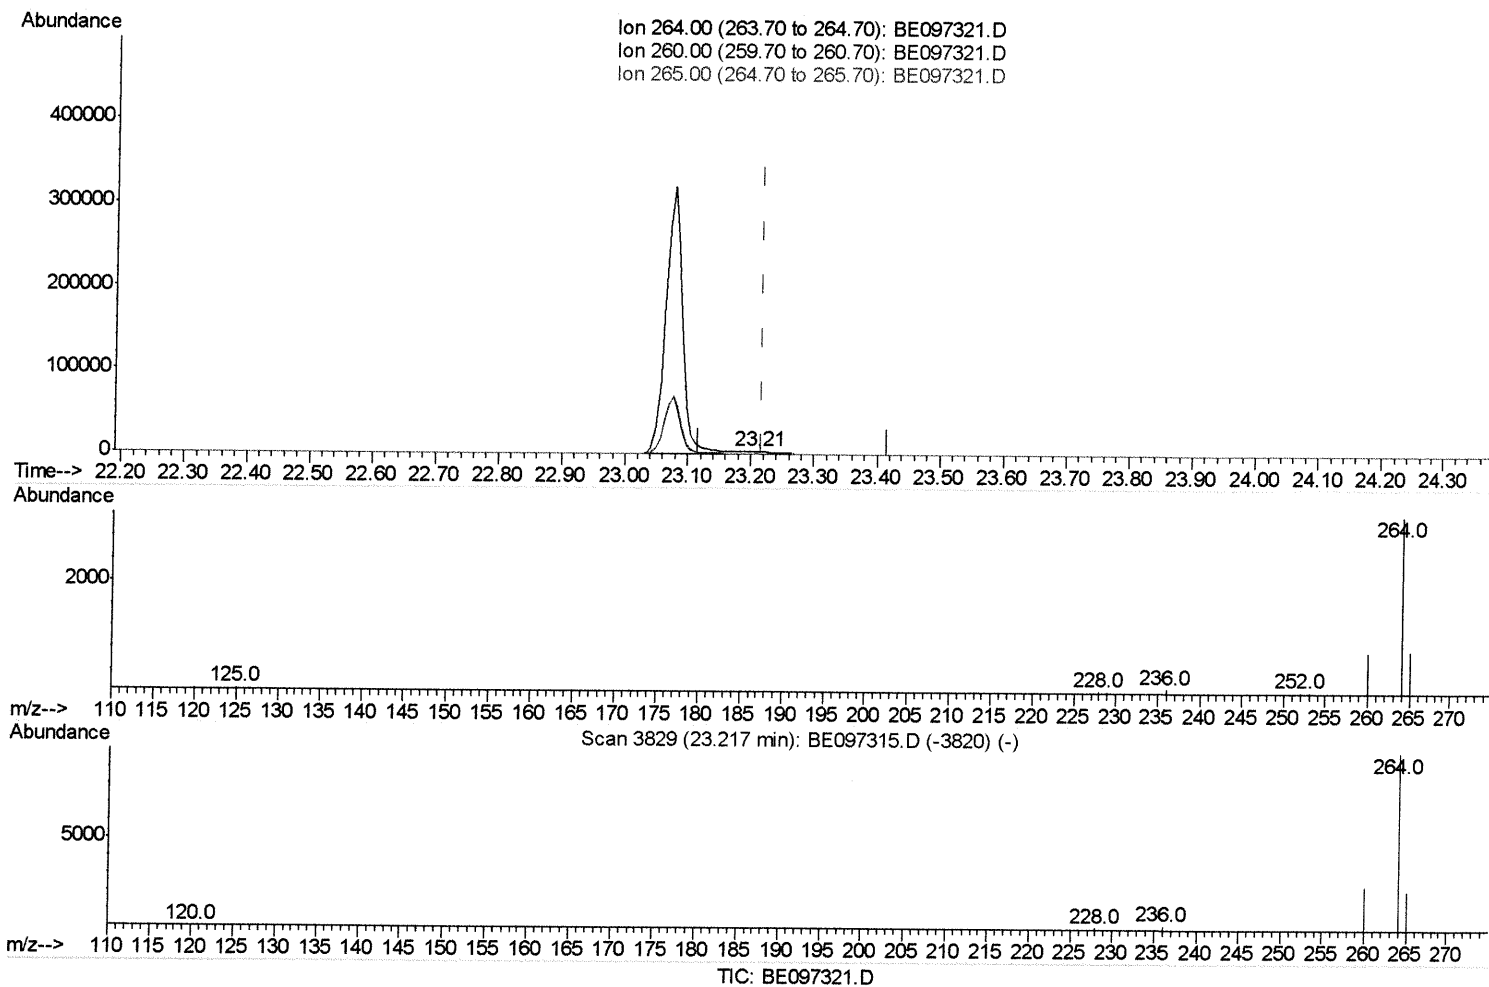

(20) Perylene-d12 (I)

23.209min (-0.008) 0.40ng/ul

response 8820

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.38
265.00	103.50	24.97#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
 Data File : BE097321.D
 Acq On : 18 Aug 2018 7:03
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/20/2018 4:15:48 PM

Quant Time: Aug 20 05:12:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 18 05:45:47 2018
 Response via : Initial Calibration

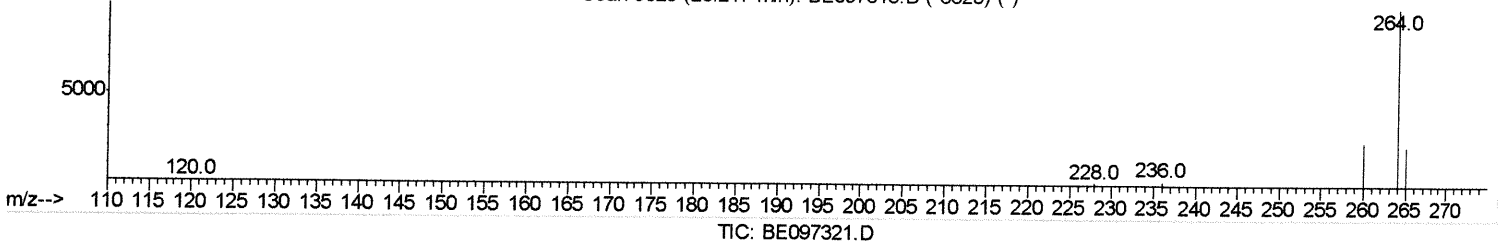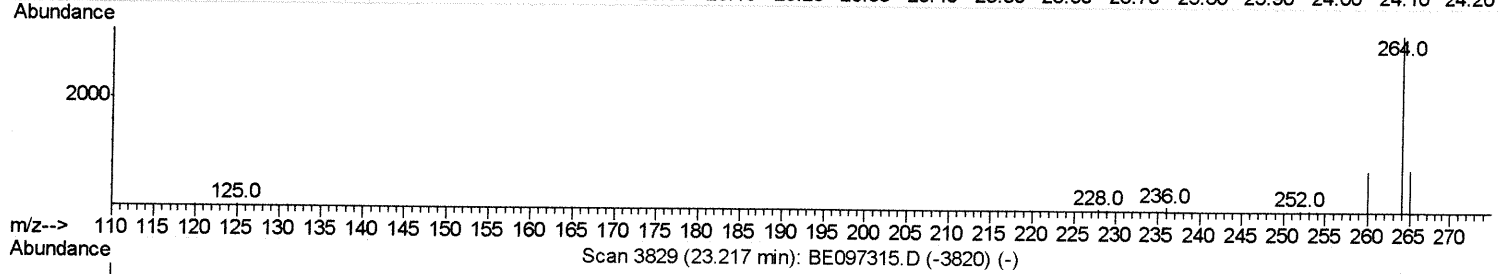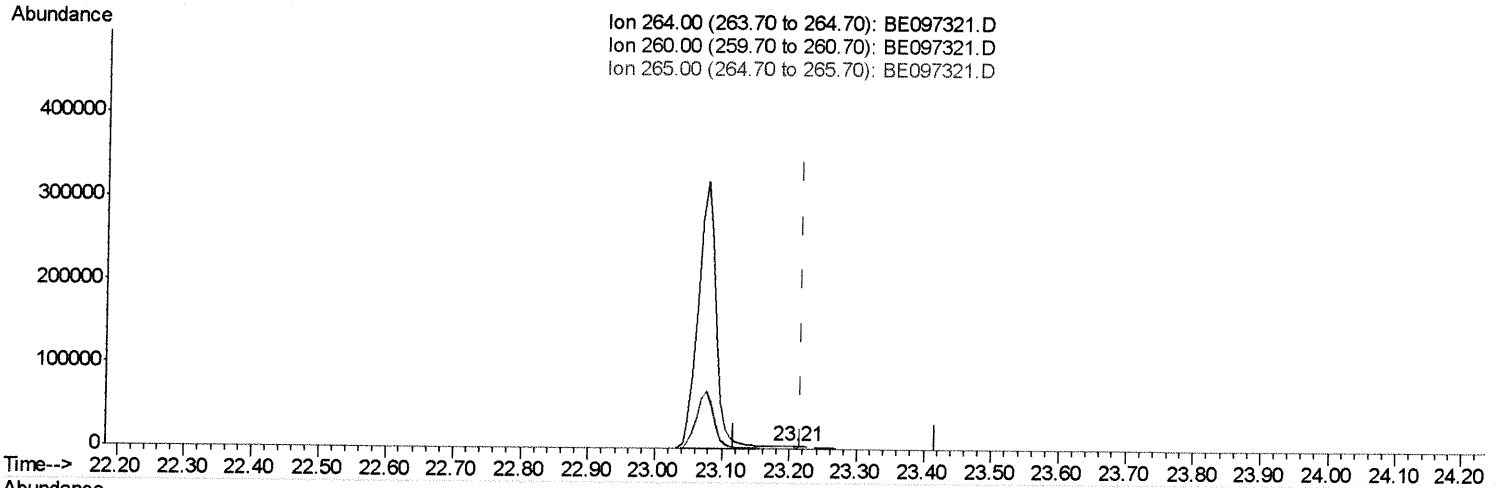

(20) Perylene-d12 (I)

23.209min (-0.008) 0.40ng/ul m

518/22/18

response 2240

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.38
265.00	103.50	24.97#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
Data File : BE097321.D
Acq On : 18 Aug 2018 7:03
Operator : SJ/JU
Sample : J4422-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AB3

Manual Integrations
APPROVED

Sohil
8/20/2018 4:15:48 PM

Quant Time: Aug 20 05:13:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 18 05:45:47 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	849	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	4089	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	1886	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.77	188	4396m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	3358m	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	2240m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.72	152	1974	0.30	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	5062m	0.43	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ 8/22/18

SJ 8/22/18