

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
 Data File : BE097302.D
 Acq On : 17 Aug 2018 18:28
 Operator : SJ/JU
 Sample : J4424-08MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3YR7MS

Quant Time: Aug 17 23:34:22 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 17 23:33:44 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1042	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	5269	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	2687	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.77	188	6362	0.40	ng/ul	0.00
16) Chrysene-d12	20.98	240	5337	0.40	ng/ul	0.00
20) Perylene-d12	23.22	264	5169	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	1617	0.19	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	3535	0.21	ng/ul	0.00
Target Compounds				Ovalue		
8) Acenaphthene	14.08	153	1622	0.186	ng/ul#	89
17) Pyrene	19.20	202	3298	0.205	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
Data File : BE097302.D
Acq On : 17 Aug 2018 18:28
Operator : SJ/JU
Sample : J4424-08MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3YR7MS

Quant Time: Aug 17 23:34:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 17 23:33:44 2018
Response via : Initial Calibration

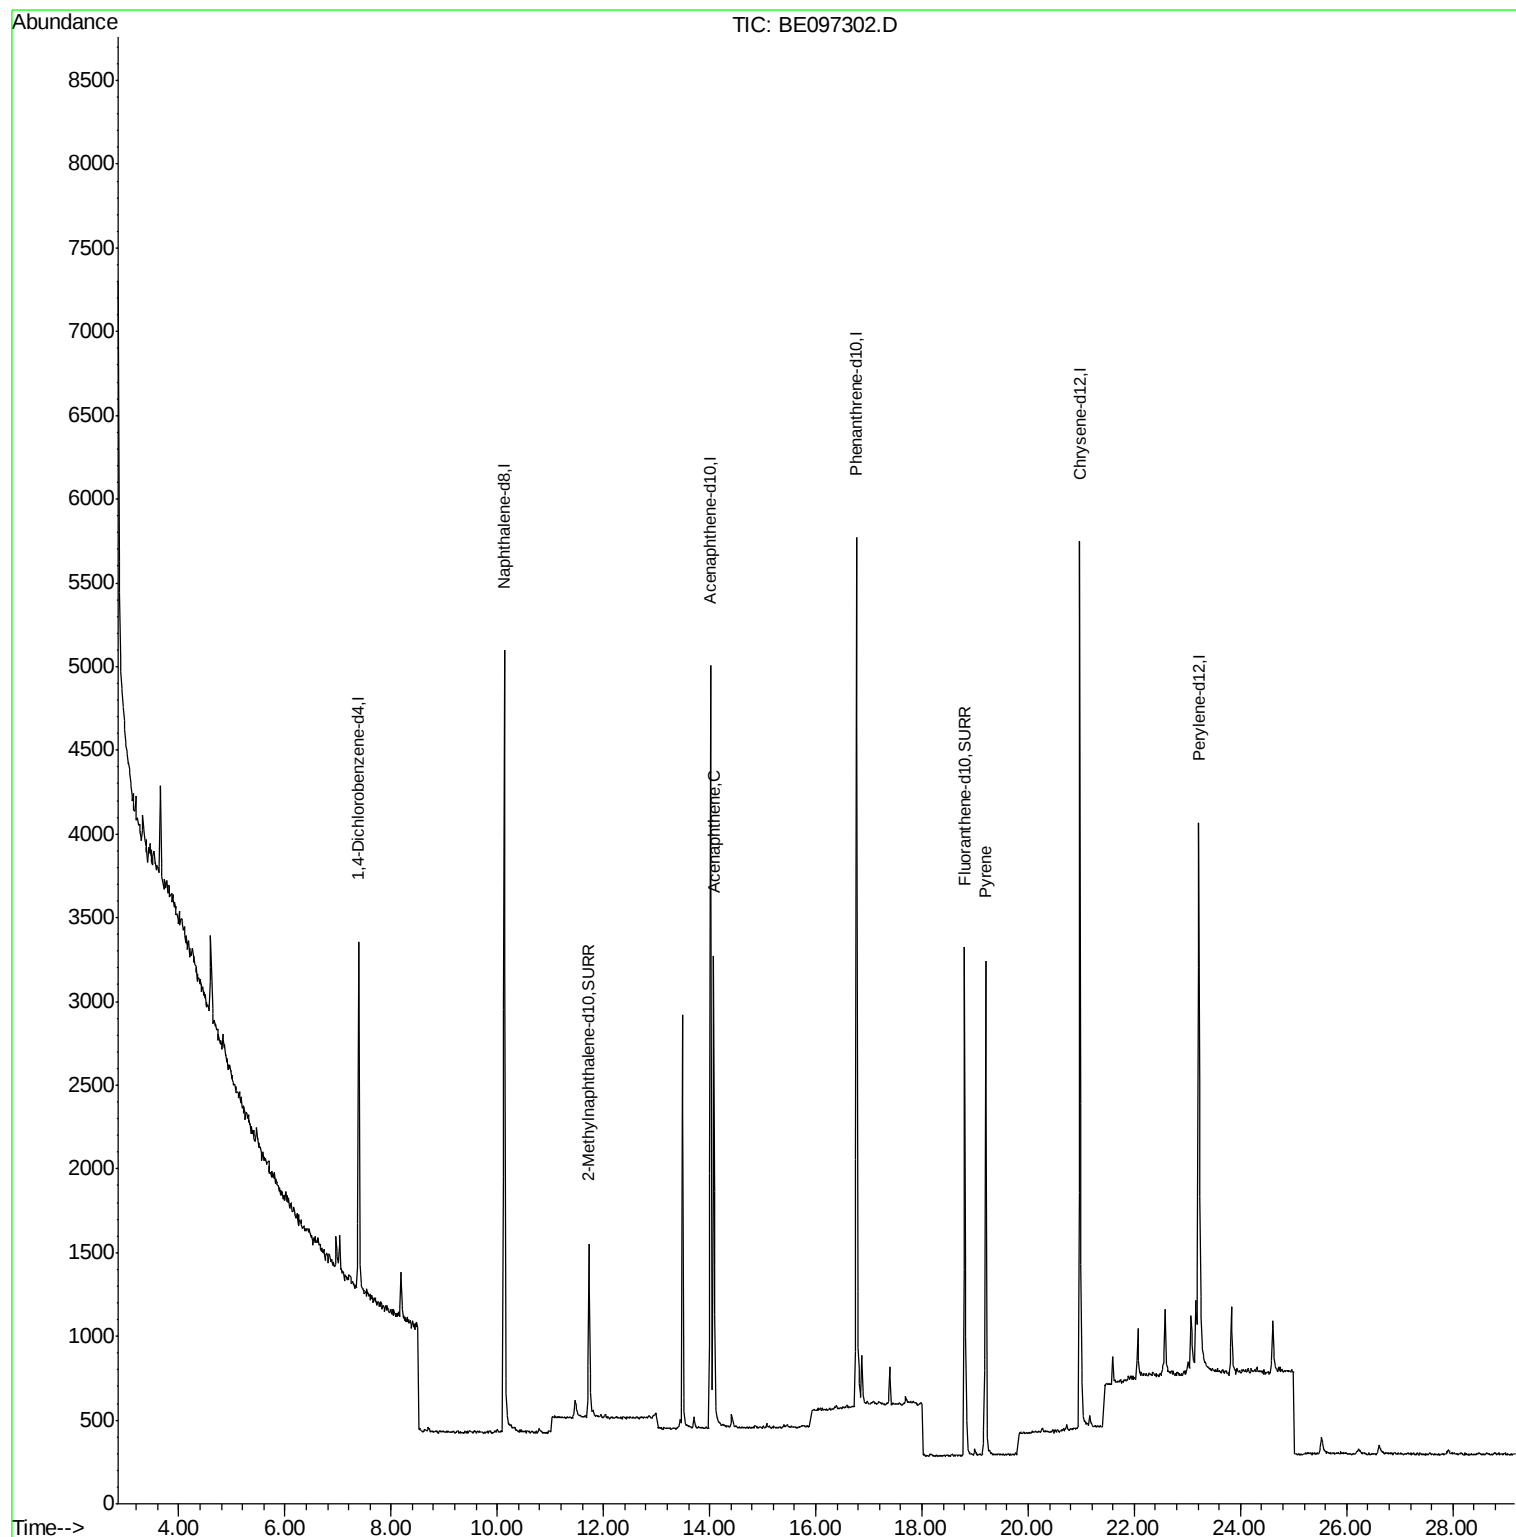

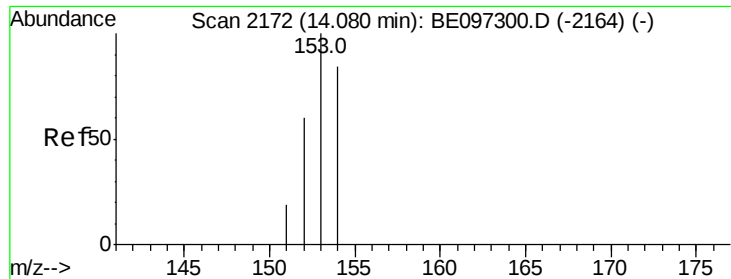

#8

Acenaphthene

Concen: 0.186 ng/ul

RT: 14.08 min Scan# 2171

Delta R.T. -0.00 min

Lab File: BE097302.D

Acq: 17 Aug 2018 18:28

Instrument :

BNA_E

ClientSampleId :

A3YR7MS


Tot Ion:153 Resp: 1622

Ion Ratio Lower Upper

153 100

152 63.3 36.0 54.0#




154 87.1 72.0 108.0

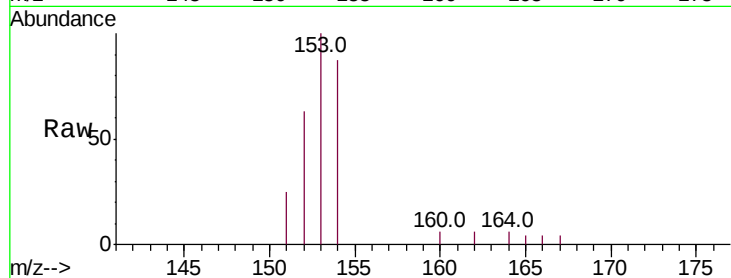

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

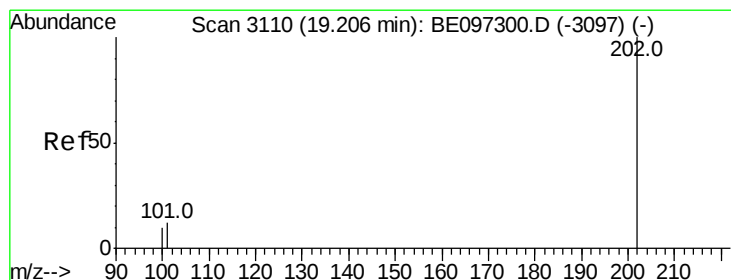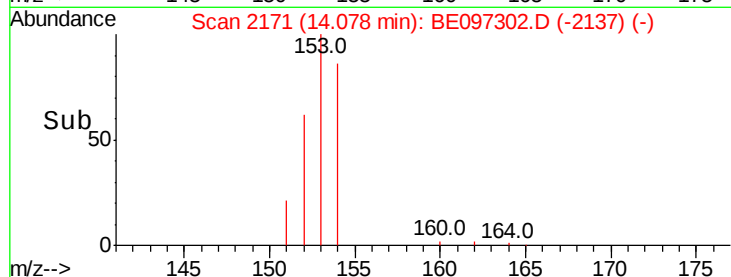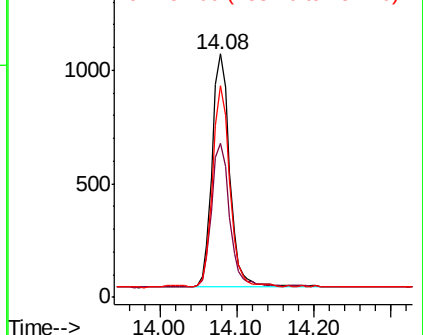

#17

Pyrene

Concen: 0.205 ng/ul

RT: 19.20 min Scan# 3108

Delta R.T. -0.00 min

Lab File: BE097302.D

Acq: 17 Aug 2018 18:28


Tgt Ion:202 Resp: 3298

Ion Ratio Lower Upper

202 100

101 14.2 18.2 27.4#

100 12.8 15.6 23.4#

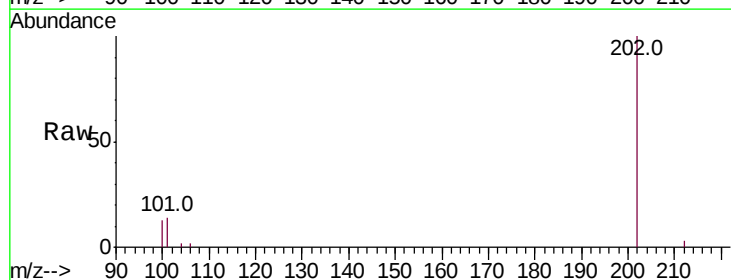

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

