

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
 Data File : BE097324.D
 Acq On : 18 Aug 2018 8:53
 Operator : SJ/JU
 Sample : J4422-20
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AE2

Manual Integrations
 APPROVED

Sohil
 8/20/2018 4:15:51 PM

Quant Time: Aug 20 05:26:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 18 05:45:47 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	782	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	3932	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	1821	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.77	188	4174m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	2577m	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	2455m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	1989	0.32	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	3966m	0.35	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.18	128	449	0.047	ng/ul#	Ovalue 76

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
Data File : BE097324.D
Acq On : 18 Aug 2018 8:53
Operator : SJ/JU
Sample : J4422-20
Misc :
ALS Vial : 36 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
C0AE2

Manual Integrations
APPROVED

Sohil
8/20/2018 4:15:51 PM

Quant Time: Aug 20 05:26:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 18 05:45:47 2018
Response via : Initial Calibration

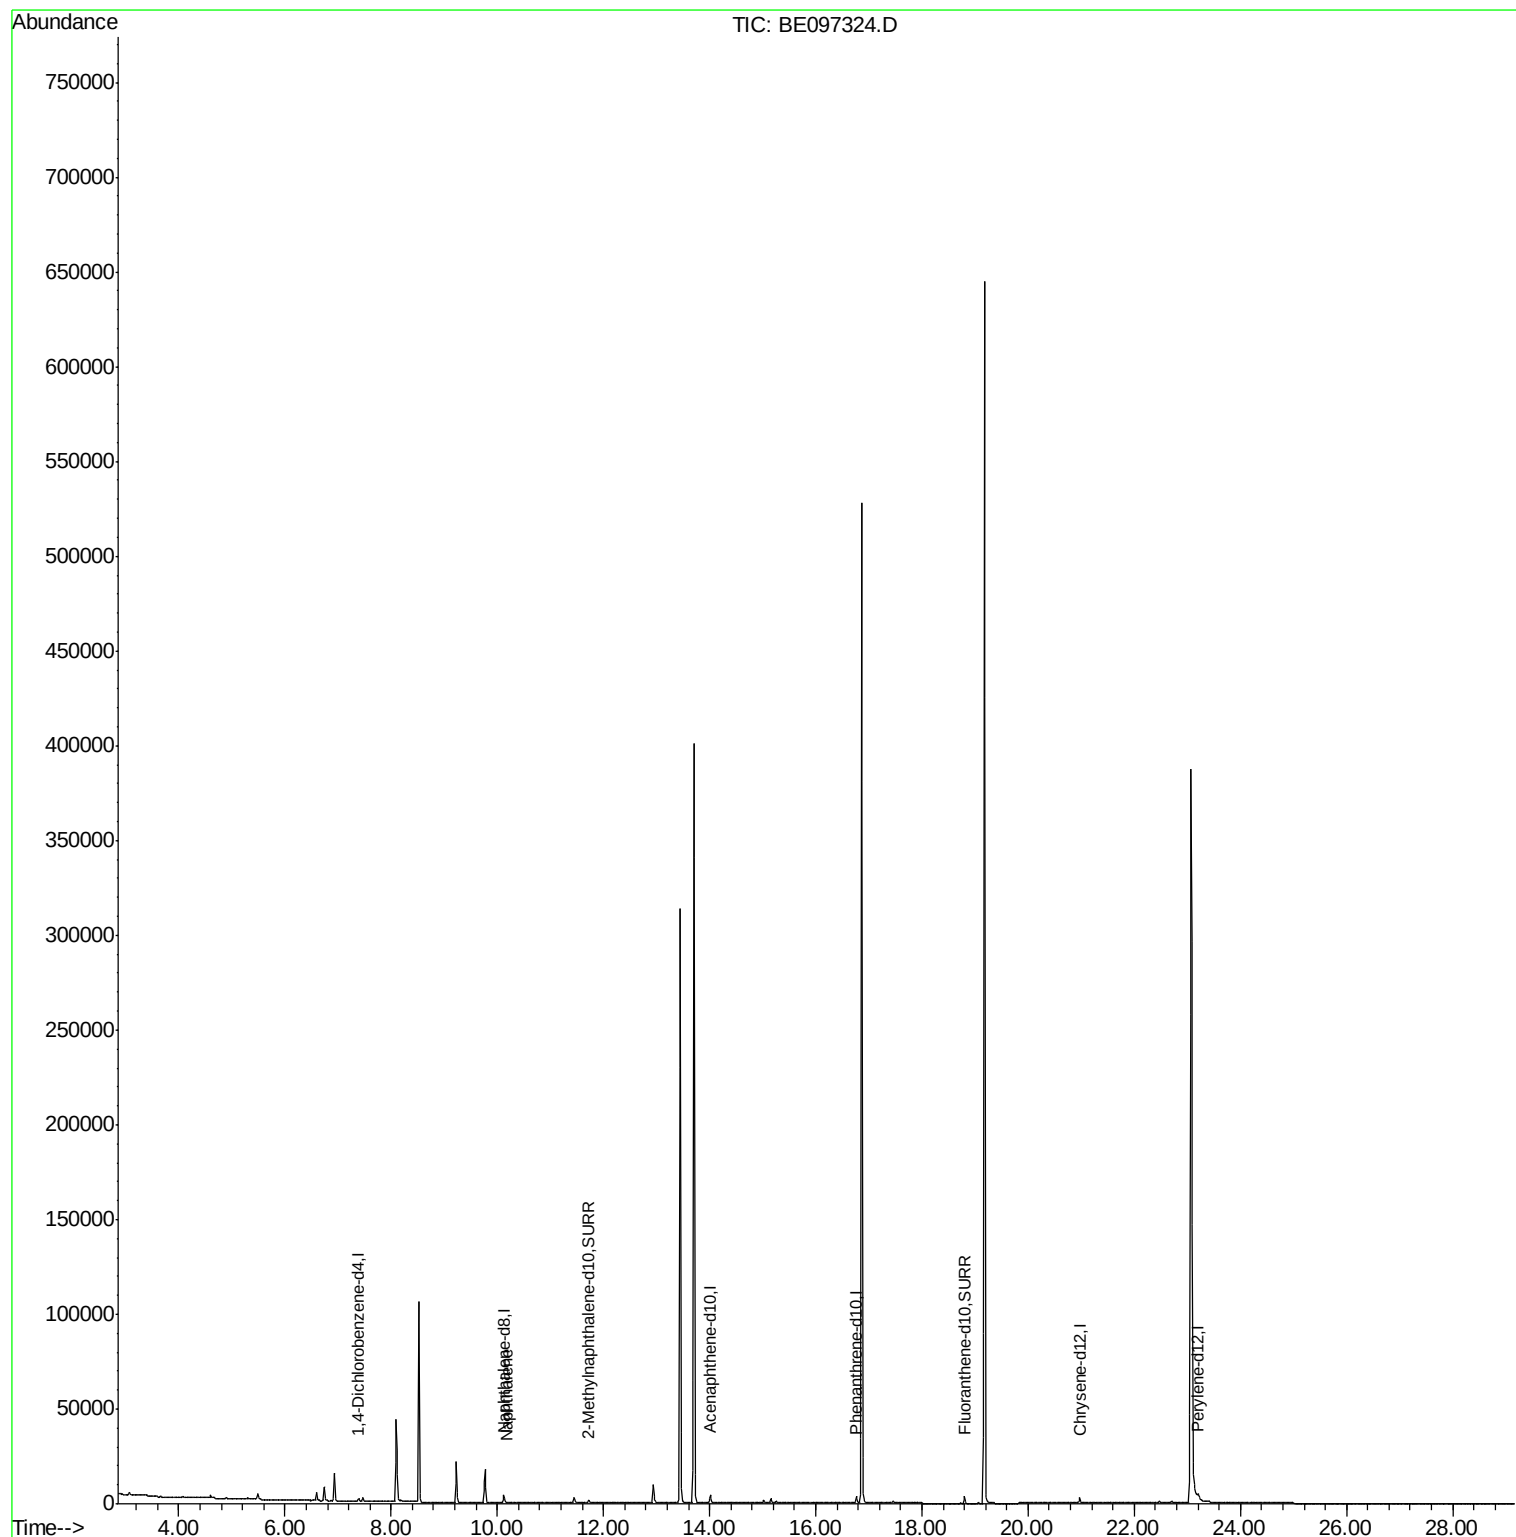

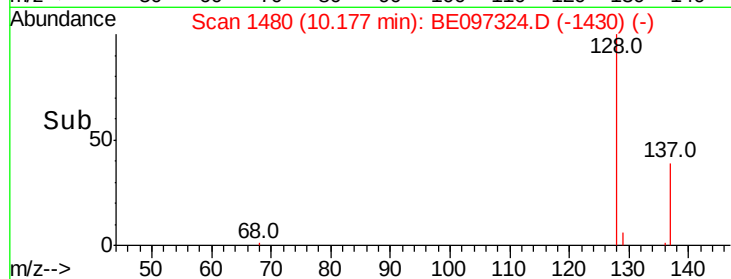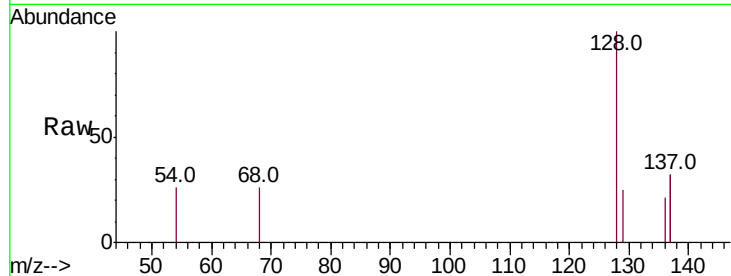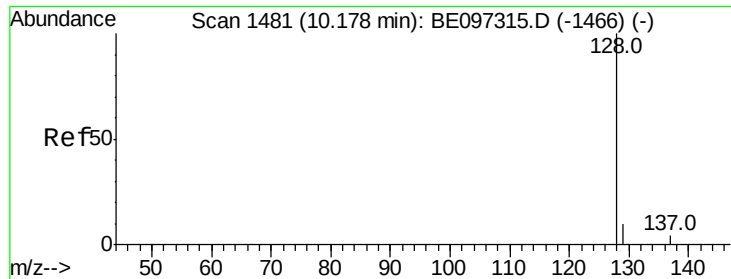

#3

Naphthalene

Concen: 0.047 ng/ul

RT: 10.18 min Scan# 1480

Delta R.T. -0.00 min

Lab File: BE097324.D

Acq: 18 Aug 2018 8:53

Instrument :

BNA_E

ClientSampleId :

C0AE2

Tot Ion:128 Resp: 449

Ion Ratio Lower Upper

128 100

129 25.1 11.3 16.9#

127 0.0 4.0 6.0#

Manual Integrations
APPROVED

Sohil
8/20/2018 4:15:51 PM

