

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
 Data File : BE097325.D
 Acq On : 18 Aug 2018 9:32
 Operator : SJ/JU
 Sample : J4424-17
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3YQ6

Manual Integrations
 APPROVED

Sohil
 8/20/2018 4:15:52 PM

Quant Time: Aug 20 05:28:49 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 18 05:45:47 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	895	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	4612	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	2325	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.77	188	5224m	0.40	ng/ul	0.00
16) Chrysene-d12	20.98	240	3454m	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	2421m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	4350	0.59	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	11434m	0.82	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.18	128	441	0.039	ng/ul#	Ovalue 75

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE081718\
Data File : BE097325.D
Acq On : 18 Aug 2018 9:32
Operator : SJ/JU
Sample : J4424-17
Misc :
ALS Vial : 37 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
A3YQ6

Manual Integrations
APPROVED

Sohil
8/20/2018 4:15:52 PM

Quant Time: Aug 20 05:28:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 18 05:45:47 2018
Response via : Initial Calibration



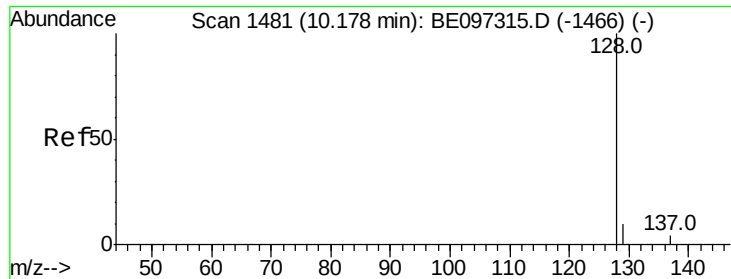

#3

Naphthalene

Concen: 0.039 ng/ul

RT: 10.18 min Scan# 1480

Delta R.T. -0.00 min

Lab File: BE097325.D

Acq: 18 Aug 2018 9:32

Instrument :

BNA_E

ClientSampleId :

A3YQ6

Tot Ion:	128	Resp:	441
Ion Ratio	Lower	Upper	
128	100		
129	25.9	11.3	16.9#
127	0.0	4.0	6.0#

Manual Integrations
APPROVED

Sohil
8/20/2018 4:15:52 PM

