
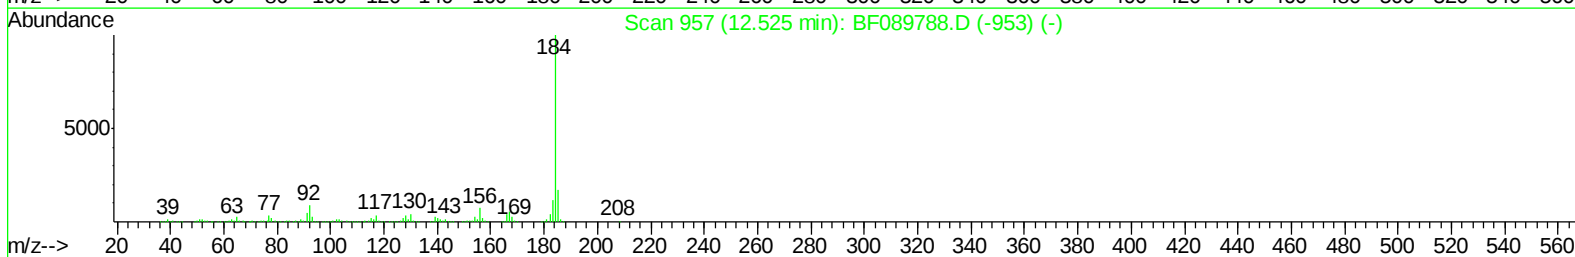
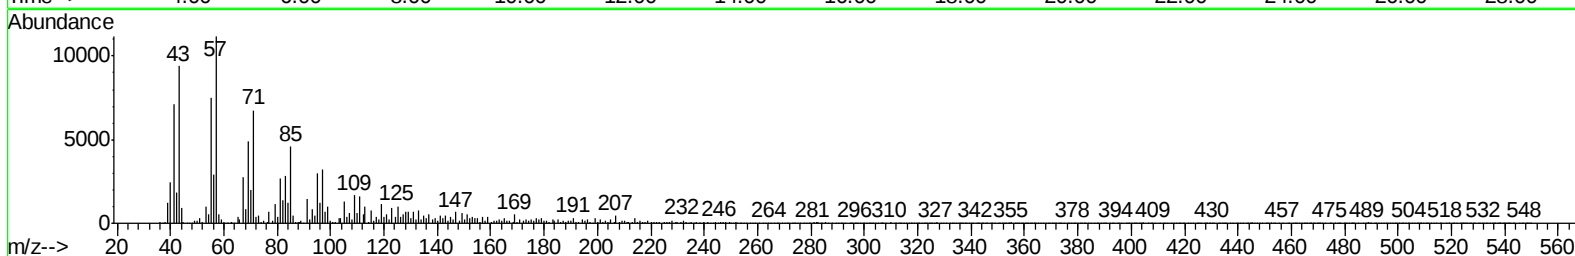


Data Path : Z:\HPCHEM1\BNA\_E\Data\BE081916\  
Data File : BE092268.D  
Acq On : 19 Aug 2016 13:35  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 06:10:47 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF081916.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 19 14:02:57 2016  
Response via : Initial Calibration

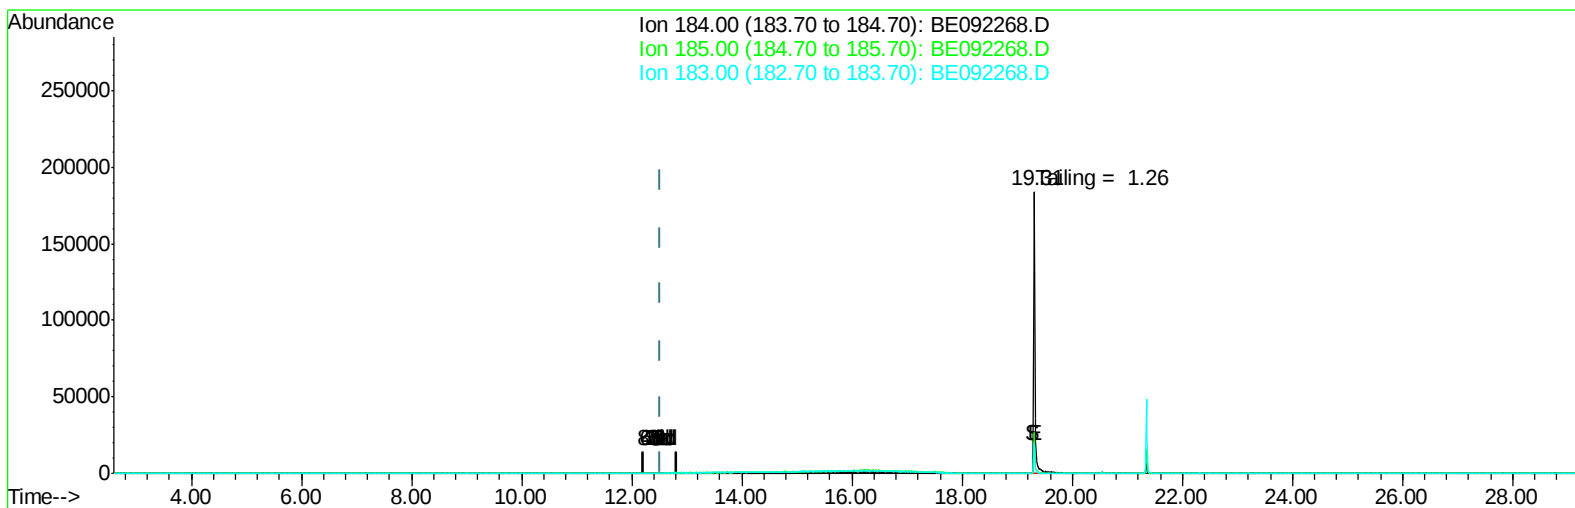

TIC: BE092268.D

(76) Benzidine




12.458min (-0.067) 20.43ng

response 39

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 184.00 | 100   | 100     |
| 185.00 | 17.30 | 119.88# |
| 183.00 | 12.10 | 137.43# |
| 0.00   | 0.00  | 0.00    |

Data Path : Z:\HPCHEM1\BNA\_E\Data\BE081916\  
Data File : BE092268.D  
Acq On : 19 Aug 2016 13:35  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 06:10:47 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF081916.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 19 14:02:57 2016  
Response via : Initial Calibration

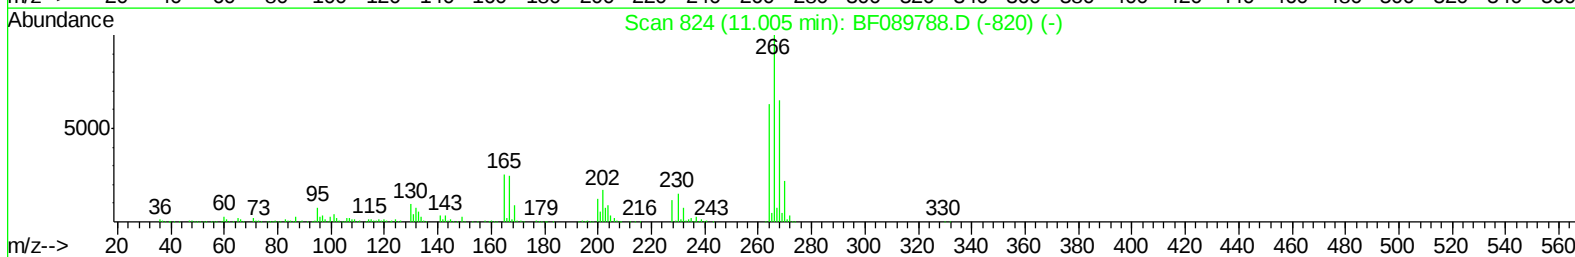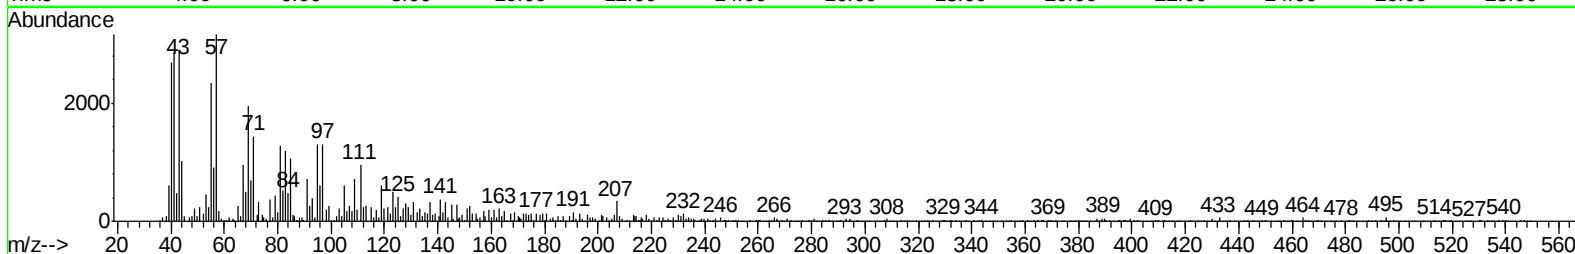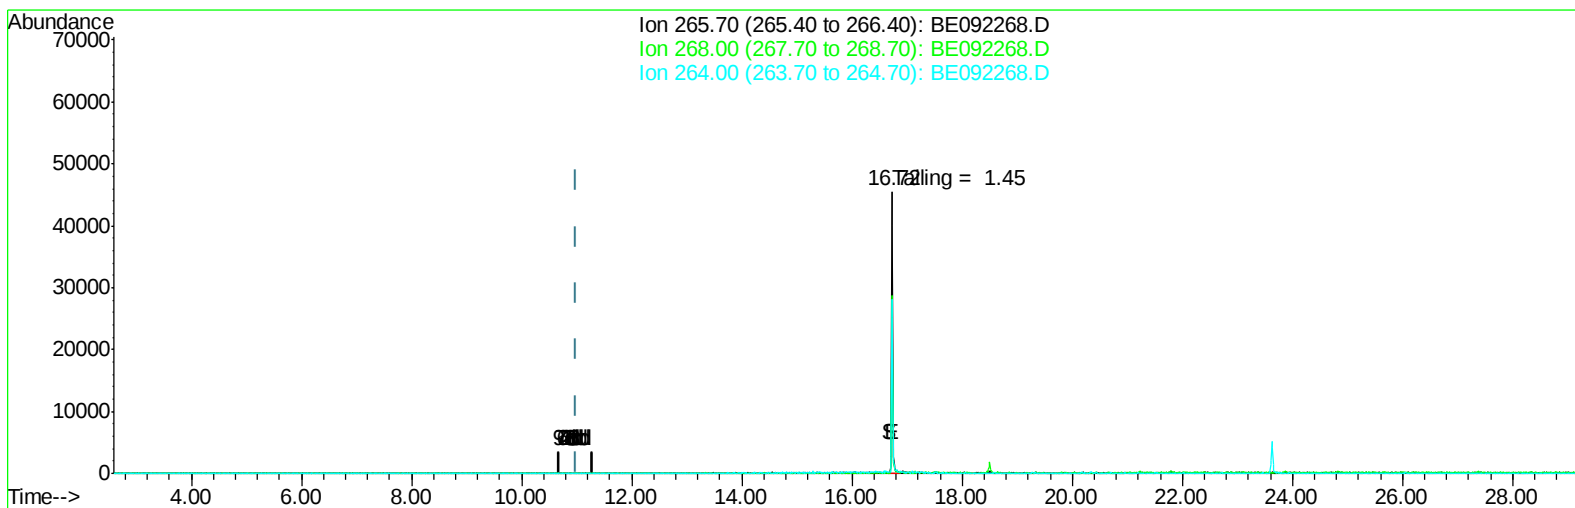

TIC: BE092268.D

(69) Pentachlorophenol (C)

10.942min (-0.063) 39.75ng

response 38

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 265.70 | 100   | 100    |
| 268.00 | 66.50 | 16.36# |
| 264.00 | 63.90 | 21.82# |
| 0.00   | 0.00  | 0.00   |