


Data Path : Z:\HPCHEM1\BNA E\Data\BE081916\
 Data File : BE092268.D
 Acq On : 19 Aug 2016 13:35
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 10 11:12:32 2016

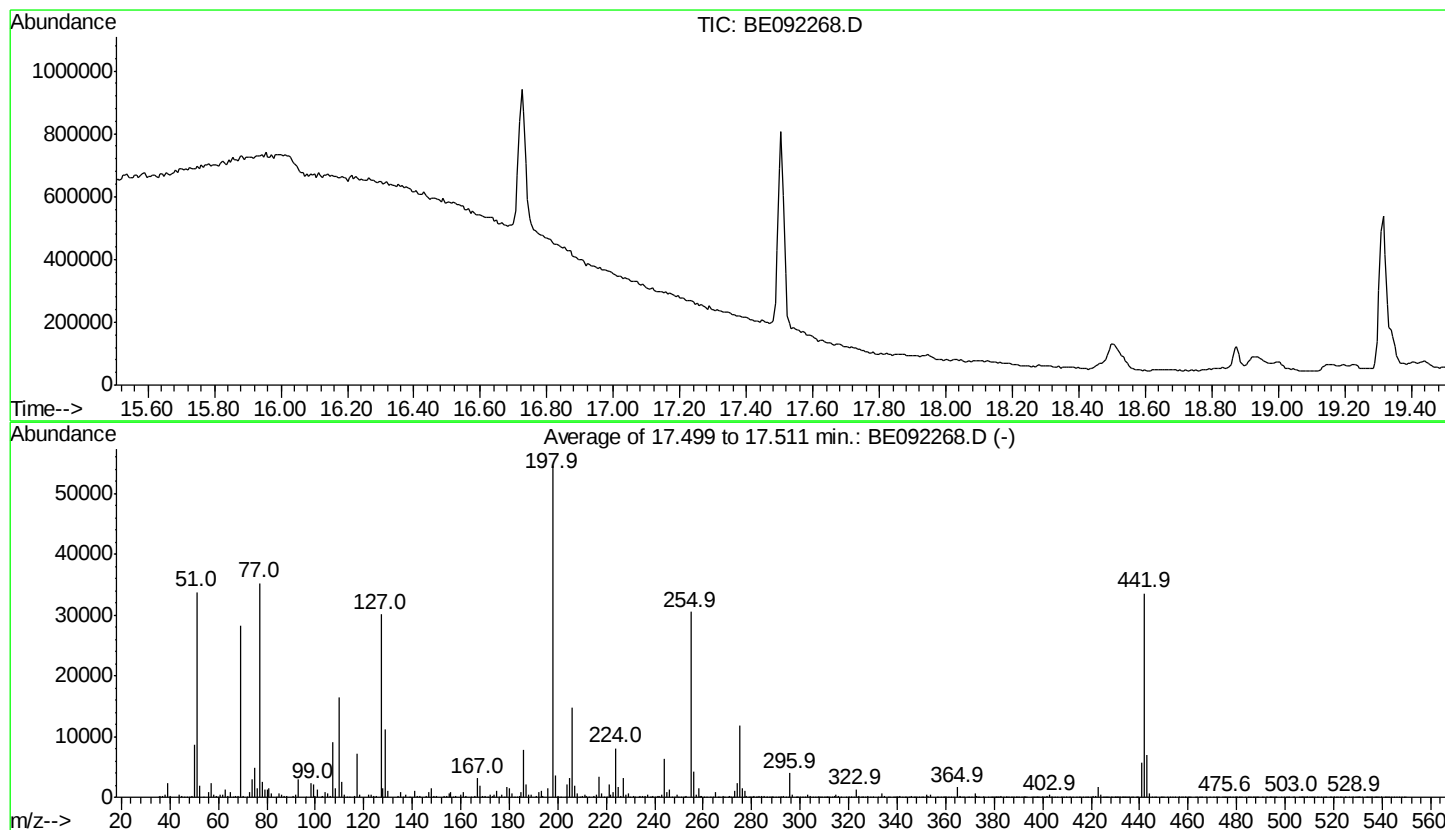

AutoFind: Scans 2538, 2539, 2540; Background Corrected with Scan 2532

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.9	33763	PASS
68	69	0.00	2	0.8	225	PASS
69	198	0.00	100	51.6	28177	PASS
70	69	0.00	2	0.9	256	PASS
127	198	10	80	55.1	30045	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54560	PASS
199	198	5	9	6.6	3581	PASS
275	198	10	60	21.5	11745	PASS
365	198	1	100	3.0	1633	PASS
441	442	0.01	24	17.0	5694	PASS
442	198	50	100	61.4	33509	PASS
443	442	15	24	20.7	6938	PASS