


Data Path : Z:\HPCHEM1\BNA_E\Data\BE082015\
 Data File : BE090570.D
 Acq On : 20 Aug 2015 11:29
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE081415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 14 16:52:42 2015

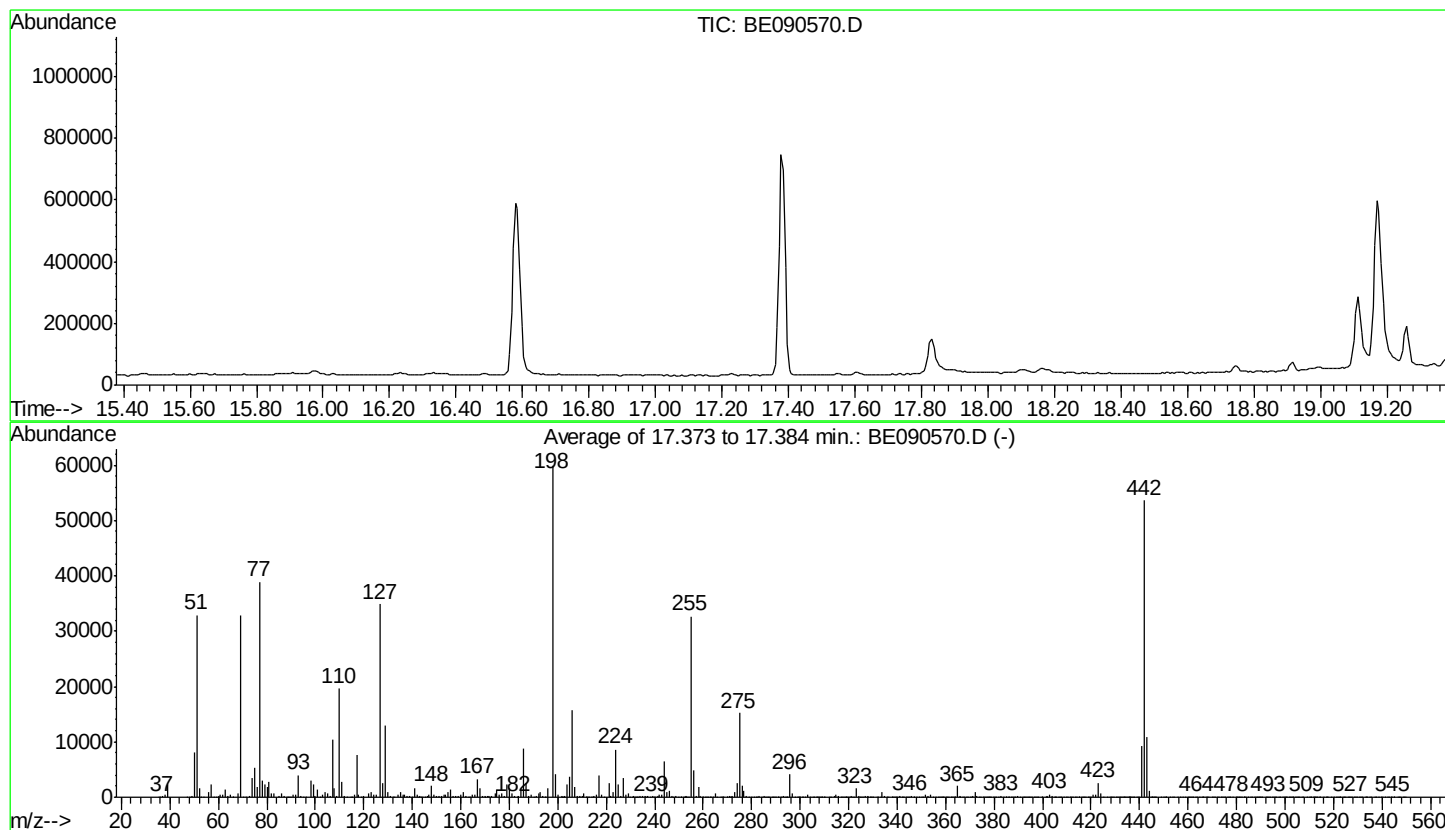

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.9	32913	PASS
68	69	0.00	2	1.8	598	PASS
69	198	0.00	100	54.9	32878	PASS
70	69	0.00	2	0.1	22	PASS
127	198	10	80	58.2	34834	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59898	PASS
199	198	5	9	7.0	4189	PASS
275	198	10	60	25.4	15199	PASS
365	198	1	100	3.4	2051	PASS
441	442	0.01	24	17.2	9218	PASS
442	198	50	100	89.5	53628	PASS
443	442	15	24	20.1	10780	PASS