


Data Path : U:\HPCHEM1\BNA E\Data\BE082217\
 Data File : BE093870.D
 Acq On : 22 Aug 2017 11:39
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 07 14:30:21 2017

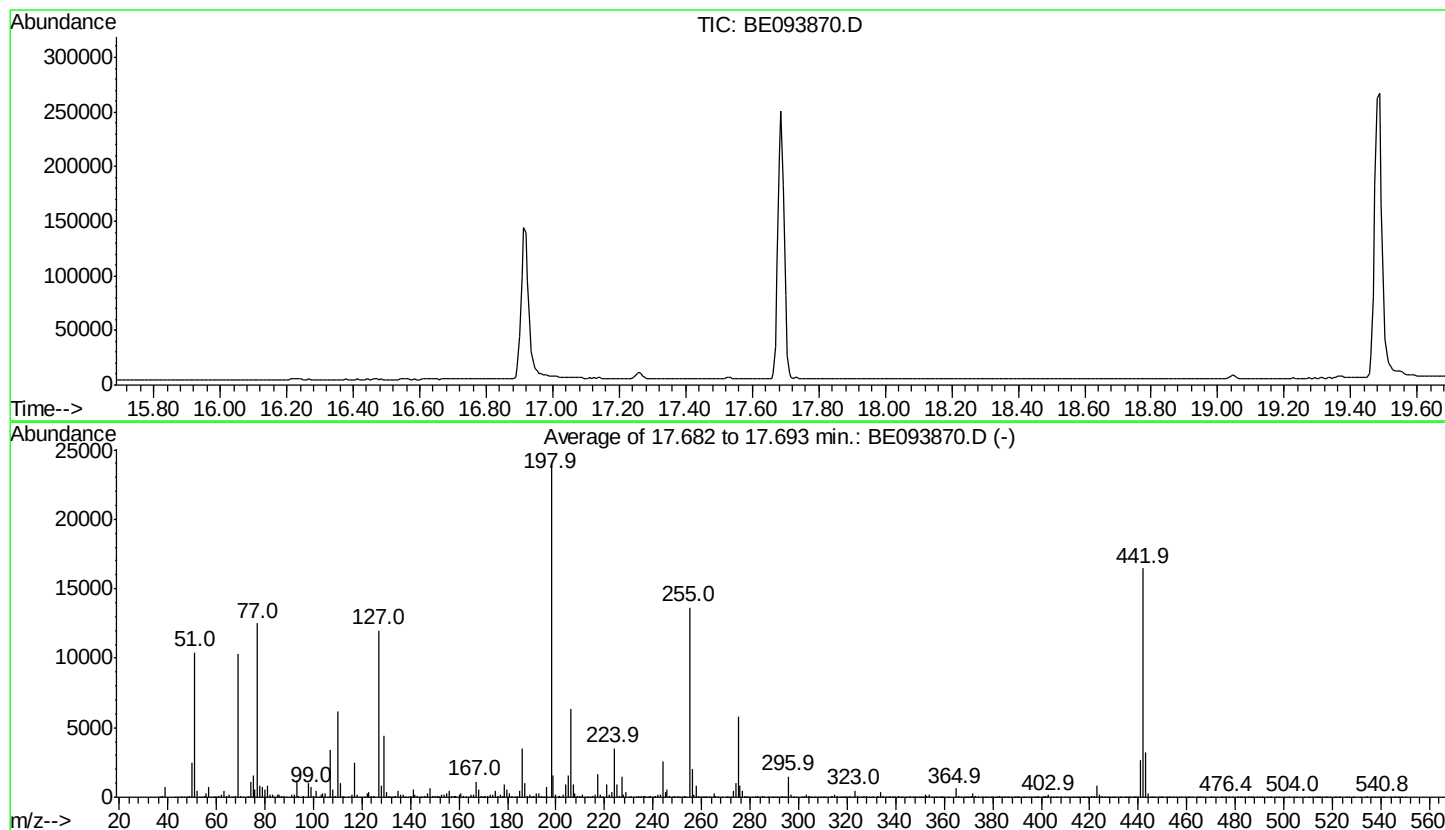

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2562

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	10418	PASS
68	69	0.00	2	1.0	99	PASS
69	198	0.00	100	43.4	10357	PASS
70	69	0.00	2	0.5	49	PASS
127	198	10	80	50.3	11988	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	23856	PASS
199	198	5	9	6.7	1604	PASS
275	198	10	60	24.5	5846	PASS
365	198	1	100	2.7	643	PASS
441	442	0.01	24	16.3	2685	PASS
442	198	50	100	68.9	16447	PASS
443	442	15	24	19.5	3207	PASS