
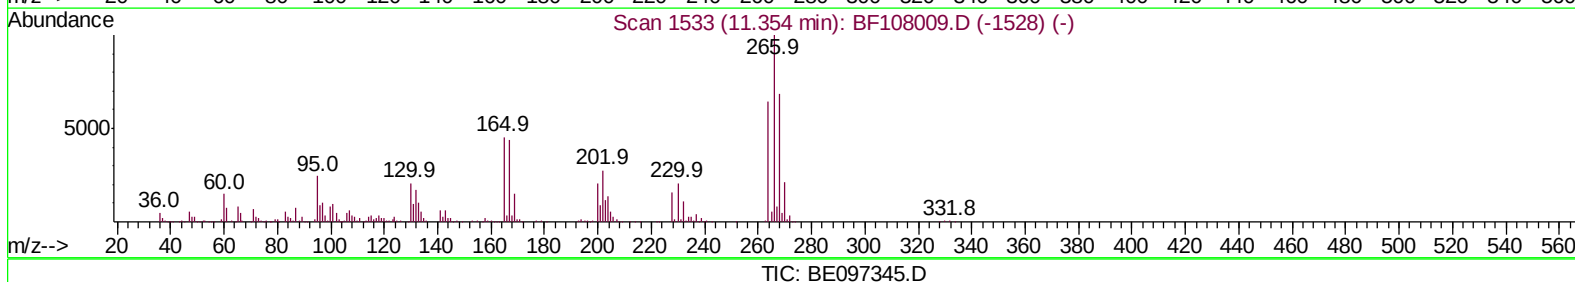
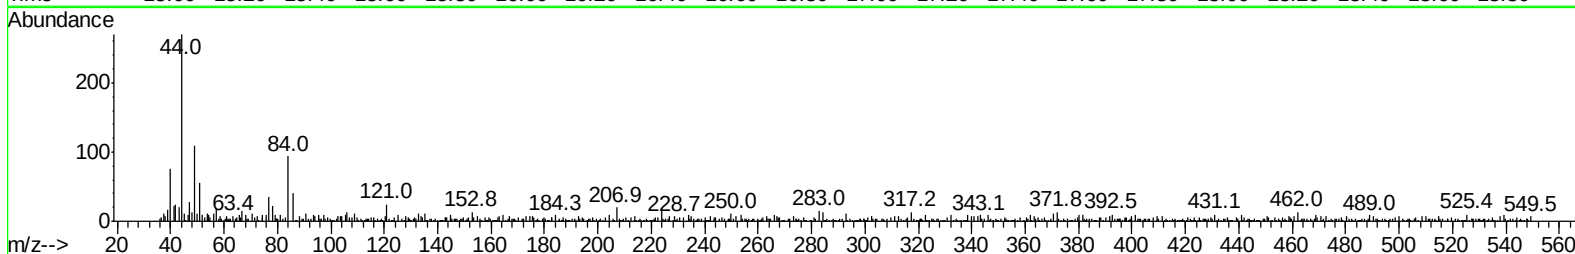


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082218\
Data File : BE097345.D
Acq On : 22 Aug 2018 13:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 01:57:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

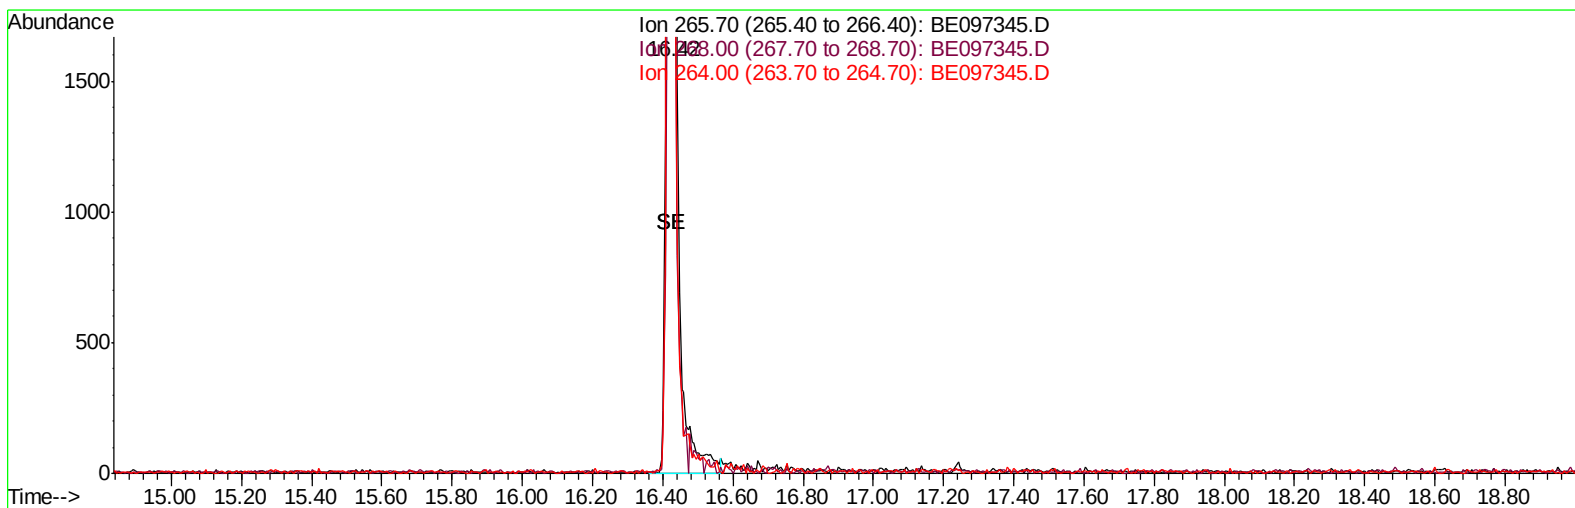

TIC: BE097345.D

(69) Pentachlorophenol (C)




11.213min (-0.135) 205.56ng

response 9

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	80.00#
264.00	61.90	90.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082218\
Data File : BE097345.D
Acq On : 22 Aug 2018 13:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 01:57:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

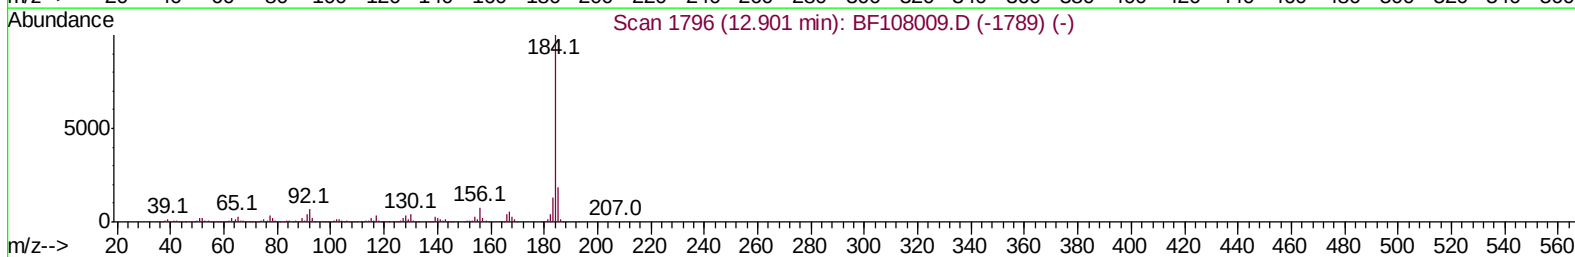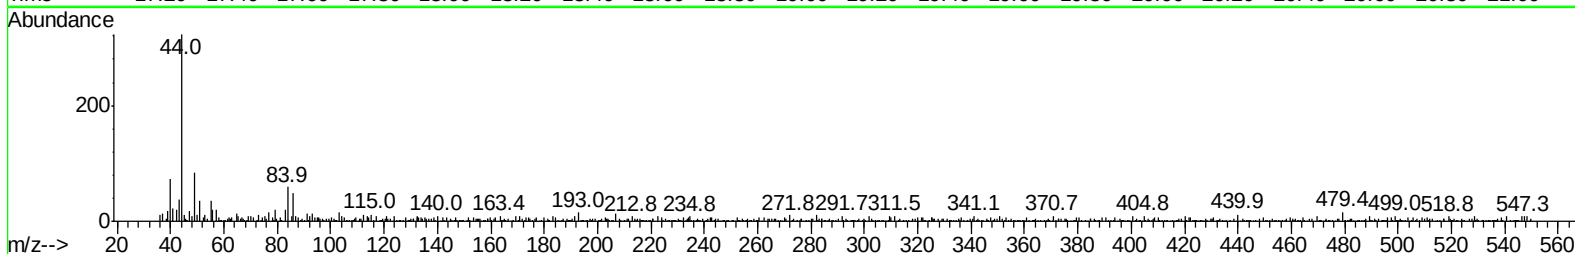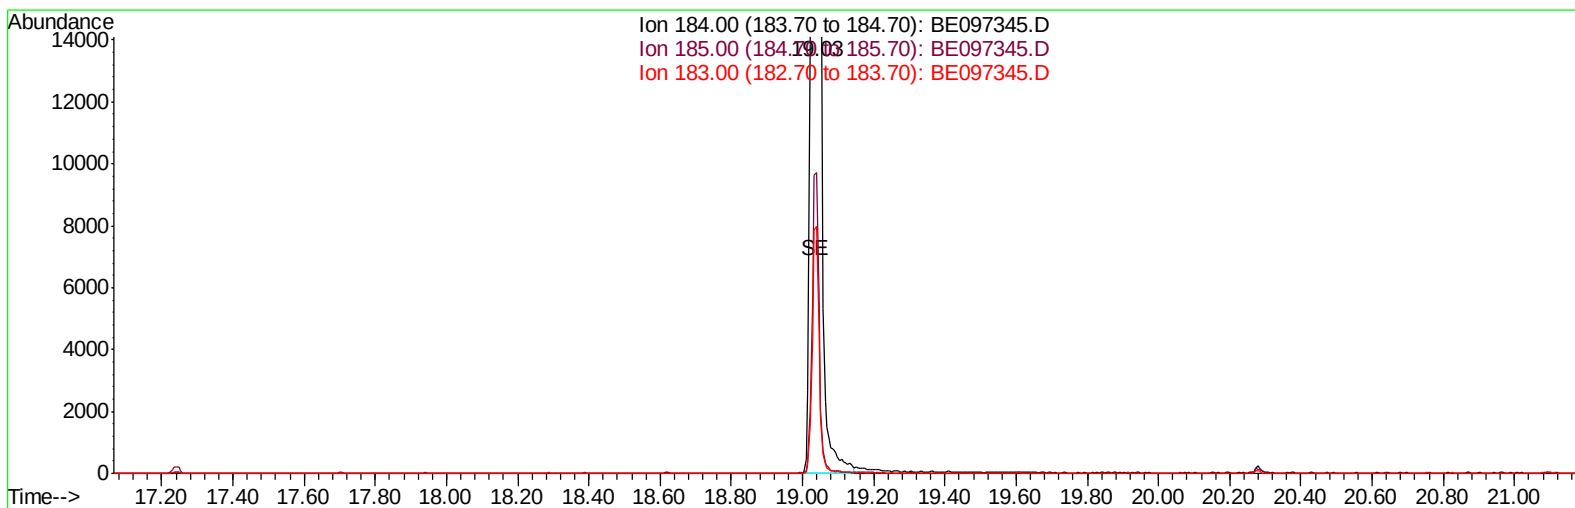

TIC: BE097345.D

(76) Benzidine

12.764min (-0.119) 1.49ng

response 1

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	42.86#
183.00	11.60	142.86#
0.00	0.00	0.00