


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE082218\
 Data File : BE097345.D
 Acq On : 22 Aug 2018 13:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE082218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 22 18:07:26 2018

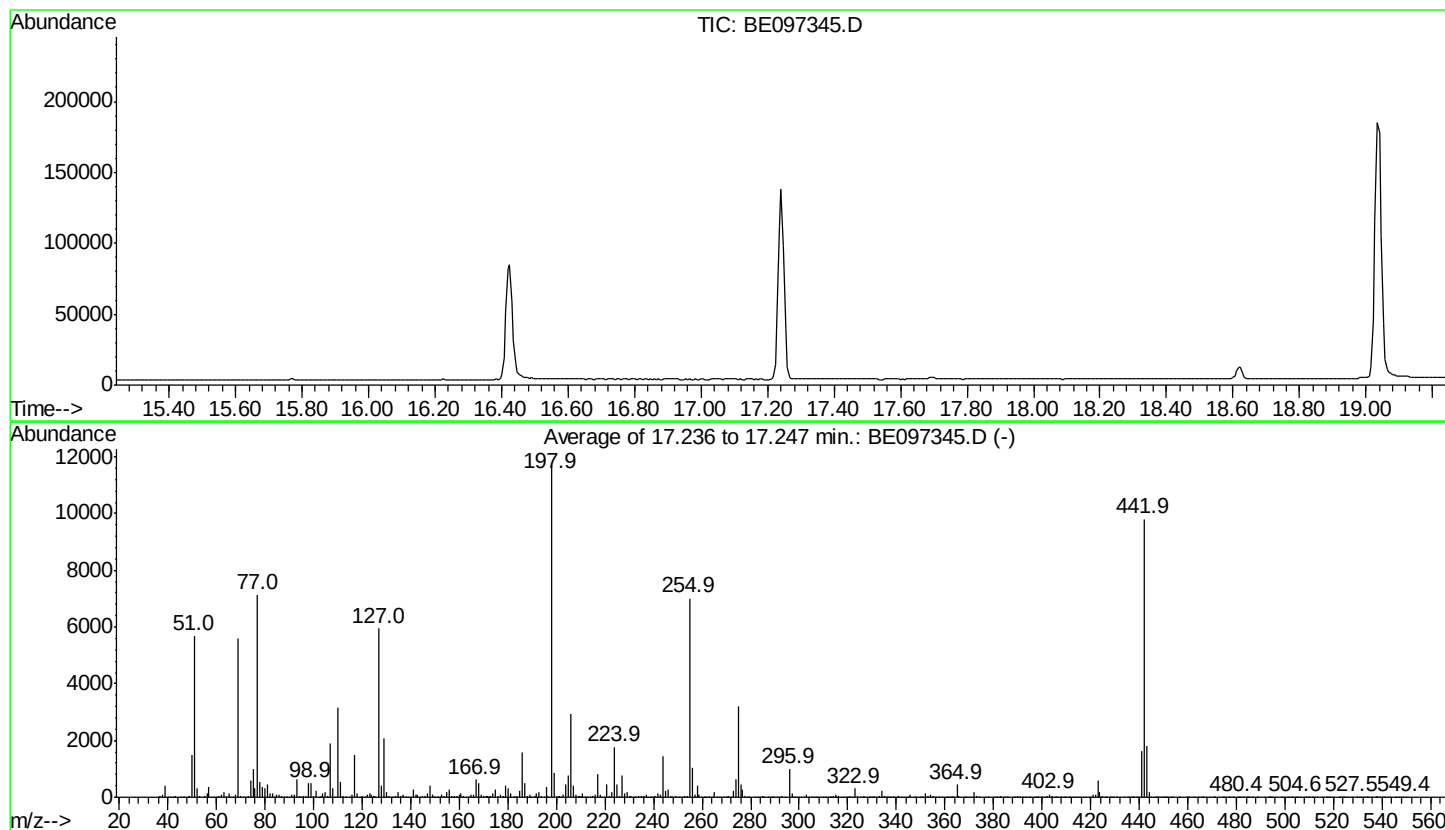

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.7	5689	PASS
68	69	0.00	2	1.9	108	PASS
69	198	0.00	100	48.1	5619	PASS
70	69	0.00	2	0.8	44	PASS
127	198	10	80	50.8	5937	PASS
197	198	0.00	2	0.3	38	PASS
198	198	100	100	100.0	11690	PASS
199	198	5	9	7.2	838	PASS
275	198	10	60	27.2	3185	PASS
365	198	1	100	3.7	437	PASS
441	198	0.01	100	13.8	1613	PASS
442	198	50	100	83.8	9802	PASS
443	442	15	24	18.2	1787	PASS