


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE082415\
 Data File : BE090596.D
 Acq On : 24 Aug 2015 9:08
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE081415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 14 16:52:42 2015

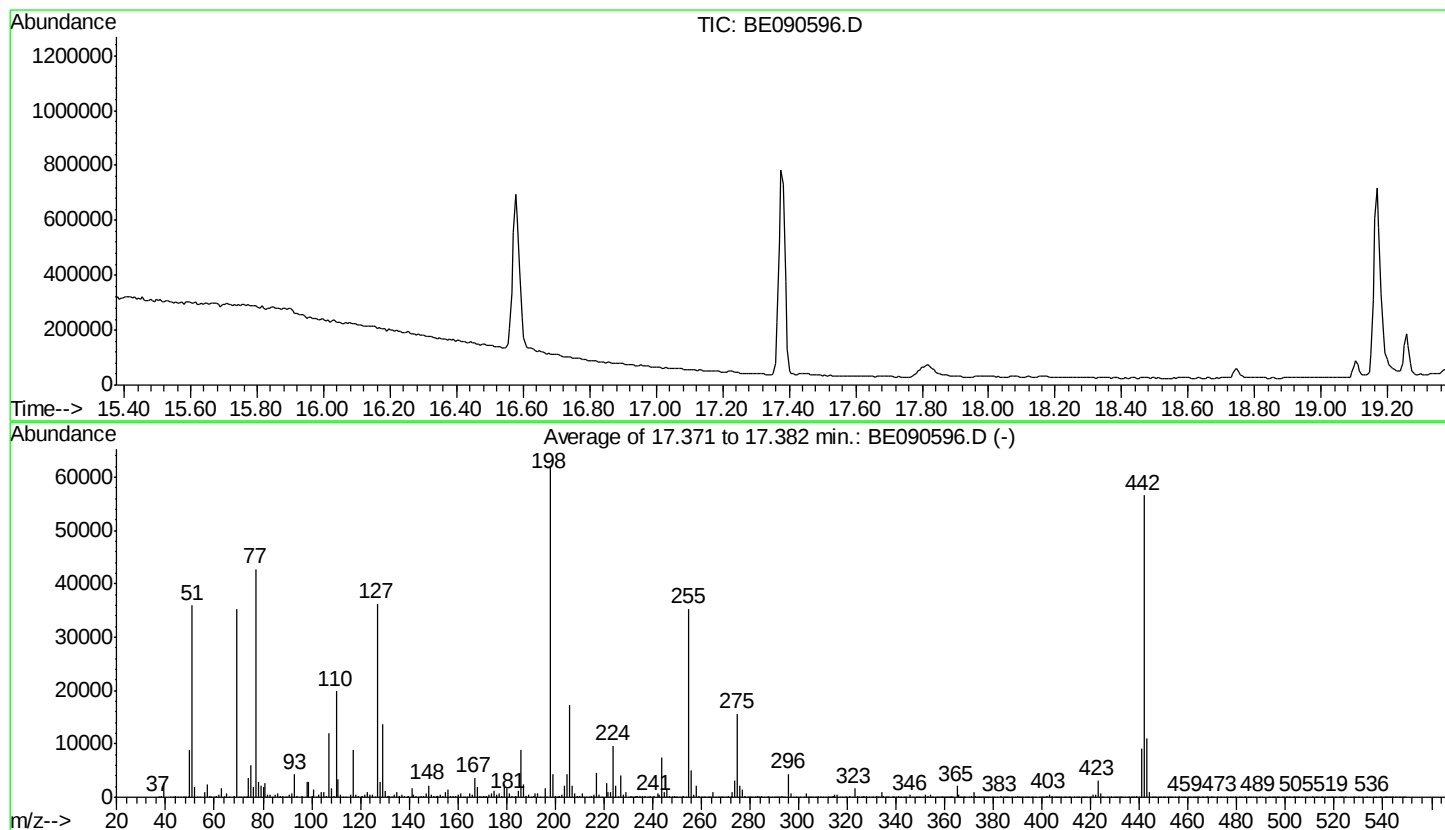

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.7	35883	PASS
68	69	0.00	2	0.9	322	PASS
69	198	0.00	100	56.7	35215	PASS
70	69	0.00	2	0.1	30	PASS
127	198	10	80	58.4	36296	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62154	PASS
199	198	5	9	7.1	4413	PASS
275	198	10	60	25.2	15670	PASS
365	198	1	100	3.4	2133	PASS
441	442	0.01	24	16.3	9219	PASS
442	198	50	100	91.0	56559	PASS
443	442	15	24	19.5	11006	PASS