

Data Path : Z:\HPCHEM1\BNA E\DATA\BE082515\
 Data File : BE090622.D
 Acq On : 25 Aug 2015 20:21
 Operator : UM/IZ
 Sample : G3401-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 26 03:28:03 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE081415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 14 16:52:42 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	14398	5.00	ng	0.00
6) Naphthalene-d8	10.34	136	62008	5.00	ng	0.00
12) Acenaphthene-d10	14.20	164	37290	5.00	ng	0.00
18) Phenanthrene-d10	16.94	188	98147	5.00	ng	0.00
25) Chrysene-d12	21.09	240	112155	5.00	ng	0.00
32) Perylene-d12	23.40	264	96216	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.21	112	10228	2.46	ng	0.00
5) Phenol-d6	6.78	99	7526	1.23	ng	0.00
7) Nitrobenzene-d5	8.74	82	17100	3.46	ng	0.01
13) 2,4,6-Tribromophenol	15.71	330	13379	9.32	ng	0.00
14) 2-Fluorobiphenyl	12.83	172	39546	3.55	ng	0.01
27) Terphenyl-d14	19.55	244	90726	4.42	ng	0.00
Target Compounds						
21) Pentachlorophenol	16.61	266	4	0.30	ng	Qvalue # 67
30) Bis(2-ethylhexyl)phthalate	21.02	149	1794	0.24	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE082515\
Data File : BE090622.D
Acq On : 25 Aug 2015 20:21
Operator : UM/IZ
Sample : G3401-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 26 03:28:03 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE081415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 14 16:52:42 2015
Response via : Initial Calibration

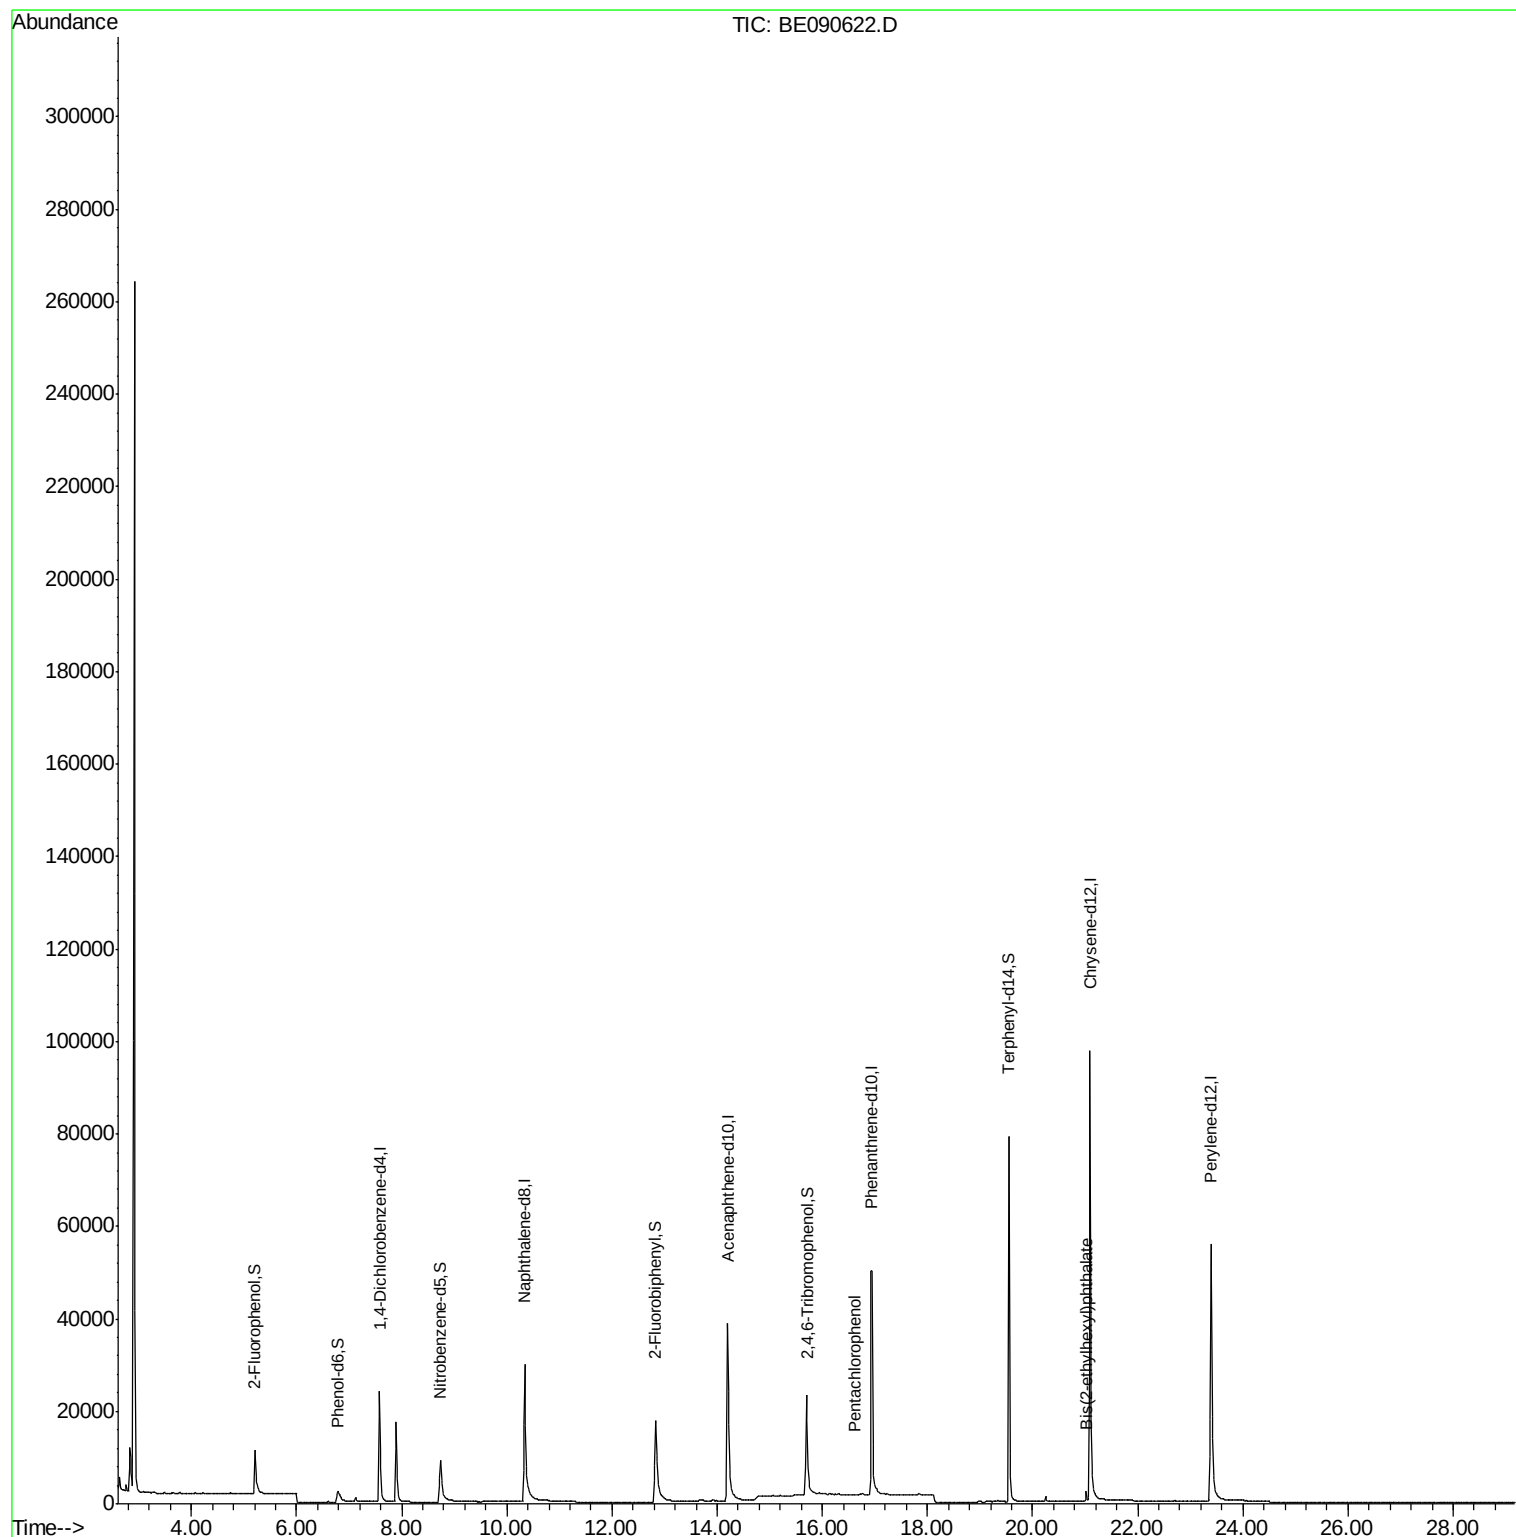

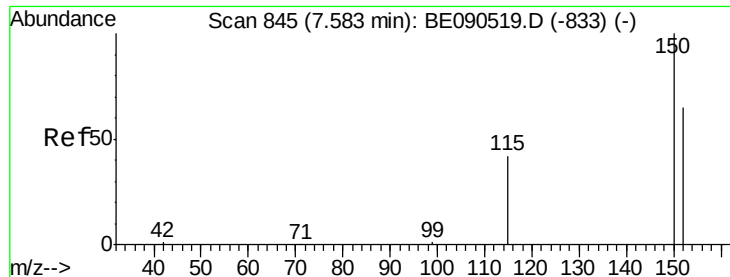

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.58 min Scan# 844

Delta R.T. -0.00 min

Lab File: BE090622.D

Acq: 25 Aug 2015 20:21

Instrument :

BNA_E

ClientSampleId :


Tot Ion:152 Resp: 14398

Ion Ratio Lower Upper

152 100

150 155.7 123.0 184.4




115 67.4 48.9 73.3

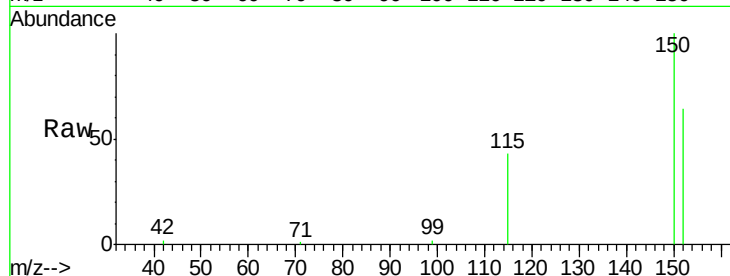

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

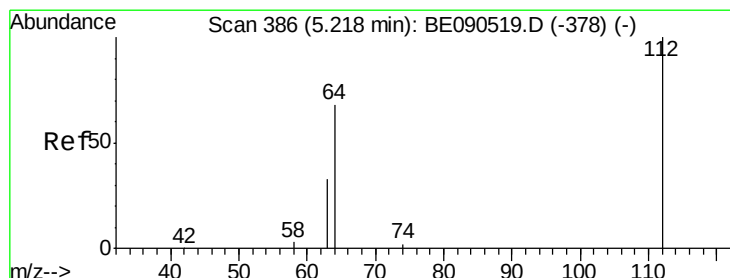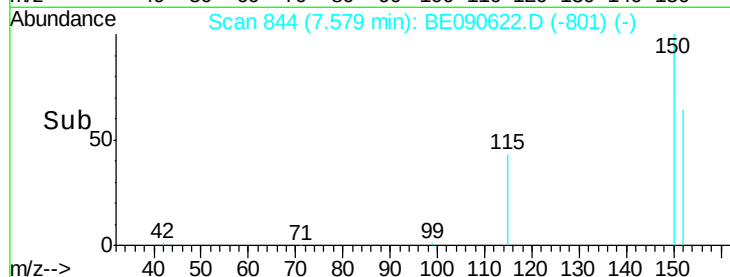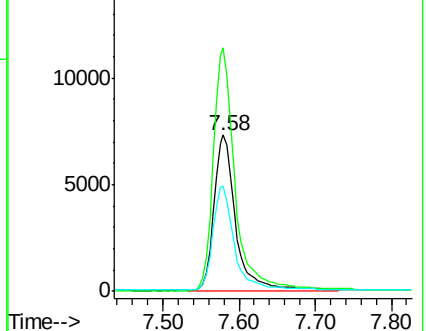

#4

2-Fluorophenol

Concen: 2.46 ng

RT: 5.21 min Scan# 385

Delta R.T. -0.01 min

Lab File: BE090622.D

Acq: 25 Aug 2015 20:21


Tgt Ion:112 Resp: 10228

Ion Ratio Lower Upper

112 100

64 69.6 37.1 55.7#



63 35.9 19.5 29.3#

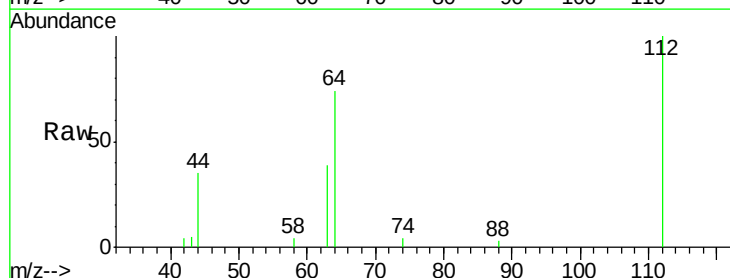


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

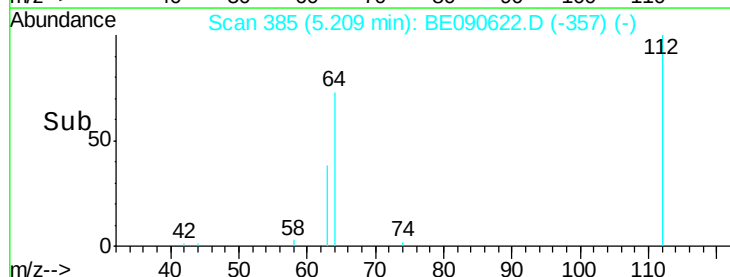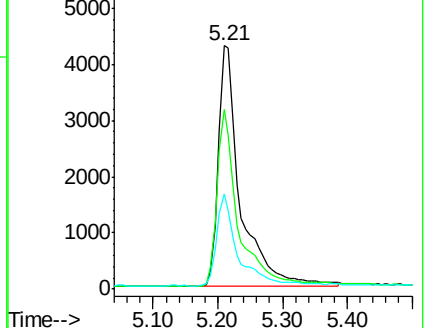

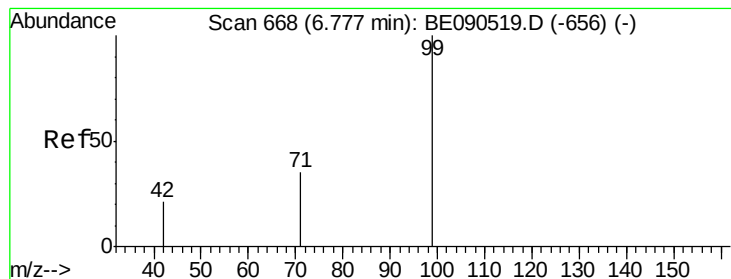

#5

Phenol-d6

Concen: 1.23 ng

RT: 6.78 min Scan# 668

Delta R.T. 0.00 min

Lab File: BE090622.D

Acq: 25 Aug 2015 20:21

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 99 Resp: 7526

Ion Ratio Lower Upper




99 100

42 20.1 18.2 27.4

71 34.8 27.4 41.0



Abundance Ion 99.00 (98.70 to 99.70): BE0
Ion 42.00 (41.70 to 42.70): BE0
Ion 71.00 (70.70 to 71.70): BE0

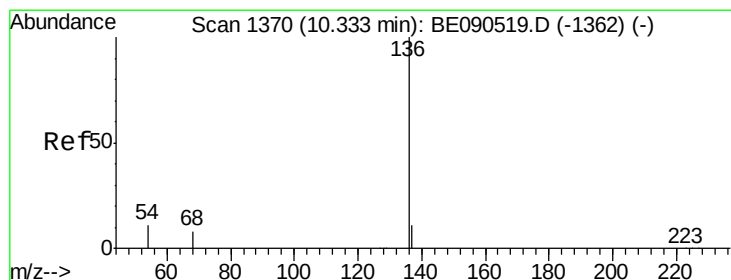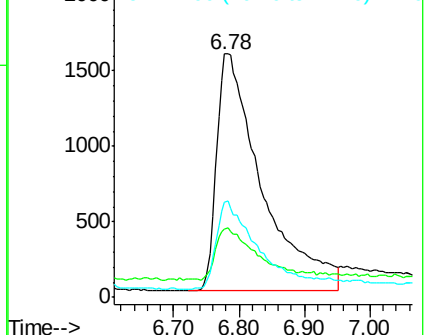

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.34 min Scan# 1371

Delta R.T. 0.01 min

Lab File: BE090622.D

Acq: 25 Aug 2015 20:21

Tgt Ion: 136 Resp: 62008


Ion Ratio Lower Upper

136 100



137 11.2 8.7 13.1


54 10.4 9.4 14.0

68 7.9 6.5 9.7



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BE0
Ion 68.00 (67.70 to 68.70): BE0

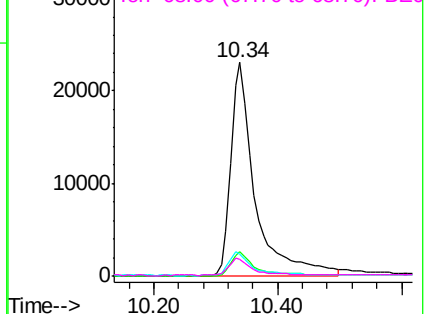

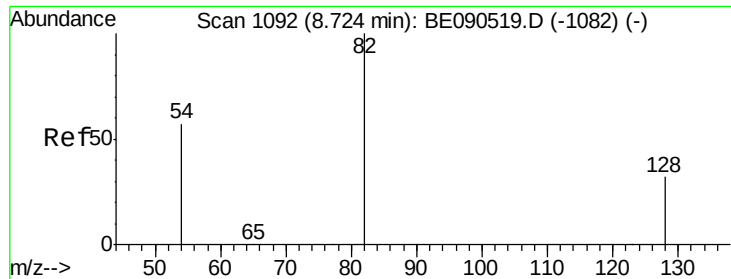

#7

Nitrobenzene-d5

Concen: 3.46 ng

RT: 8.74 min Scan# 1095

Delta R.T. 0.01 min

Lab File: BE090622.D

Acq: 25 Aug 2015 20:21

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 82 Resp: 17100

Ion Ratio Lower Upper

82 100

128 31.9 25.0 37.6




54 58.3 48.8 73.2



Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

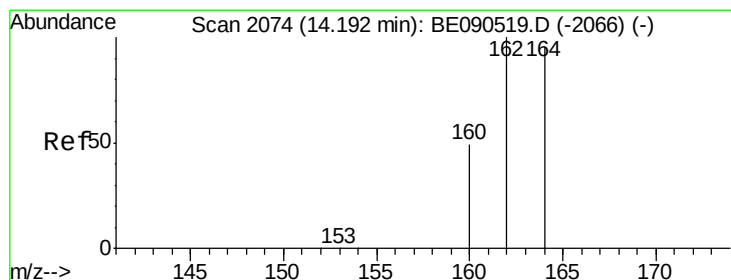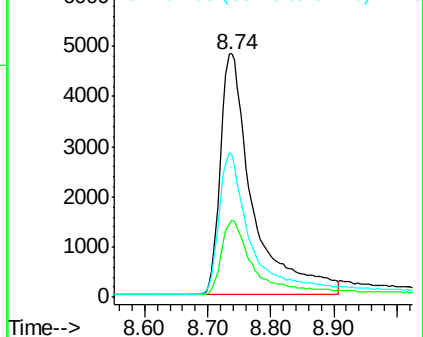

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.20 min Scan# 2075

Delta R.T. 0.01 min

Lab File: BE090622.D

Acq: 25 Aug 2015 20:21


Tgt Ion: 164 Resp: 37290

Ion Ratio Lower Upper

164 100

162 103.5 81.8 122.8



160 54.8 44.2 66.4




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

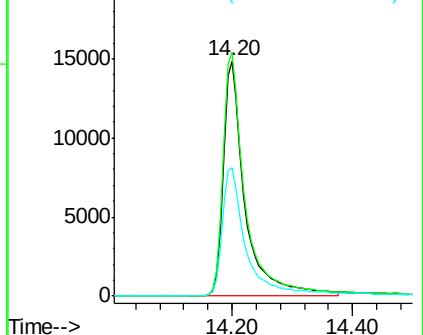







#13
 2,4,6-Tribromophenol
 Concen: 9.32 ng
 RT: 15.71 min Scan# 2206
 Delta R.T. -0.00 min
 Lab File: BE090622.D
 Acq: 25 Aug 2015 20:21

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:330 Resp: 13379
 Ion Ratio Lower Upper
 330 100
 332 96.5 75.8 113.6
 141 173.0 114.4 171.6#

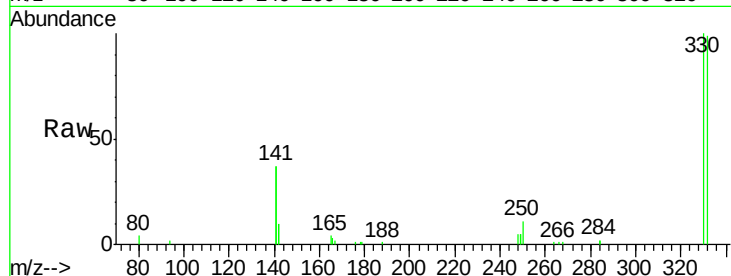


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


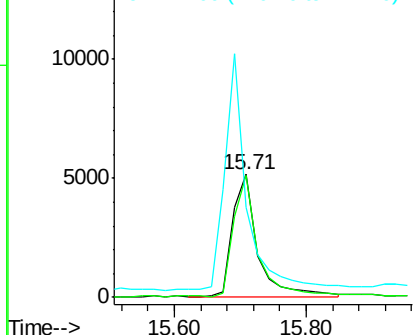



#14
 2-Fluorobiphenyl
 Concen: 3.55 ng
 RT: 12.83 min Scan# 1830
 Delta R.T. 0.01 min
 Lab File: BE090622.D
 Acq: 25 Aug 2015 20:21

Tgt Ion:172 Resp: 39546
 Ion Ratio Lower Upper
 172 100
 171 34.4 28.5 42.7
 170 23.7 19.8 29.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

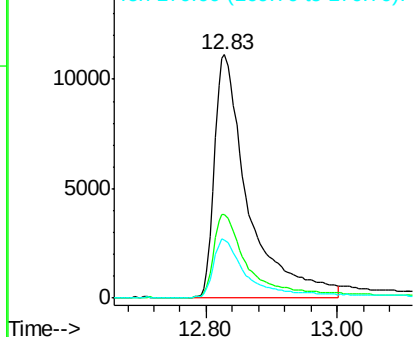



#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.94 min Scan# 2277

Delta R.T. -0.00 min

Lab File: BE090622.D

Acq: 25 Aug 2015 20:21

Instrument :

BNA_E

ClientSampled :


Tot Ion:188 Resp: 98147

Ion Ratio Lower Upper

188 100

94 7.0 5.7 8.5




80 7.3 5.8 8.8

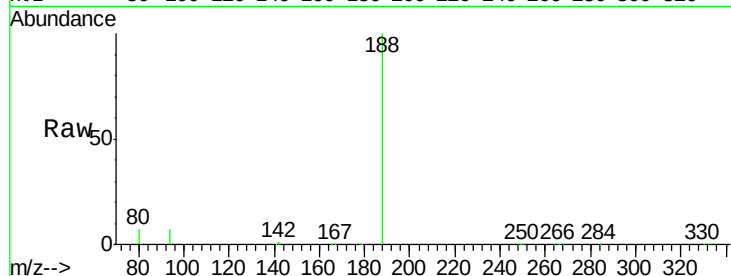

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

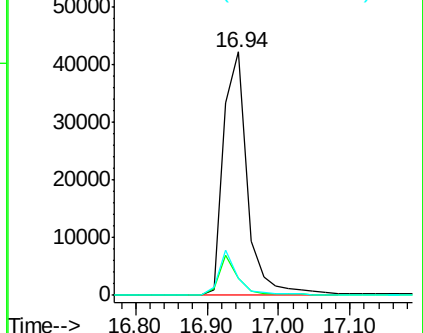

#21

Pentachlorophenol

Concen: 0.30 ng

RT: 16.61 min Scan# 2258

Delta R.T. -0.00 min

Lab File: BE090622.D

Acq: 25 Aug 2015 20:21


Tgt Ion:266 Resp: 4

Ion Ratio Lower Upper

266 100

268 102.1 58.5 87.7#



264 95.8 56.0 84.0#




Abundance Ion 265.70 (265.40 to 266.40): E

Ion 268.00 (267.70 to 268.70): E

Ion 264.00 (263.70 to 264.70): E

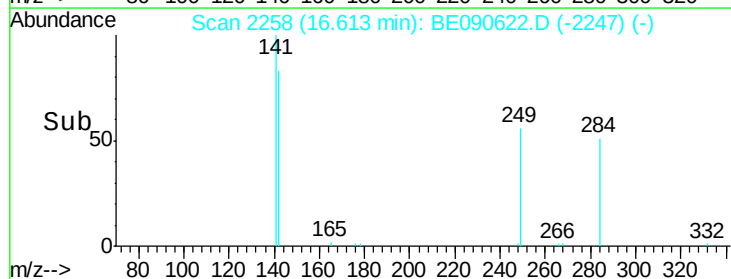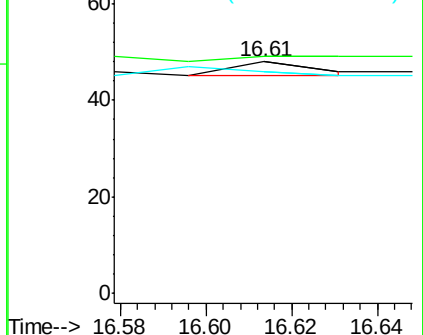

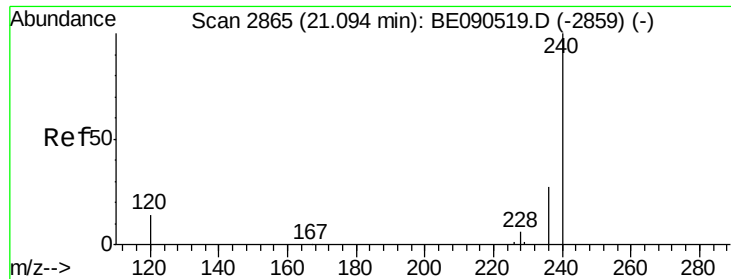

#25

Chrysene-d12

Concen: 5.00 ng

RT: 21.09 min Scan# 2864

Delta R.T. 0.00 min

Lab File: BE090622.D

Acq: 25 Aug 2015 20:21

Instrument :

BNA_E

ClientSampleId :


Tot Ion:240 Resp: 112155

Ion Ratio Lower Upper

240 100

120 13.4 8.3 12.5#




236 26.8 21.0 31.4

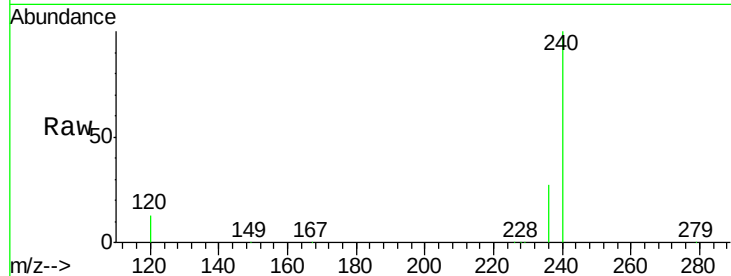

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

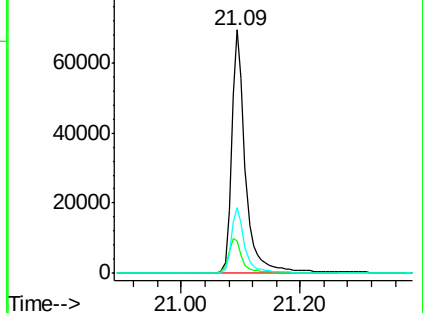

#27

Terphenyl-d14

Concen: 4.42 ng

RT: 19.55 min Scan# 2613

Delta R.T. 0.00 min

Lab File: BE090622.D

Acq: 25 Aug 2015 20:21


Tgt Ion:244 Resp: 90726

Ion Ratio Lower Upper

244 100

212 7.8 6.6 9.8



122 12.1 10.2 15.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

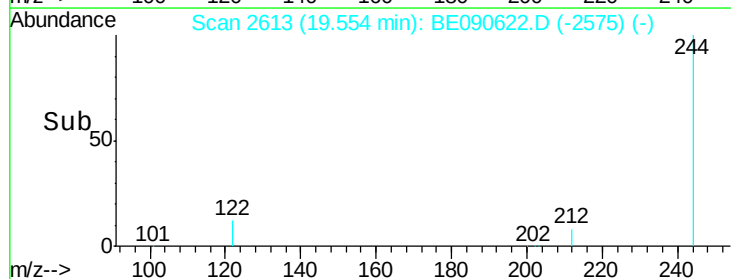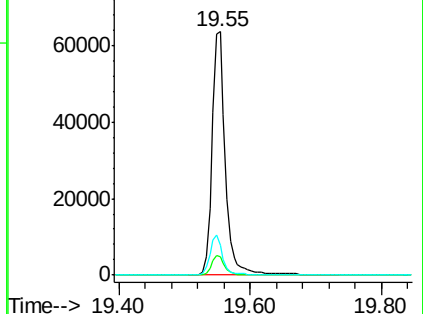


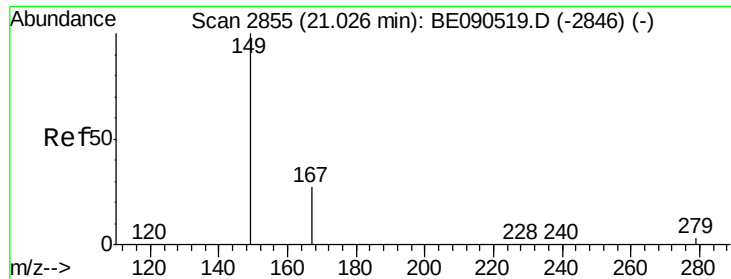




#30
 Bis(2-ethylhexyl)phthalate
 Concen: 0.24 ng
 RT: 21.02 min Scan# 2853
 Delta R.T. -0.01 min
 Lab File: BE090622.D
 Acq: 25 Aug 2015 20:21

Instrument :
 BNA_E
 ClientSampled :

Tot Ion:149 Resp: 1794
 Ion Ratio Lower Upper
 149 100
 167 26.0 19.8 29.8
 279 3.4 2.4 3.6

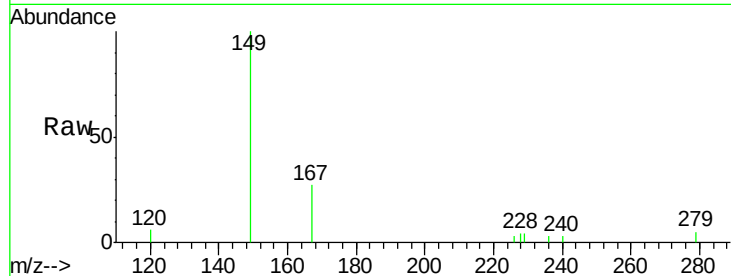


Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E

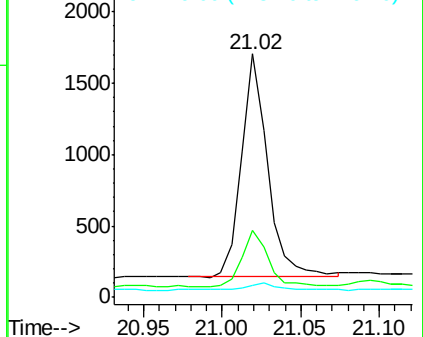

#32
 Perylene-d12
 Concen: 5.00 ng
 RT: 23.40 min Scan# 3307
 Delta R.T. 0.00 min
 Lab File: BE090622.D
 Acq: 25 Aug 2015 20:21

Tgt Ion:264 Resp: 96216
 Ion Ratio Lower Upper
 264 100
 260 24.7 20.1 30.1
 265 21.9 17.2 25.8

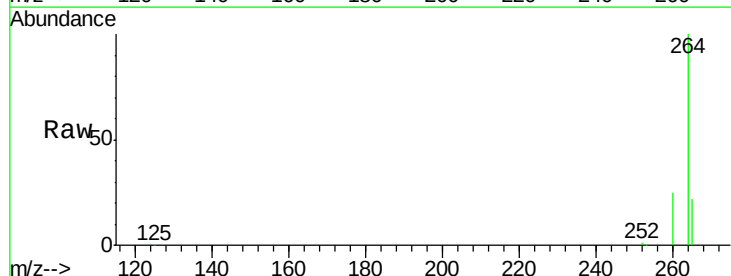

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

