


Data Path : Z:\HPCHEM1\BNA_E\Data\BE082515\
 Data File : BE090626.D
 Acq On : 25 Aug 2015 22:47
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE081415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 14 16:52:42 2015

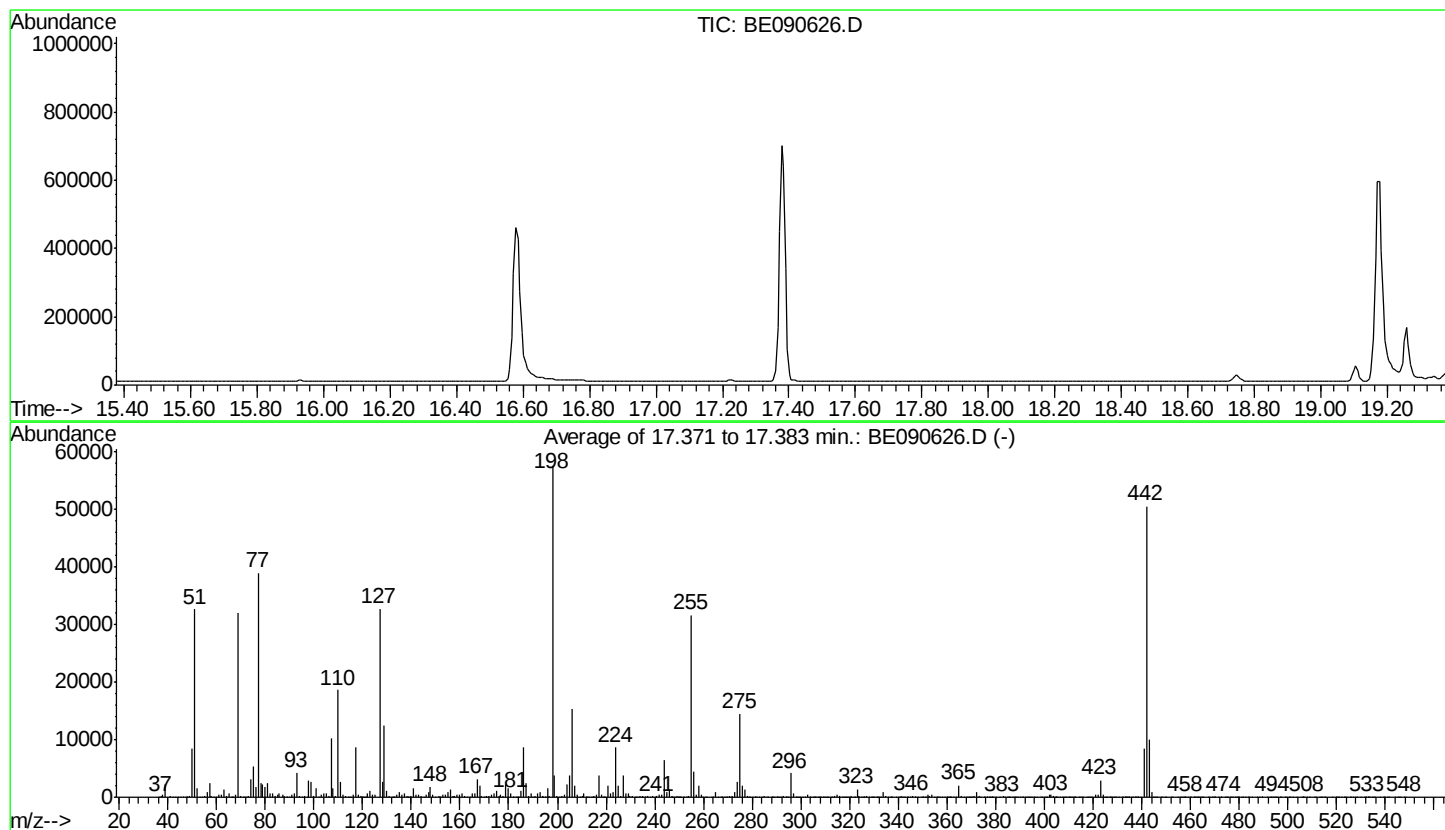

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.7	32654	PASS
68	69	0.00	2	1.2	387	PASS
69	198	0.00	100	55.7	32104	PASS
70	69	0.00	2	0.8	245	PASS
127	198	10	80	56.8	32733	PASS
197	198	0.00	2	0.3	169	PASS
198	198	100	100	100.0	57635	PASS
199	198	5	9	6.7	3842	PASS
275	198	10	60	25.2	14533	PASS
365	198	1	100	3.6	2093	PASS
441	442	0.01	24	16.5	8353	PASS
442	198	50	100	87.8	50601	PASS
443	442	15	24	19.8	9998	PASS