


Data Path : Z:\HPCHEM1\BNA E\DATA\BE082615\
Data File : BE090634.D
Acq On : 26 Aug 2015 11:16
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE081415.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 14 16:52:42 2015

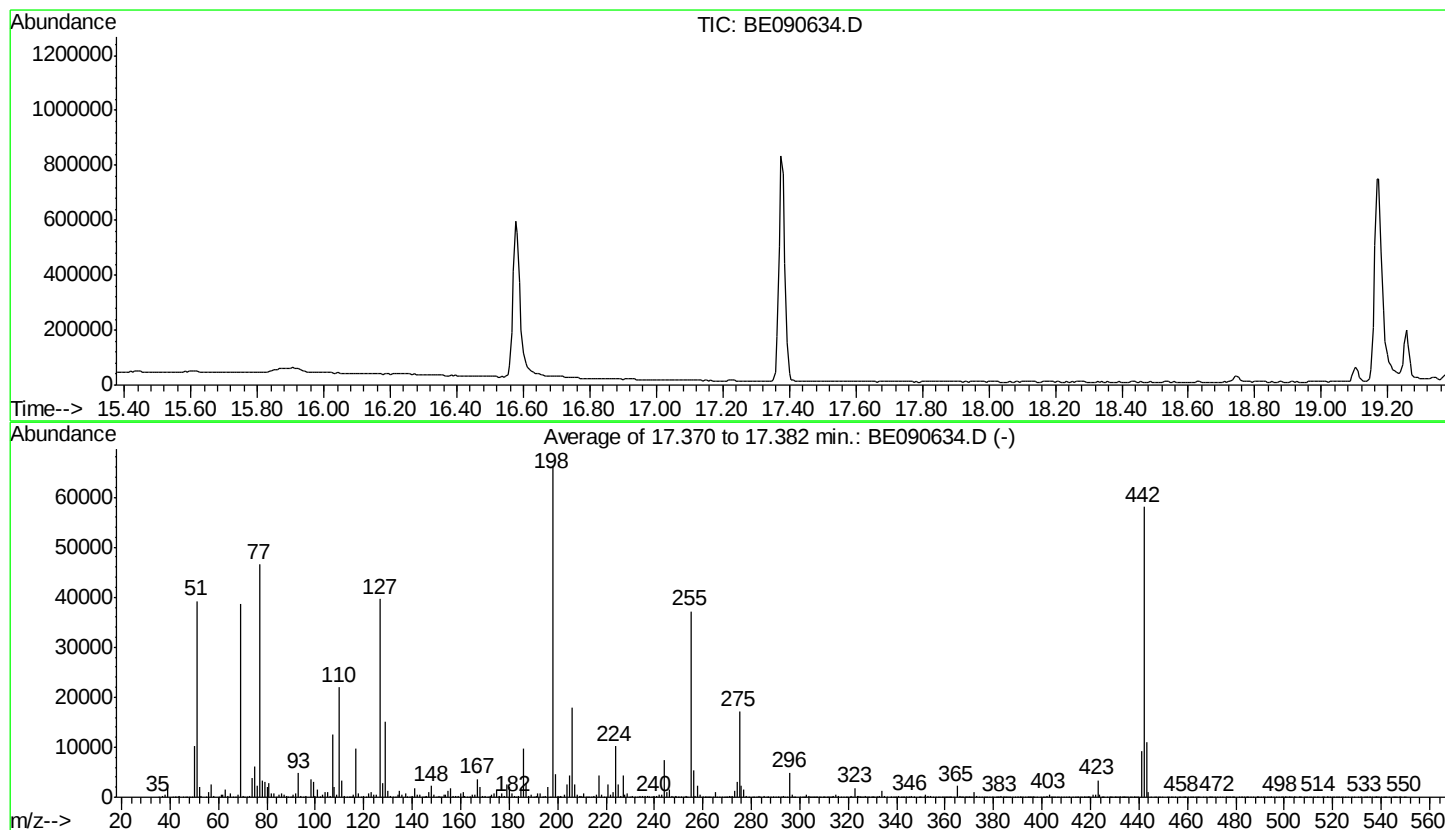

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.1	39201	PASS
68	69	0.00	2	1.3	488	PASS
69	198	0.00	100	58.4	38719	PASS
70	69	0.00	2	0.4	139	PASS
127	198	10	80	59.7	39604	PASS
197	198	0.00	2	0.1	60	PASS
198	198	100	100	100.0	66292	PASS
199	198	5	9	6.8	4519	PASS
275	198	10	60	25.7	17048	PASS
365	198	1	100	3.4	2235	PASS
441	442	0.01	24	15.7	9140	PASS
442	198	50	100	87.6	58048	PASS
443	442	15	24	19.1	11091	PASS