
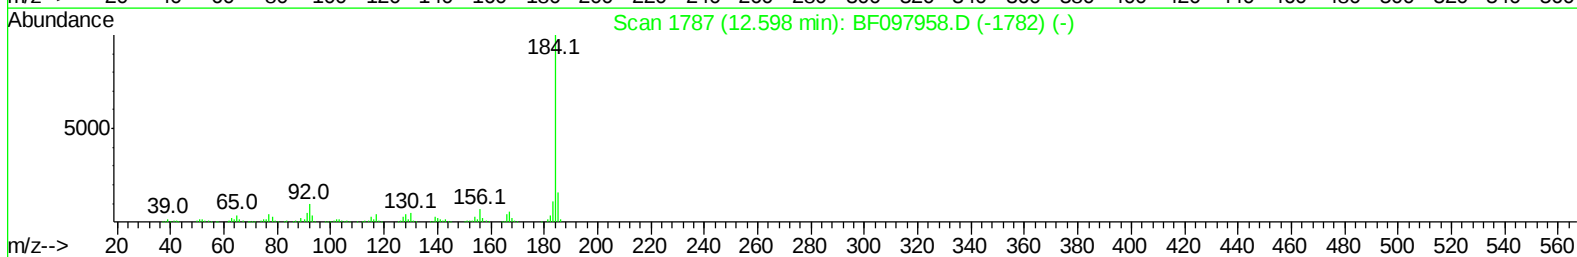
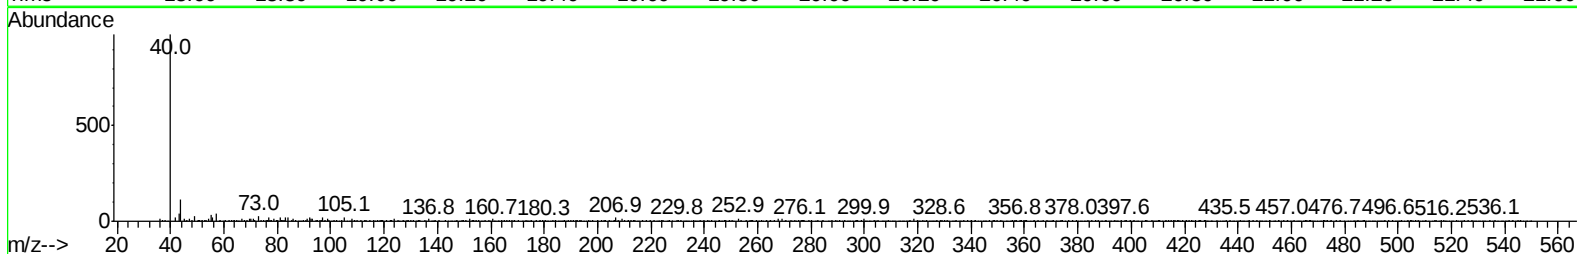


Data Path : Z:\HPCHEM1\BNA E\DATA\BE082617\
Data File : BE093880.D
Acq On : 26 Aug 2017 8:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 04:37:11 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

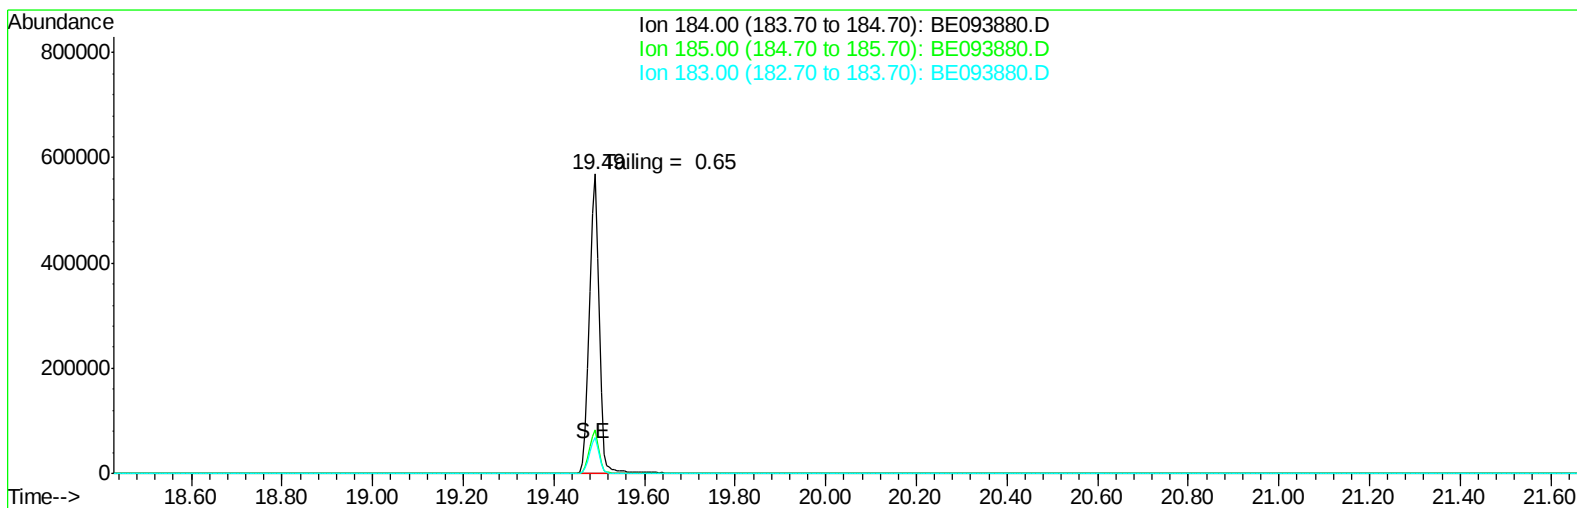

TIC: BE093880.D

(76) Benzidine




12.489min (-0.109) 54.90ng

response 18

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	40.00#
183.00	12.20	60.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE082617\
Data File : BE093880.D
Acq On : 26 Aug 2017 8:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 04:37:11 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

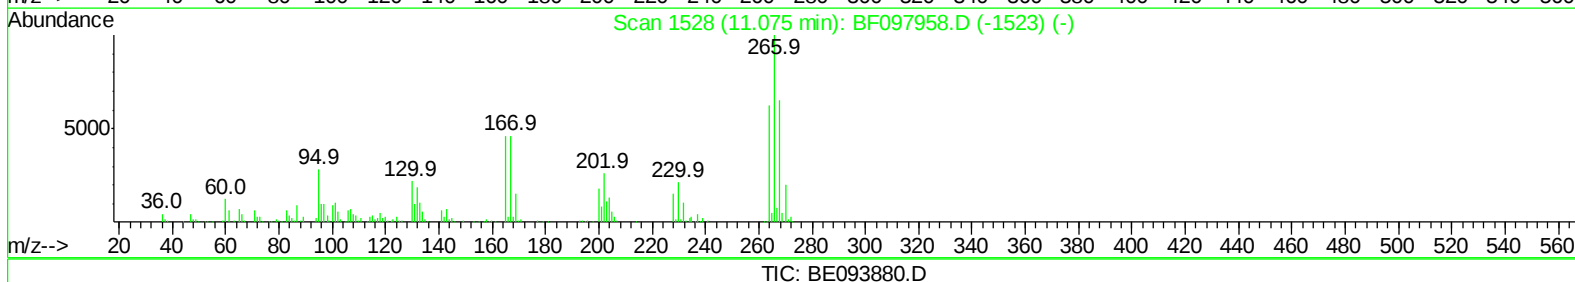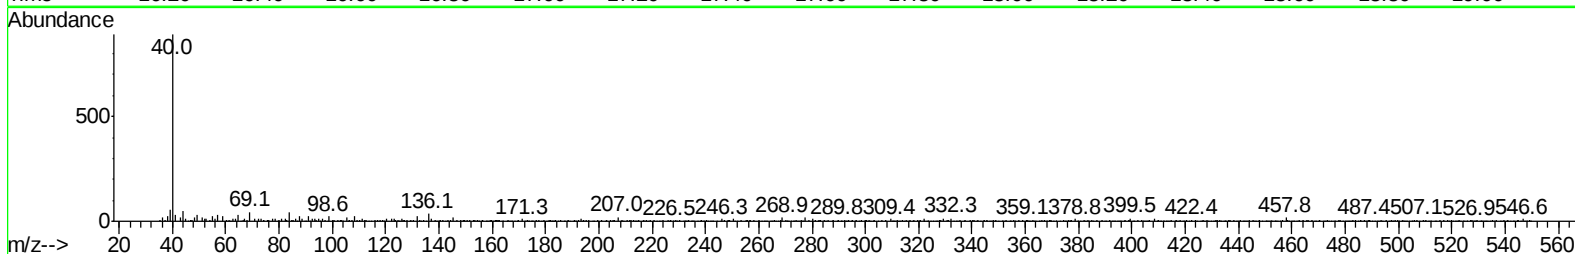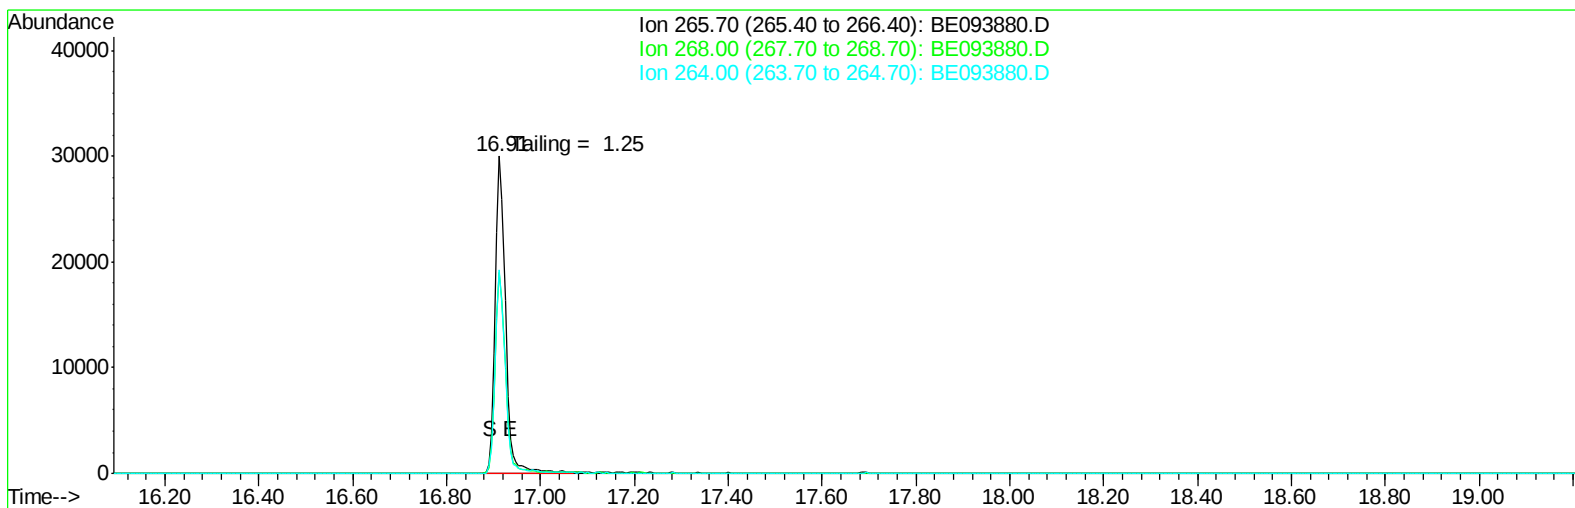

(69) Pentachlorophenol (C)
10.973min (-0.096) 243.06ng
response 12

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	75.00
264.00	64.60	37.50#
0.00	0.00	0.00