


Data Path : Z:\HPCHEM1\BNA_E\Data\BE082617\
 Data File : BE093880.D
 Acq On : 26 Aug 2017 8:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE082617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 28 11:26:07 2017

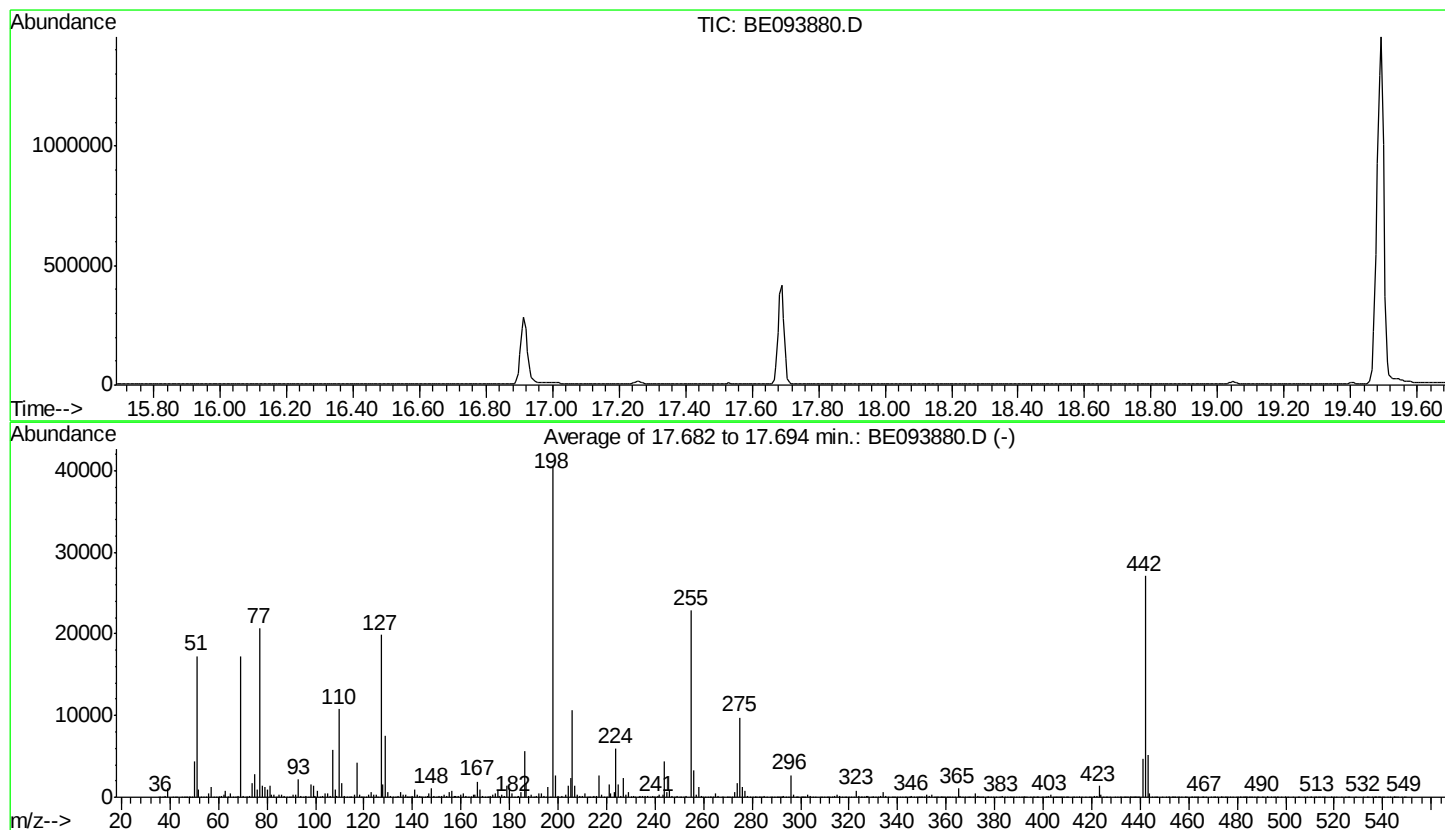

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	17308	PASS
68	69	0.00	2	0.6	112	PASS
69	198	0.00	100	42.6	17296	PASS
70	69	0.00	2	0.6	106	PASS
127	198	10	80	48.9	19844	PASS
197	198	0.00	2	0.1	55	PASS
198	198	100	100	100.0	40611	PASS
199	198	5	9	6.6	2664	PASS
275	198	10	60	24.1	9775	PASS
365	198	1	100	2.7	1085	PASS
441	442	0.01	24	17.2	4650	PASS
442	198	50	100	66.7	27092	PASS
443	442	15	24	19.1	5176	PASS