


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE082715\
Data File : BE090646.D
Acq On : 27 Aug 2015 11:41
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE081415.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 14 16:52:42 2015

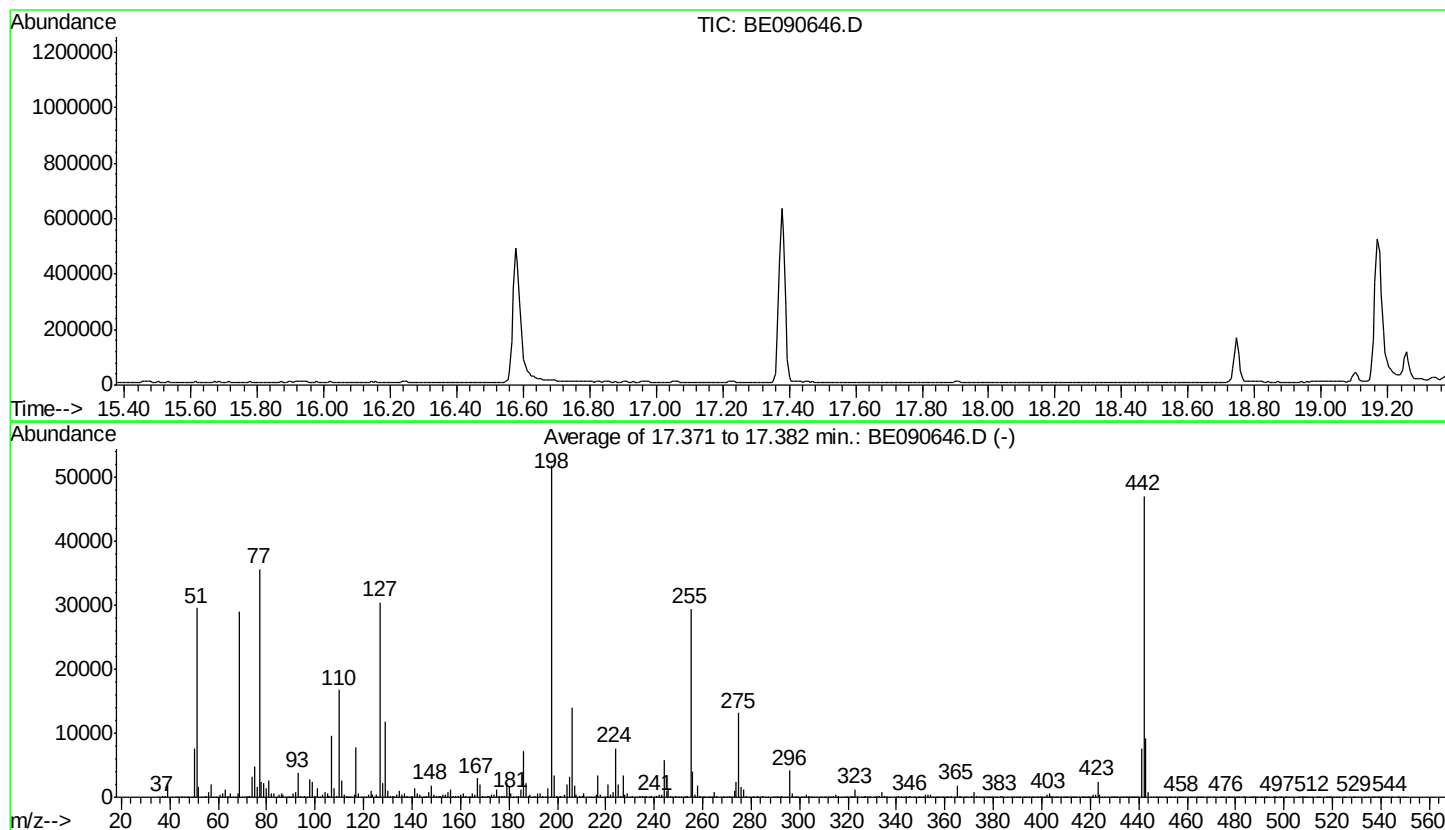

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.0	29503	PASS
68	69	0.00	2	1.9	542	PASS
69	198	0.00	100	56.0	29006	PASS
70	69	0.00	2	0.3	99	PASS
127	198	10	80	58.9	30480	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51773	PASS
199	198	5	9	6.8	3496	PASS
275	198	10	60	25.4	13169	PASS
365	198	1	100	3.5	1835	PASS
441	442	0.01	24	16.2	7627	PASS
442	198	50	100	90.8	46994	PASS
443	442	15	24	19.6	9209	PASS