
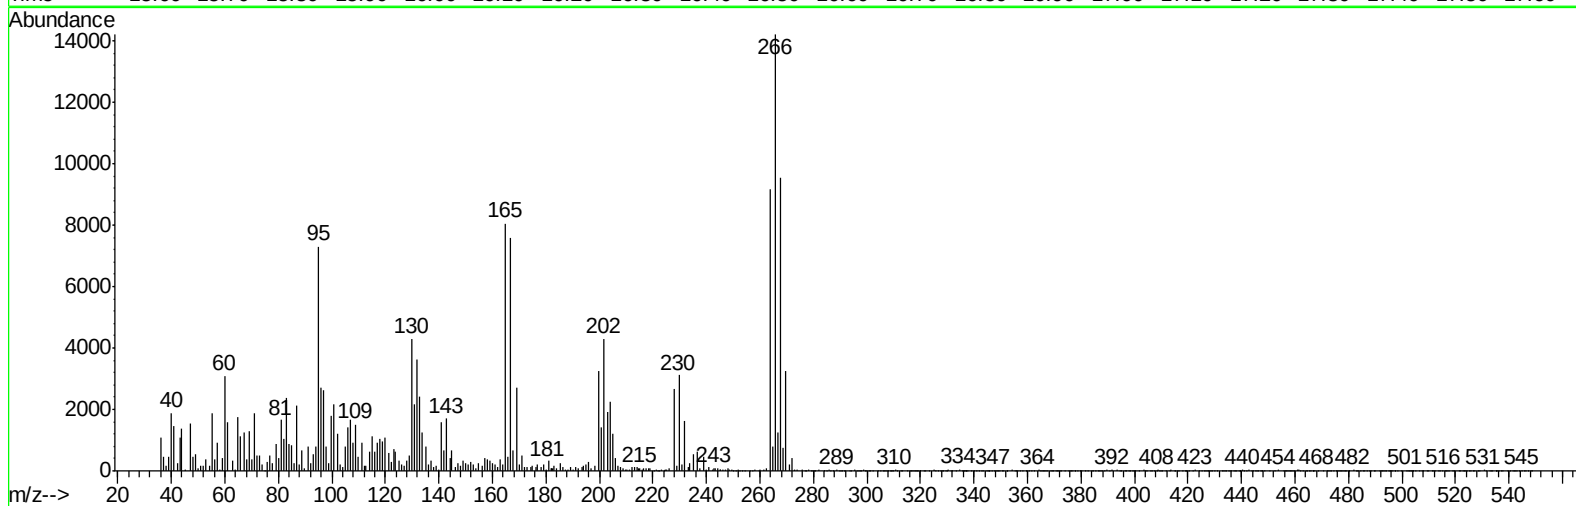


Data Path : Z:\HPCHEM1\BNA E\DATA\BE082815\
Data File : BE090655.D
Acq On : 28 Aug 2015 10:25
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 05:27:45 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE081415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 14 16:52:42 2015
Response via : Initial Calibration

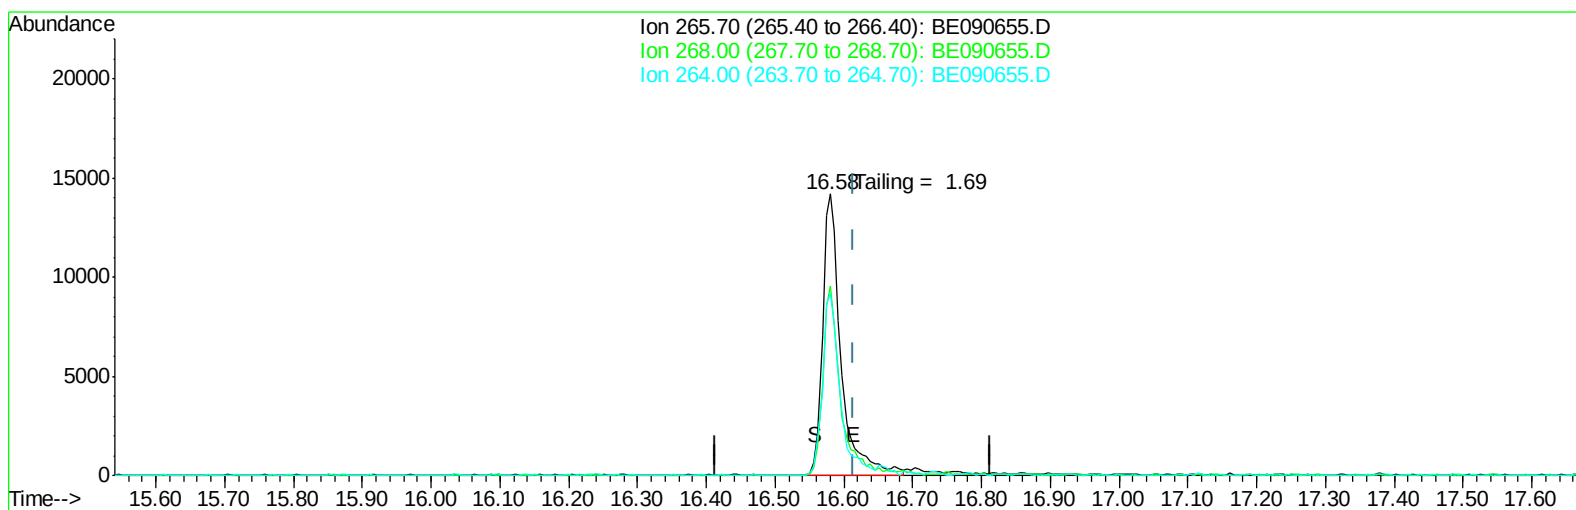

TIC: BE090655.D

(21) Pentachlorophenol

16.580min (-0.034) 7047.89ng

response 26206

Ion	Exp%	Act%
265.70	100	100
268.00	73.10	67.27
264.00	70.00	64.49
0.00	0.00	0.00