


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE082815\
Data File : BE090655.D
Acq On : 28 Aug 2015 10:25
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE081415.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 14 16:52:42 2015

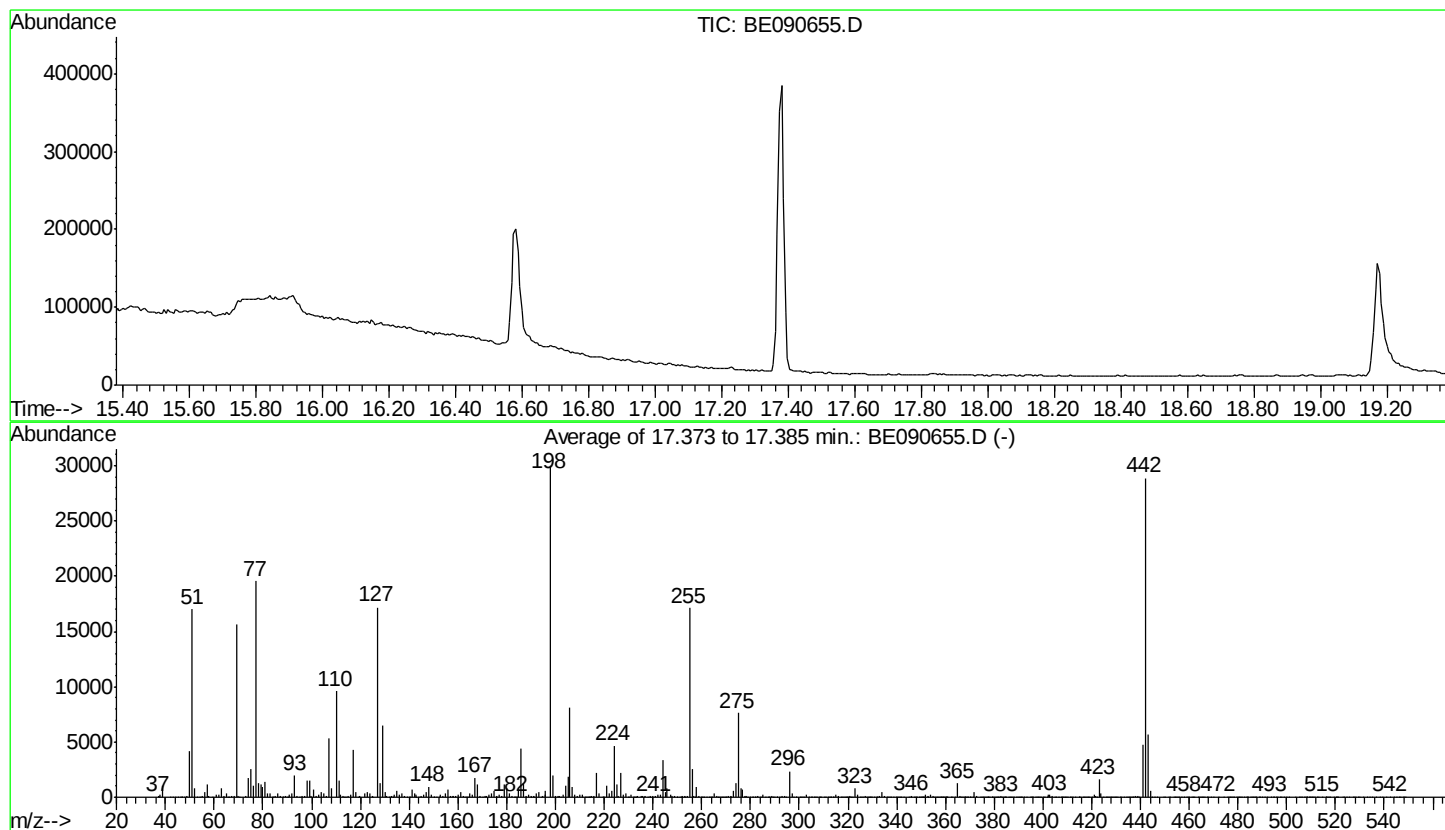

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.7	16997	PASS
68	69	0.00	2	1.0	163	PASS
69	198	0.00	100	52.3	15683	PASS
70	69	0.00	2	0.5	76	PASS
127	198	10	80	57.1	17140	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	30000	PASS
199	198	5	9	6.6	1988	PASS
275	198	10	60	25.4	7606	PASS
365	198	1	100	4.1	1220	PASS
441	442	0.01	24	16.6	4795	PASS
442	198	50	100	96.2	28866	PASS
443	442	15	24	19.8	5719	PASS