


Data Path : Z:\HPCHEM1\BNA_E\Data\BE082817\
 Data File : BE093888.D
 Acq On : 28 Aug 2017 8:48
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE082617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 28 11:26:07 2017

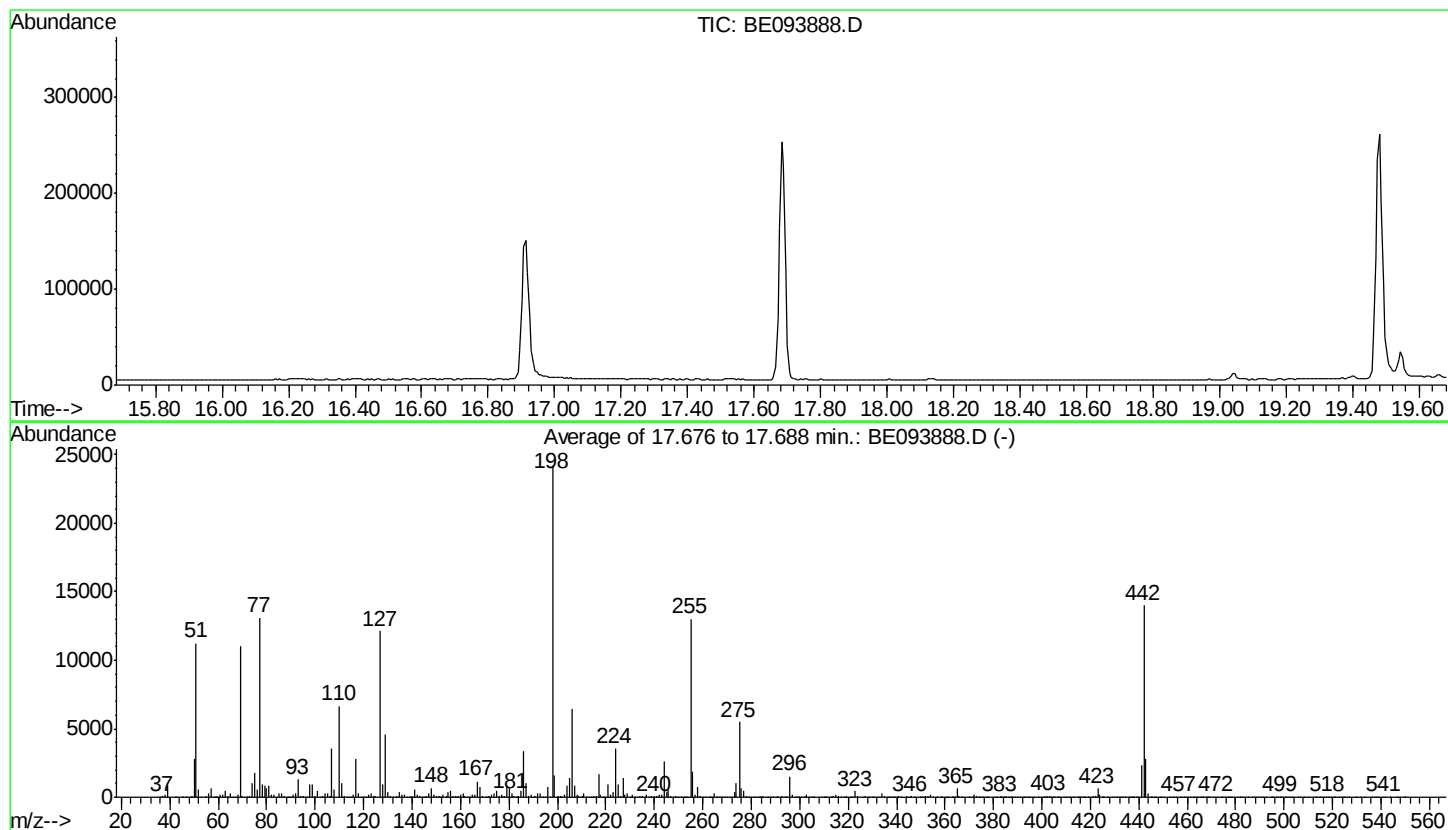

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	11243	PASS
68	69	0.00	2	1.3	149	PASS
69	198	0.00	100	45.6	11038	PASS
70	69	0.00	2	0.5	54	PASS
127	198	10	80	50.0	12105	PASS
197	198	0.00	2	0.2	40	PASS
198	198	100	100	100.0	24205	PASS
199	198	5	9	6.7	1613	PASS
275	198	10	60	22.7	5495	PASS
365	198	1	100	2.7	652	PASS
441	442	0.01	24	16.9	2360	PASS
442	198	50	100	57.8	13981	PASS
443	442	15	24	19.8	2762	PASS