


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE082818\
 Data File : BE097373.D
 Acq On : 28 Aug 2018 10:38
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE082218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 22 18:07:26 2018

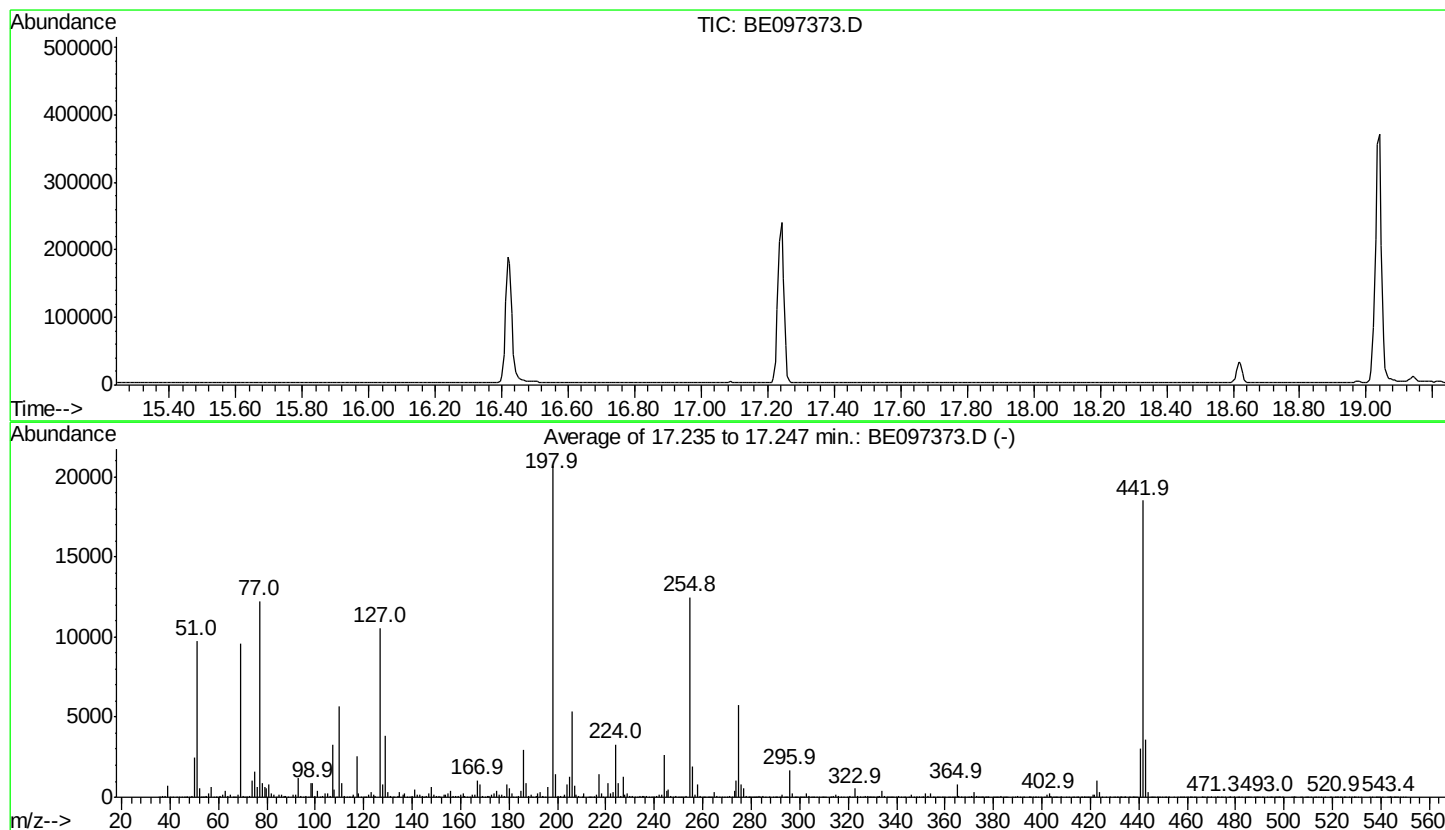

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.1	9749	PASS
68	69	0.00	2	1.5	148	PASS
69	198	0.00	100	46.2	9561	PASS
70	69	0.00	2	0.5	49	PASS
127	198	10	80	51.1	10578	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20696	PASS
199	198	5	9	6.9	1430	PASS
275	198	10	60	28.0	5788	PASS
365	198	1	100	4.0	830	PASS
441	198	0.01	100	14.5	3004	PASS
442	198	50	100	89.5	18523	PASS
443	442	15	24	19.4	3597	PASS