
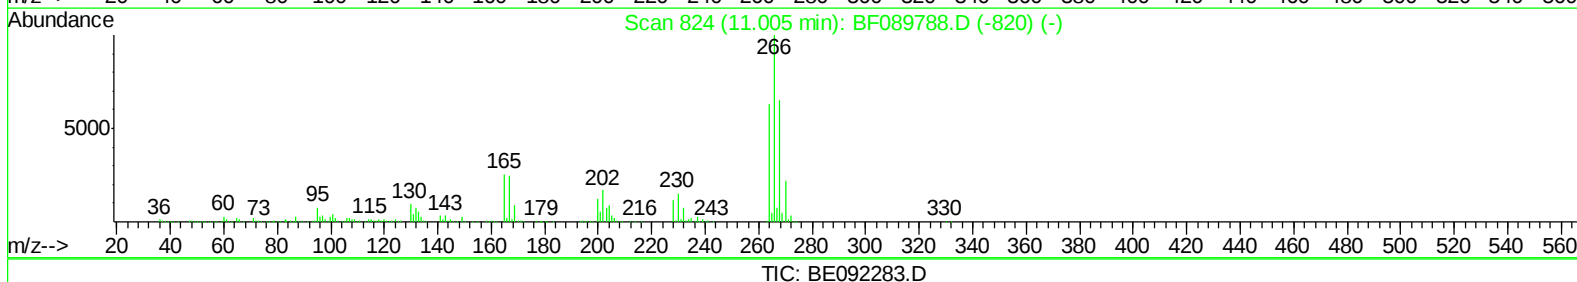
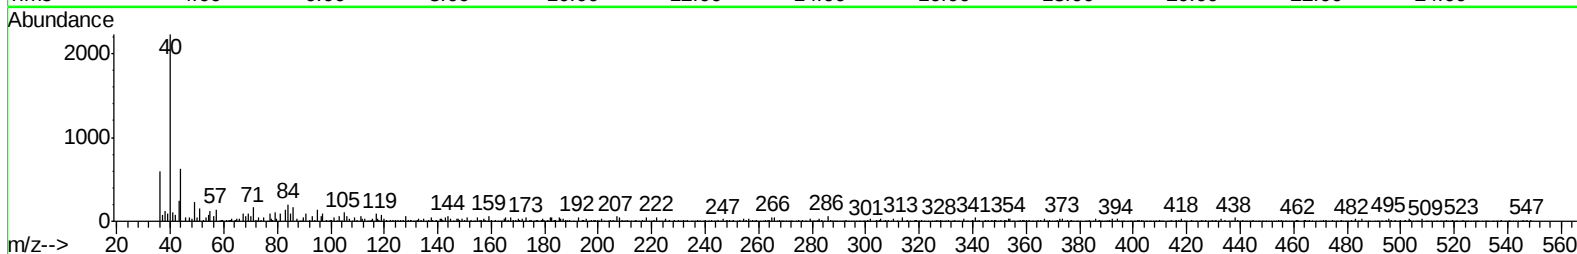


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE082916\
Data File : BE092283.D
Acq On : 29 Aug 2016 10:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 04:40:29 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 26 18:51:25 2016
Response via : Initial Calibration

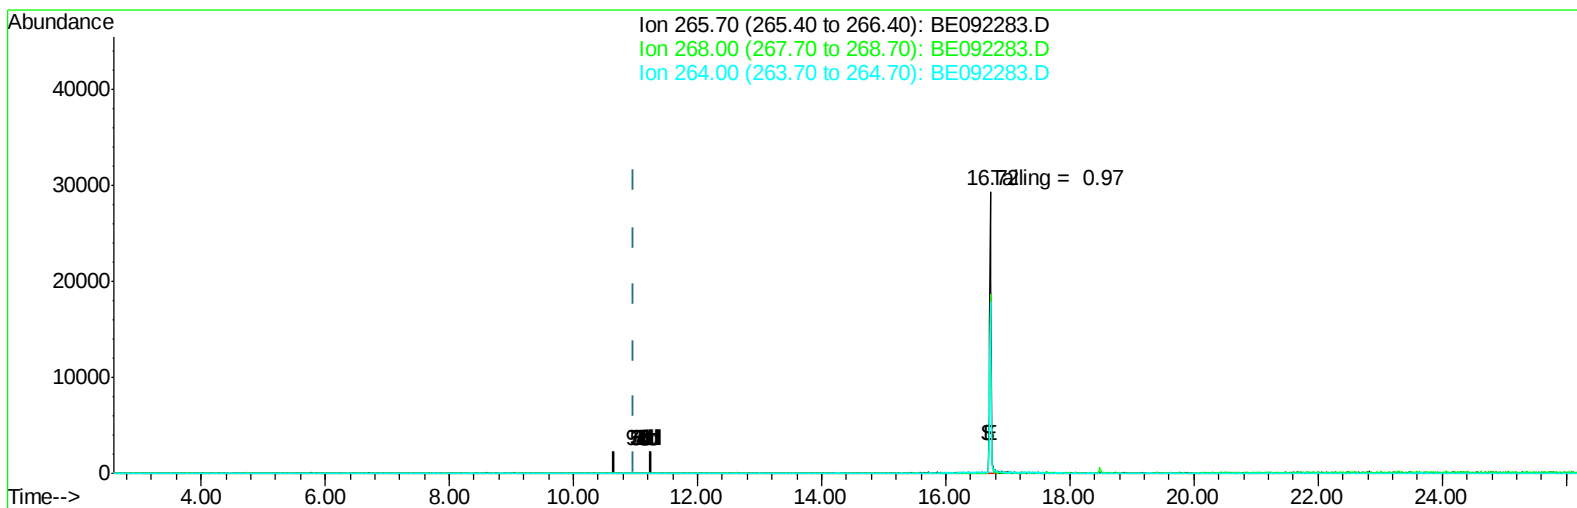

TIC: BE092283.D

(69) Pentachlorophenol (C)




11.154min (+0.183) 125.65ng

response 23

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	41.67#
264.00	63.90	35.42#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE082916\
Data File : BE092283.D
Acq On : 29 Aug 2016 10:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 04:40:29 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 26 18:51:25 2016
Response via : Initial Calibration

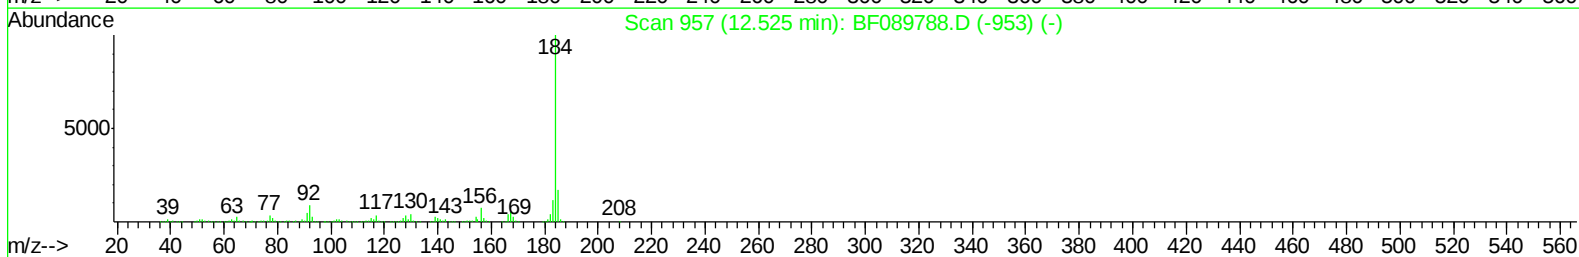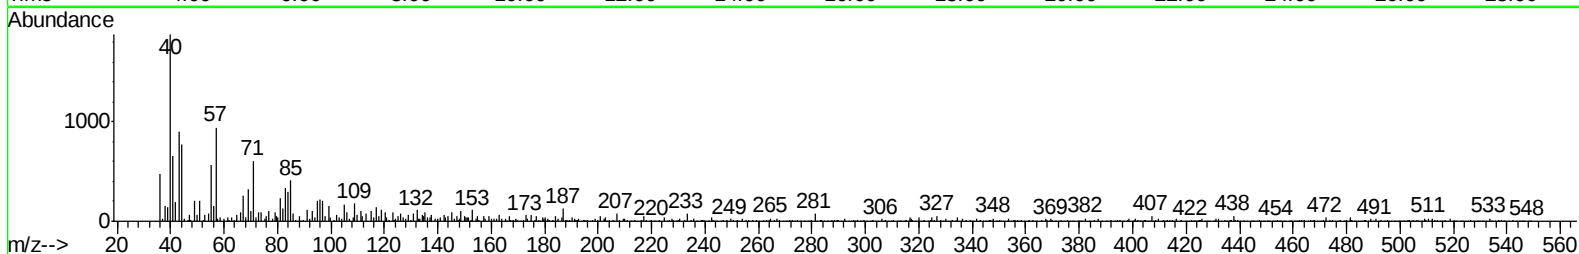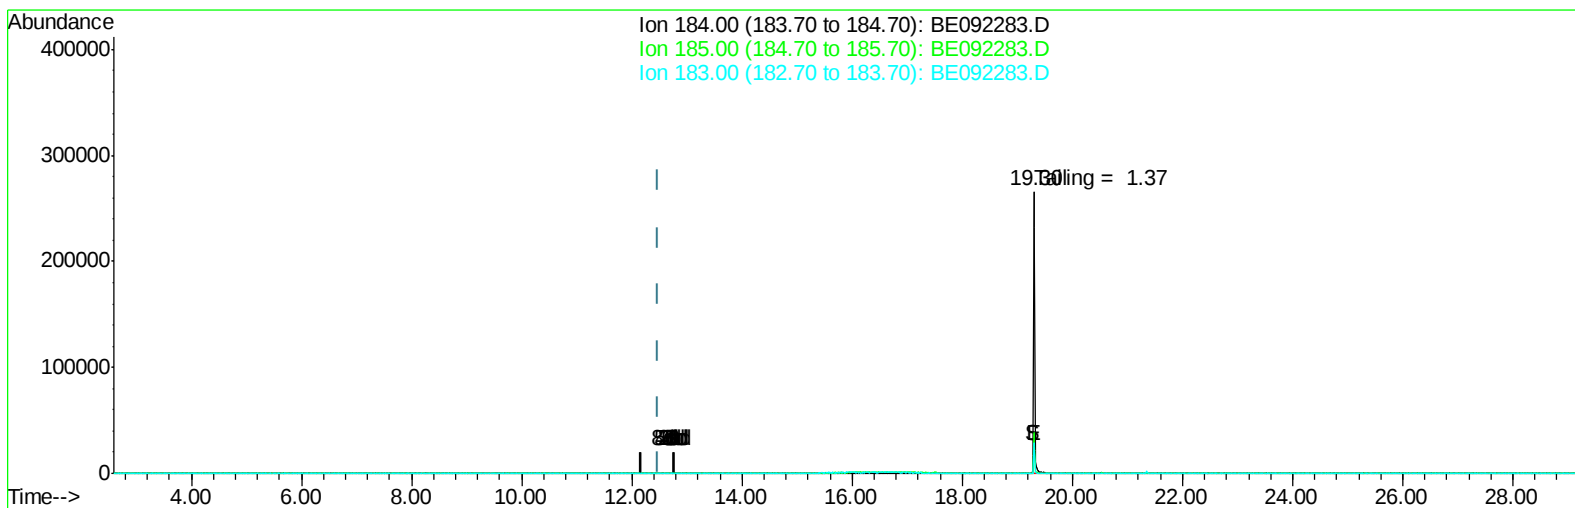

TIC: BE092283.D

(76) Benzidine

12.717min (+0.226) 54.08ng

response 28

Ion	Exp%	Act%
184.00	100	100
185.00	17.30	48.21#
183.00	12.10	28.57#
0.00	0.00	0.00