


Data Path : Z:\HPCHEM1\BNA E\DATA\BE082916\
Data File : BE092283.D
Acq On : 29 Aug 2016 10:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE082916.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 29 18:19:23 2016

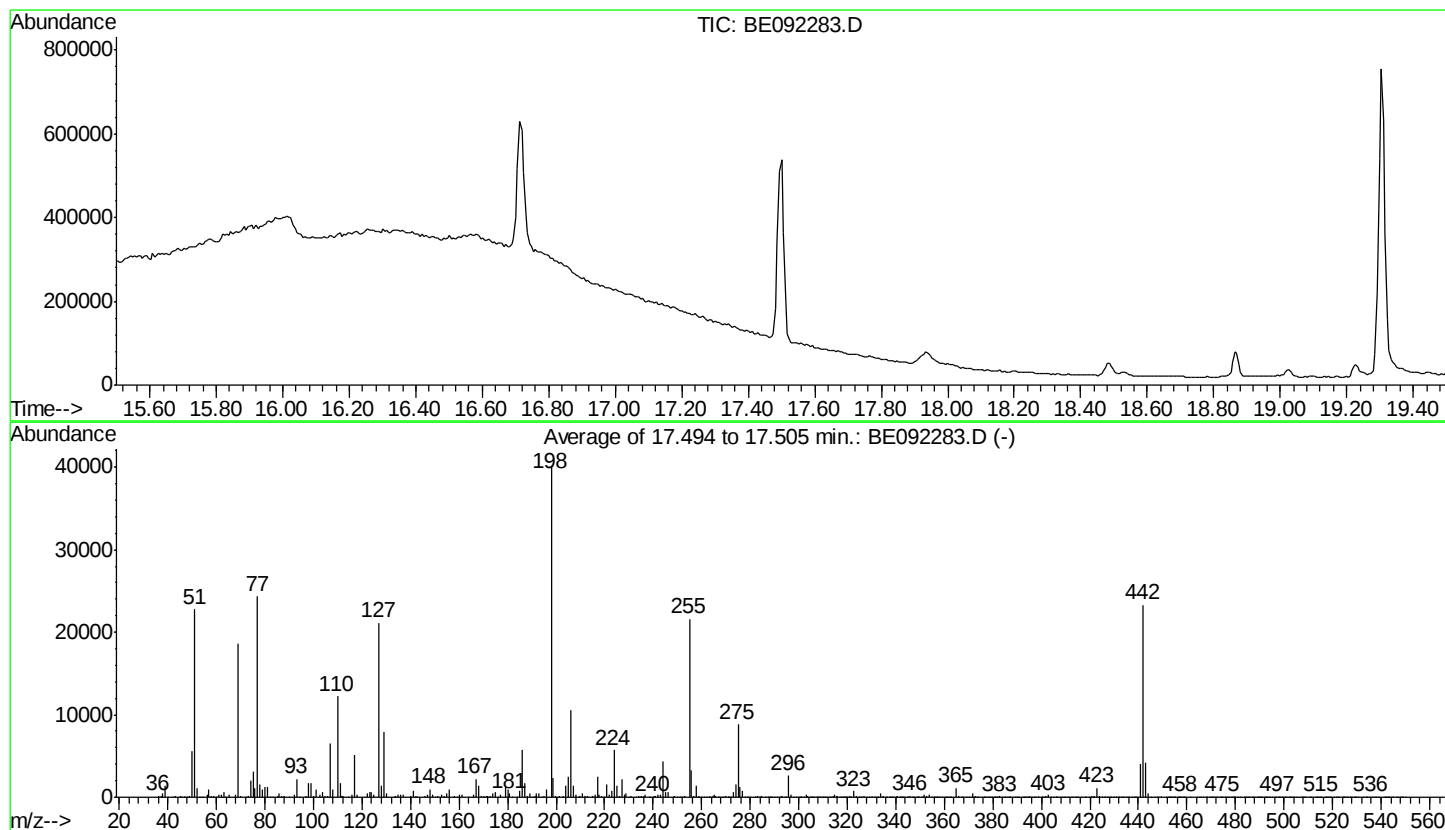

AutoFind: Scans 2537, 2538, 2539; Background Corrected with Scan 2527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.6	22743	PASS
68	69	0.00	2	1.8	329	PASS
69	198	0.00	100	46.5	18696	PASS
70	69	0.00	2	0.8	154	PASS
127	198	10	80	52.6	21146	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40190	PASS
199	198	5	9	5.9	2371	PASS
275	198	10	60	22.0	8835	PASS
365	198	1	100	2.9	1149	PASS
441	442	0.01	24	17.3	4044	PASS
442	198	50	100	58.1	23347	PASS
443	442	15	24	18.3	4264	PASS