
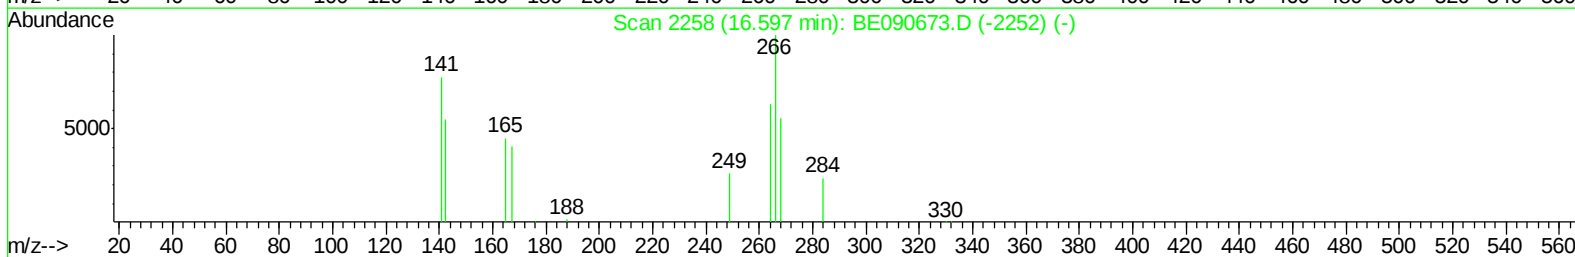
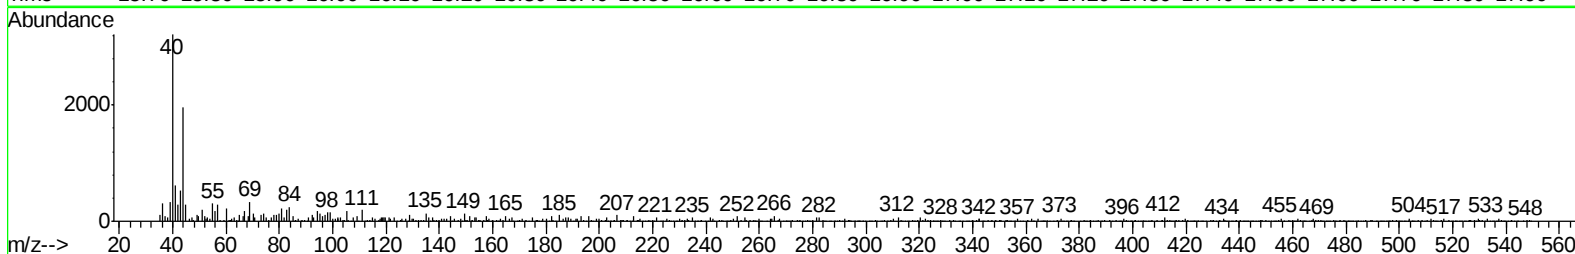


Data Path : Z:\HPCHEM1\BNA E\DATA\BE090115\
Data File : BE090668.D
Acq On : 1 Sep 2015 16:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 05:45:18 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 01:57:39 2015
Response via : Initial Calibration

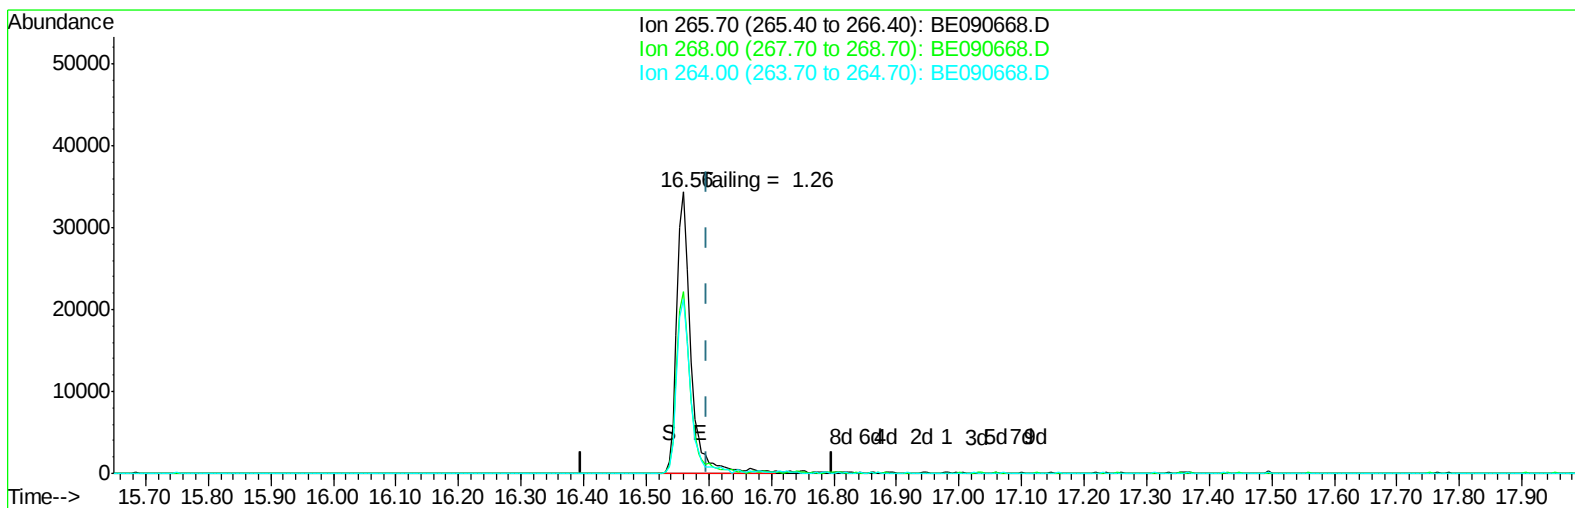

TIC: BE090668.D

(21) Pentachlorophenol

16.983min (+0.386) 14.82ng

response 24

Ion	Exp%	Act%
265.70	100	100
268.00	62.00	41.84#
264.00	67.40	41.84#
0.00	0.00	0.00