

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE090115\
 Data File : BE090691.D
 Acq On : 2 Sep 2015 6:13
 Operator : UM/IZ
 Sample : G3504-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 083015-D534-F-U-S

Quant Time: Sep 02 06:54:49 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 02 01:57:39 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	37383	5.00	ng	0.00
6) Naphthalene-d8	10.31	136	161294	5.00	ng	0.00
12) Acenaphthene-d10	14.17	164	82337	5.00	ng	0.00
18) Phenanthrene-d10	16.91	188	212278	5.00	ng	0.00
25) Chrysene-d12	21.07	240	284613	5.00	ng	0.00
32) Perylene-d12	23.36	264	271623	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.18	112	29407	4.04	ng	0.00
5) Phenol-d6	6.75	99	25048	2.41	ng	0.00
7) Nitrobenzene-d5	8.71	82	40383	3.79	ng	0.00
13) 2,4,6-Tribromophenol	15.68	330	21881	9.03	ng	0.00
14) 2-Fluorobiphenyl	12.80	172	89672	3.93	ng	0.00
27) Terphenyl-d14	19.53	244	197737	6.28	ng	0.00
Target Compounds						
30) Bis(2-ethylhexyl)phthalate	21.00	149	2164	0.20	ng	Qvalue # 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE090115\
Data File : BE090691.D
Acq On : 2 Sep 2015 6:13
Operator : UM/IZ
Sample : G3504-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
083015-D534-F-U-S

Quant Time: Sep 02 06:54:49 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 01:57:39 2015
Response via : Initial Calibration

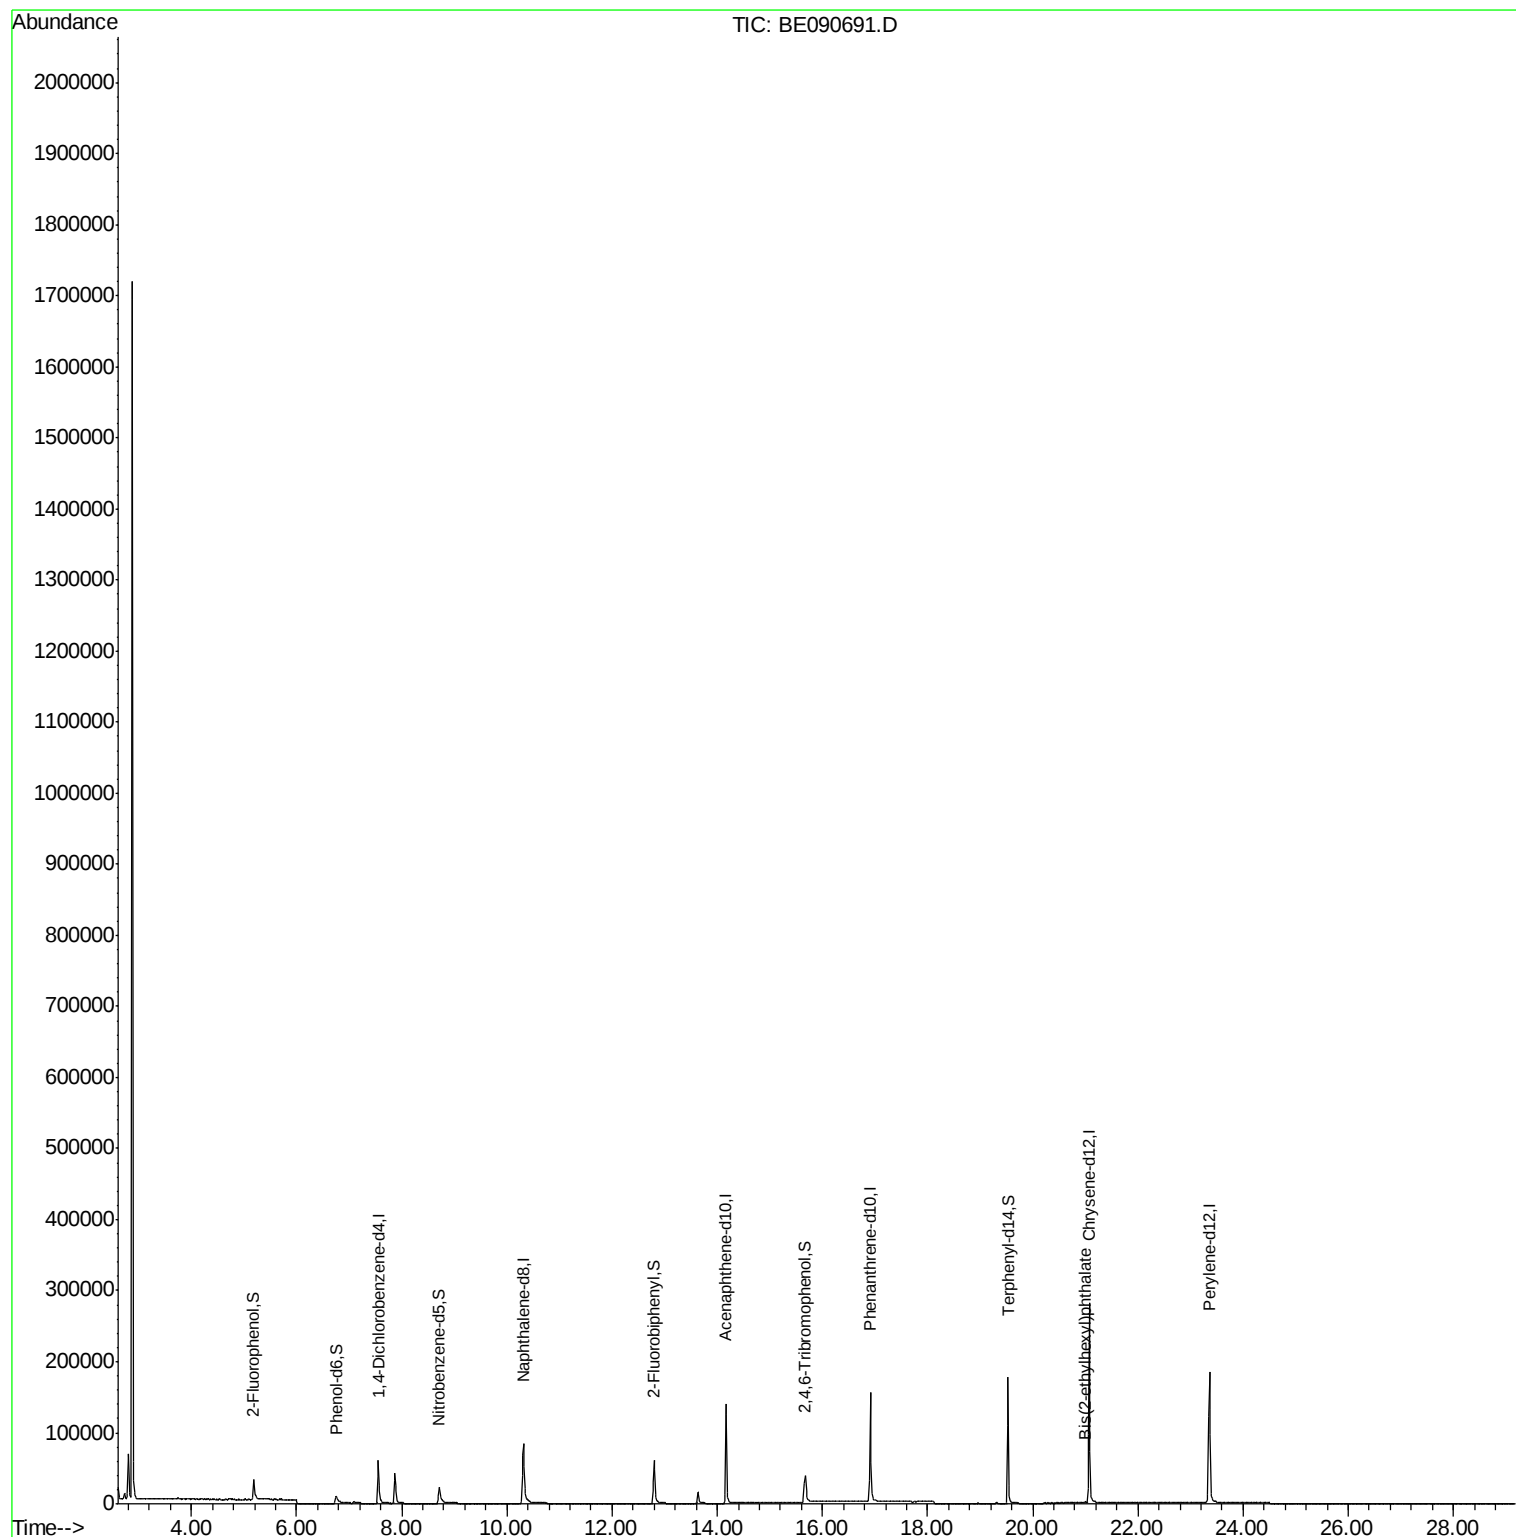

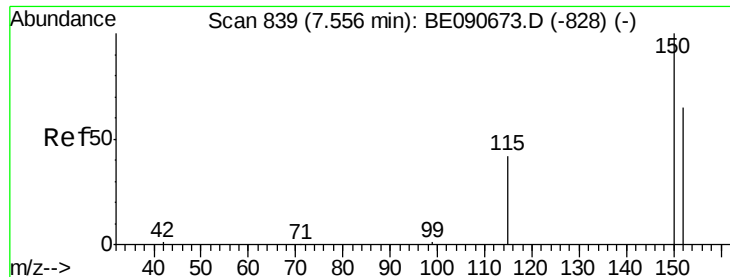

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.56 min Scan# 839

Delta R.T. -0.00 min

Lab File: BE090691.D

Acq: 2 Sep 2015 6:13

Instrument :

BNA_E

ClientSampleId :

083015-D534-F-U-S


Tgt Ion:152 Resp: 37383

Ion Ratio Lower Upper

152 100

150 152.2 122.2 183.4




115 63.7 51.0 76.4

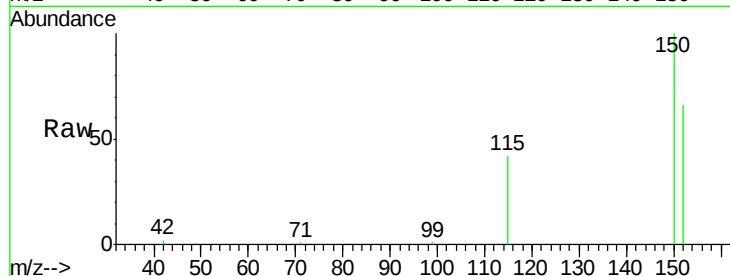

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

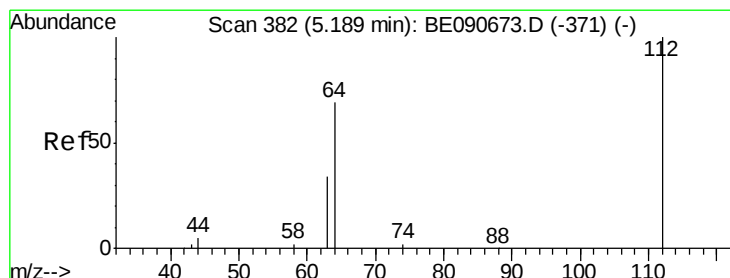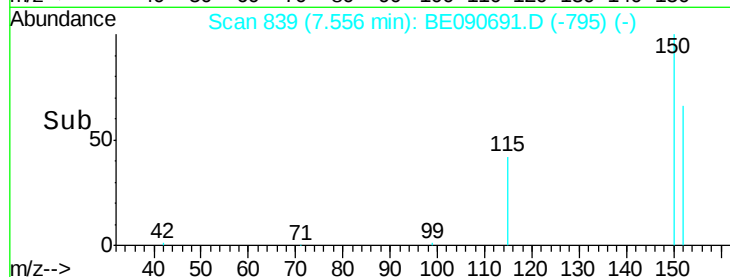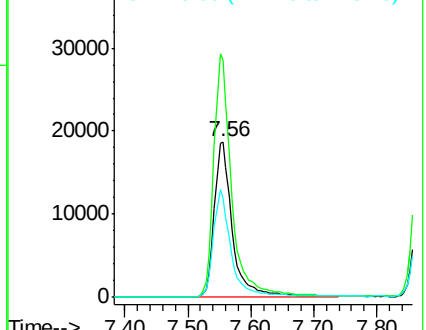

#4

2-Fluorophenol

Concen: 4.04 ng

RT: 5.18 min Scan# 381

Delta R.T. -0.01 min

Lab File: BE090691.D

Acq: 2 Sep 2015 6:13


Tgt Ion:112 Resp: 29407

Ion Ratio Lower Upper

112 100

64 70.6 57.3 85.9



63 37.0 29.2 43.8

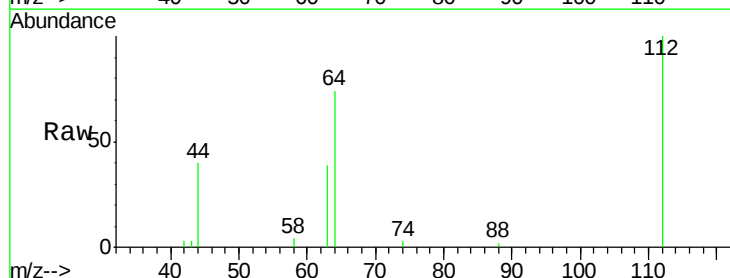


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

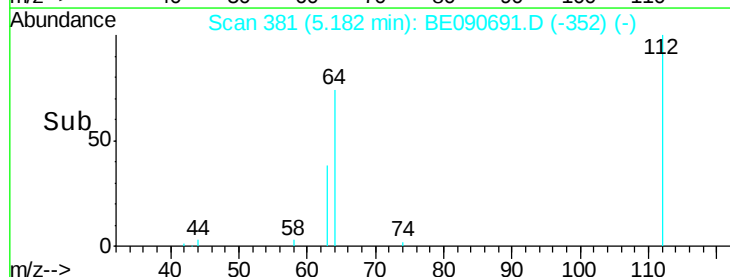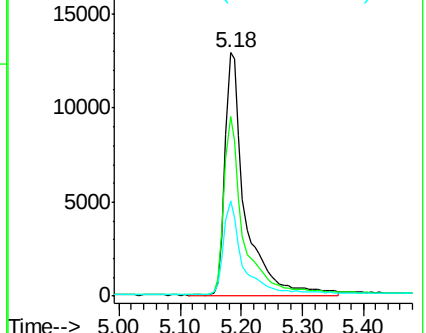

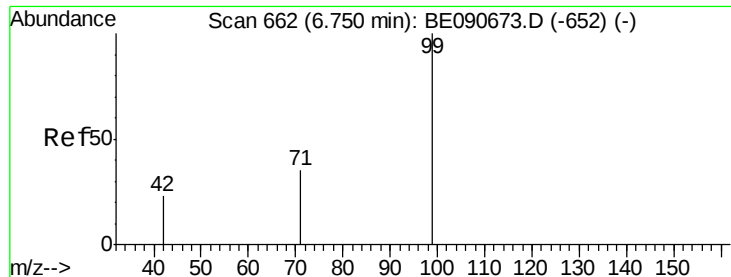

#5

Phenol-d6

Concen: 2.41 ng

RT: 6.75 min Scan# 662

Delta R.T. -0.00 min

Lab File: BE090691.D

Acq: 2 Sep 2015 6:13

Instrument :

BNA_E

ClientSampleId :

083015-D534-F-U-S


Tgt Ion: 99 Resp: 25048

Ion Ratio Lower Upper

99 100

42 21.0 16.8 25.2




71 33.8 28.3 42.5

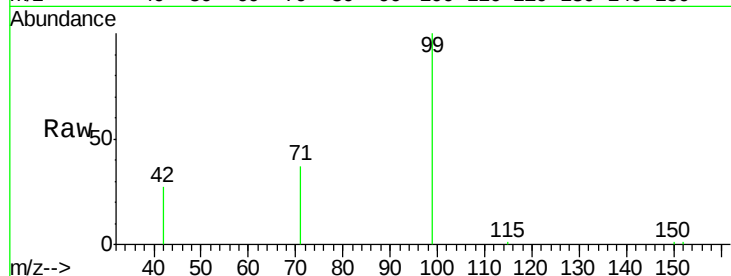

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

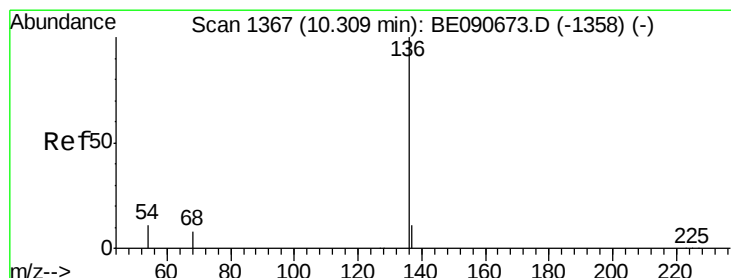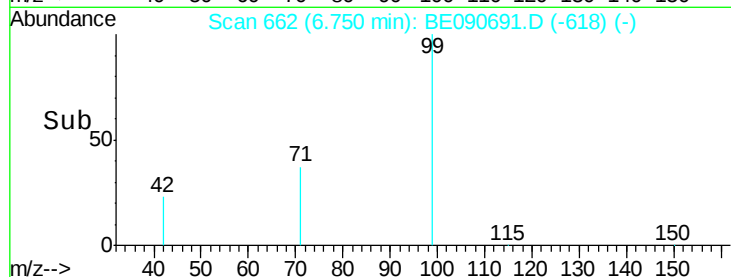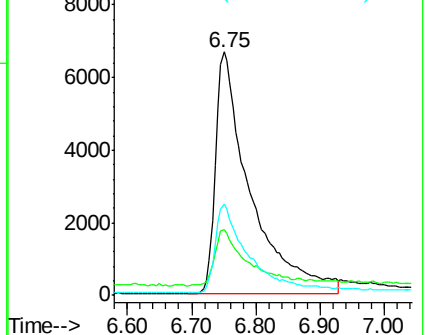

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.31 min Scan# 1367

Delta R.T. 0.00 min

Lab File: BE090691.D

Acq: 2 Sep 2015 6:13

Tgt Ion: 136 Resp: 161294


Ion Ratio Lower Upper

136 100

137 10.9 8.7 13.1

54 11.5 9.0 13.6

68 8.3 6.3 9.5


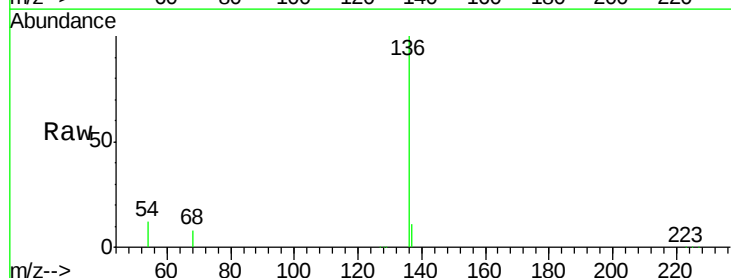



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

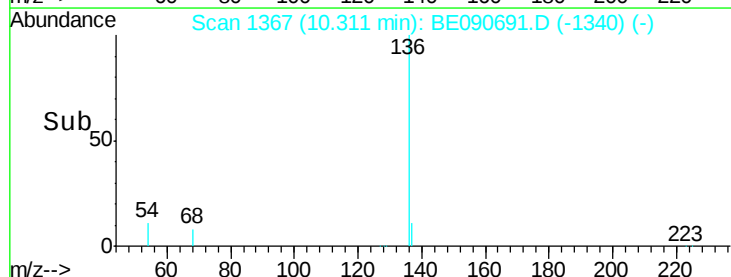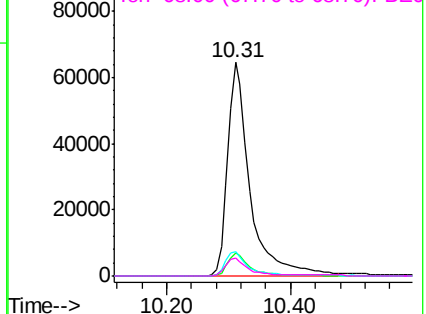

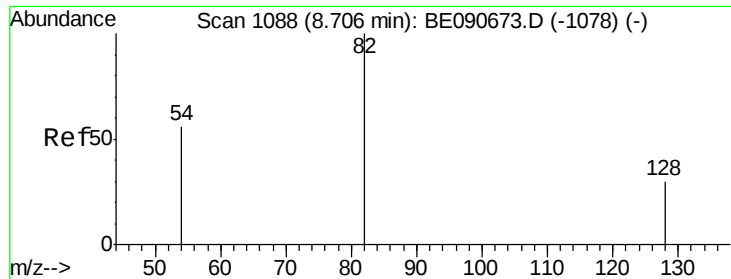

#7

Nitrobenzene-d5

Concen: 3.79 ng

RT: 8.71 min Scan# 1089

Delta R.T. 0.00 min

Lab File: BE090691.D

Acq: 2 Sep 2015 6:13

Instrument :

BNA_E

ClientSampleId :

083015-D534-F-U-S





Tgt Ion: 82 Resp: 40383

Ion Ratio Lower Upper

82 100

128 30.5 25.0 37.4

54 59.7 46.3 69.5

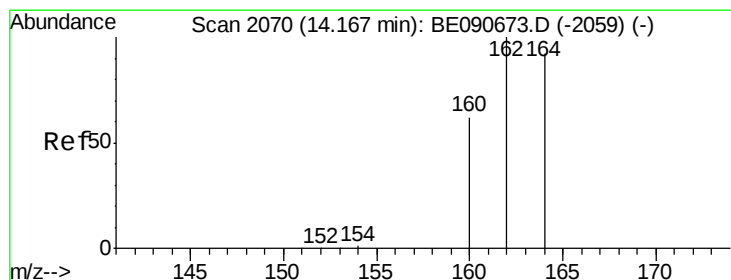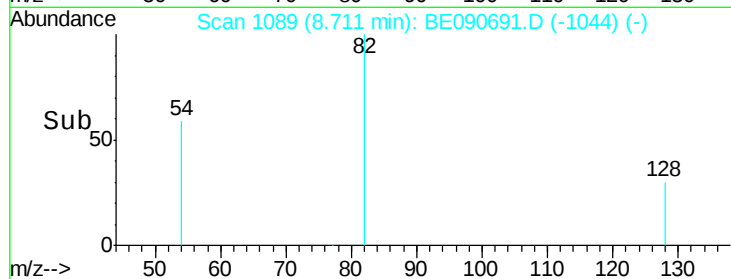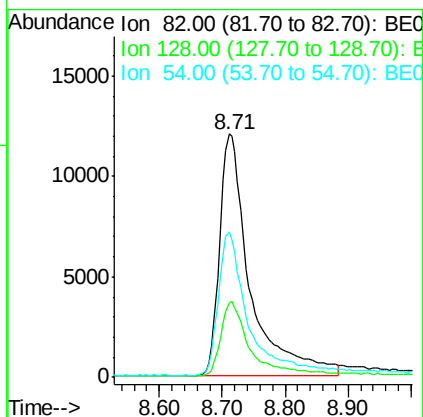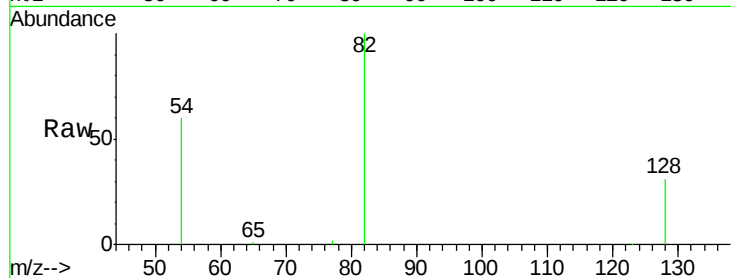

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.17 min Scan# 2070

Delta R.T. 0.00 min

Lab File: BE090691.D

Acq: 2 Sep 2015 6:13




Tgt Ion: 164 Resp: 82337


Ion Ratio Lower Upper

164 100

162 106.3 86.8 130.2

160 65.9 53.9 80.9


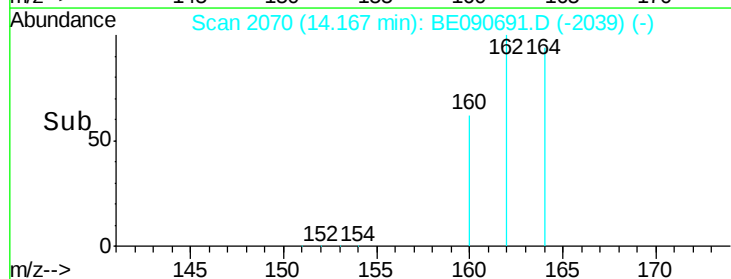
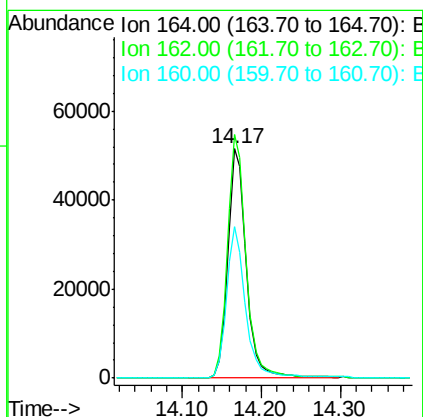
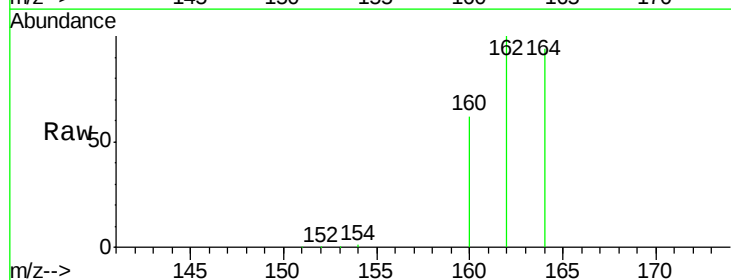


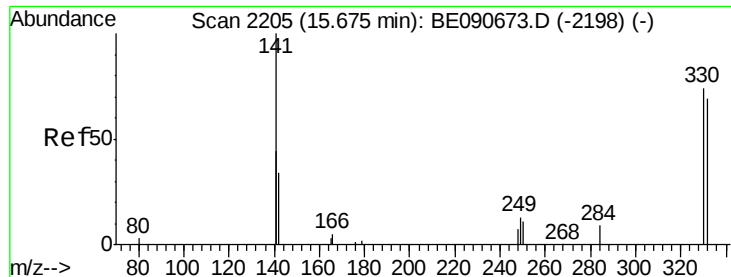

#13
 2,4,6-Tribromophenol
 Concen: 9.03 ng
 RT: 15.68 min Scan# 2205
 Delta R.T. 0.00 min
 Lab File: BE090691.D
 Acq: 2 Sep 2015 6:13




Instrument :
 BNA_E
 ClientSampleId :
 083015-D534-F-U-S


Tgt Ion: 330 Resp: 21881
 Ion Ratio Lower Upper
 330 100
 332 97.7 74.9 112.3
 141 178.5 145.2 217.8

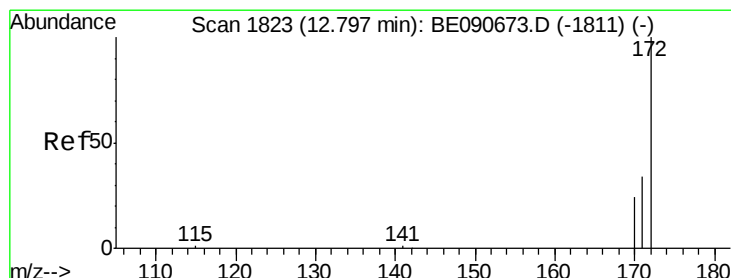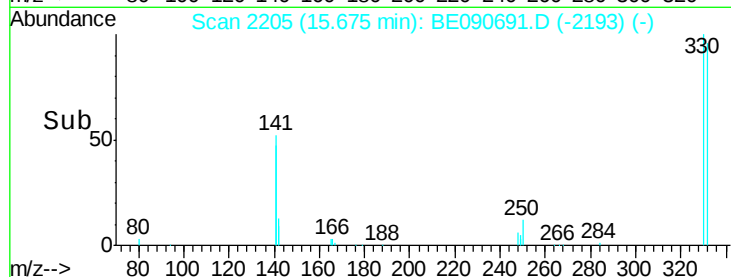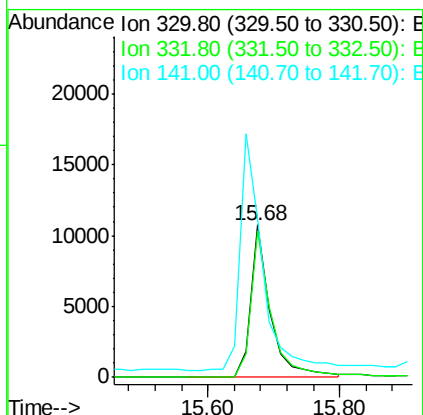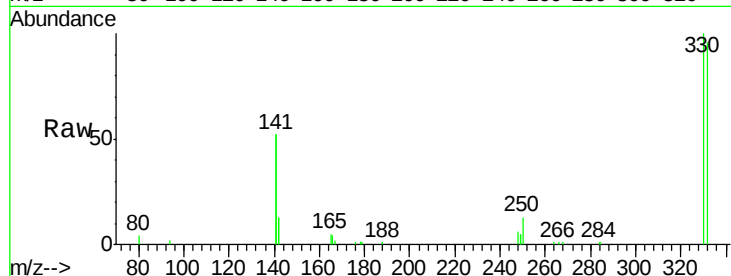

#14
 2-Fluorobiphenyl
 Concen: 3.93 ng
 RT: 12.80 min Scan# 1823
 Delta R.T. -0.00 min
 Lab File: BE090691.D
 Acq: 2 Sep 2015 6:13

Tgt Ion: 172 Resp: 89672
 Ion Ratio Lower Upper
 172 100
 171 35.3 27.8 41.8
 170 24.0 19.8 29.6

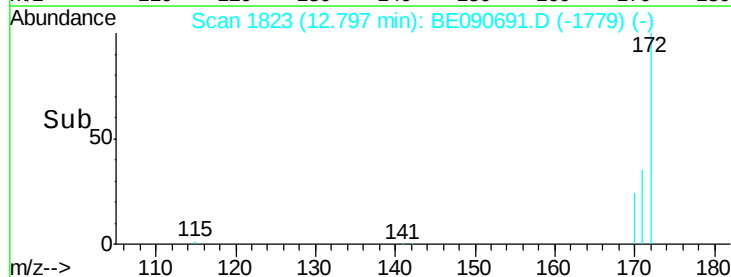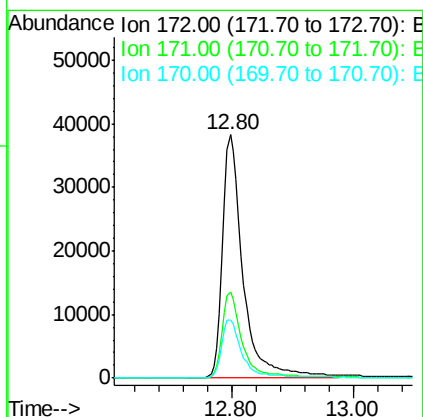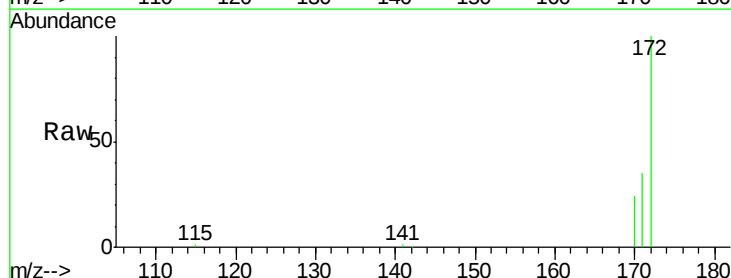

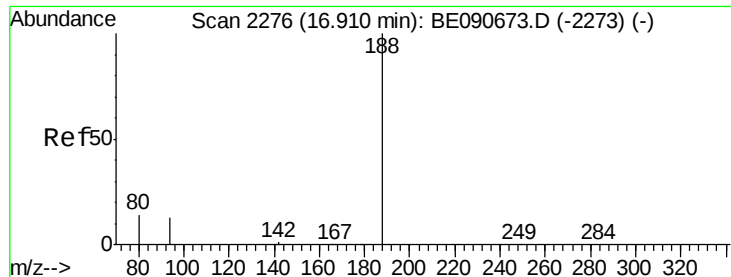

#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.91 min Scan# 2276

Delta R.T. 0.00 min

Lab File: BE090691.D

Acq: 2 Sep 2015 6:13

Instrument :

BNA_E

ClientSampleId :

083015-D534-F-U-S


Tgt Ion:188 Resp: 212278

Ion Ratio Lower Upper

188 100

94 12.2 10.3 15.5




80 13.6 11.0 16.6

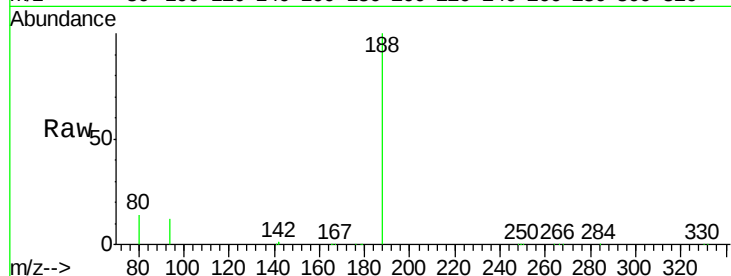

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

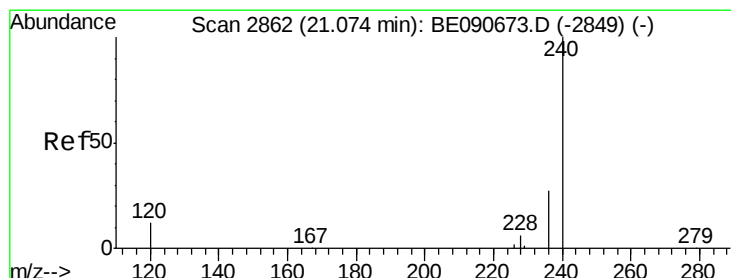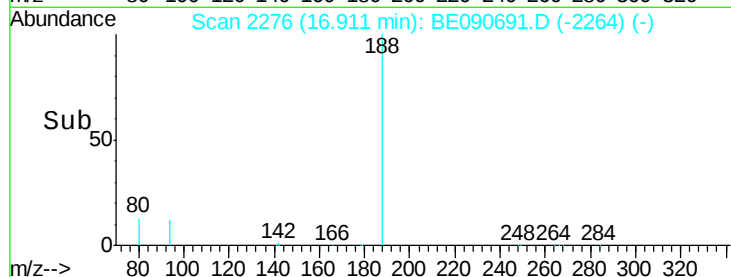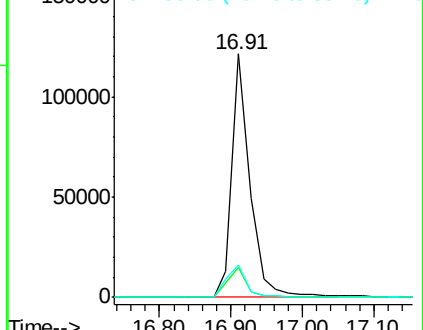

#25

Chrysene-d12

Concen: 5.00 ng

RT: 21.07 min Scan# 2862

Delta R.T. -0.00 min

Lab File: BE090691.D

Acq: 2 Sep 2015 6:13


Tgt Ion:240 Resp: 284613

Ion Ratio Lower Upper

240 100

120 11.8 10.1 15.1



236 26.9 21.9 32.9

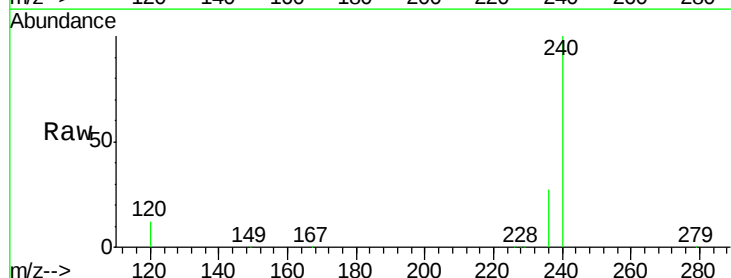


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



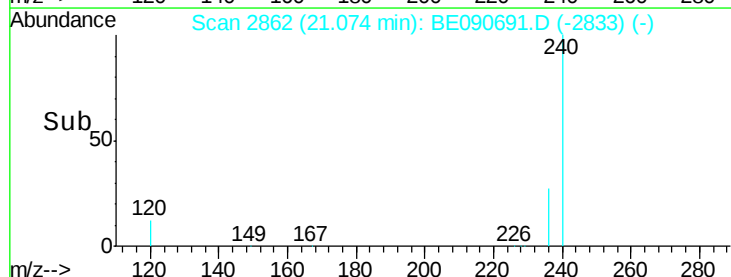
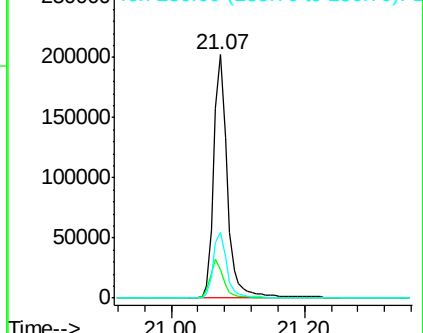


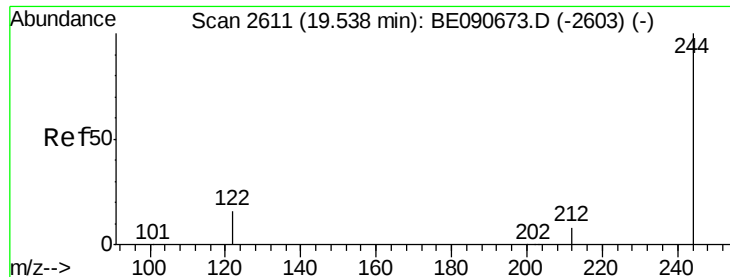

#27
 Terphenyl-d14
 Concen: 6.28 ng
 RT: 19.53 min Scan# 2610
 Delta R.T. -0.01 min
 Lab File: BE090691.D
 Acq: 2 Sep 2015 6:13




Instrument :
 BNA_E
 ClientSampleId :
 083015-D534-F-U-S




Tgt Ion: 244 Resp: 197737
 Ion Ratio Lower Upper
 244 100
 212 8.0 6.9 10.3
 122 13.0 12.9 19.3

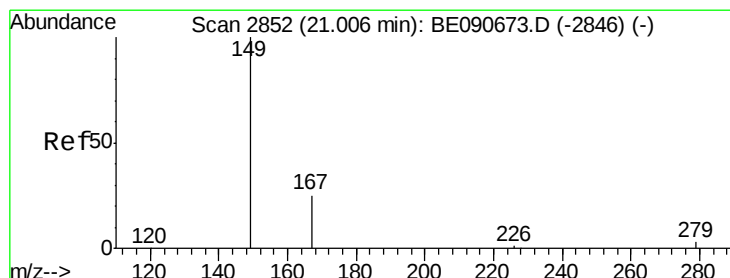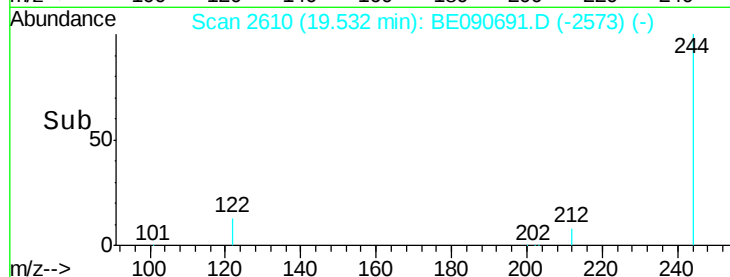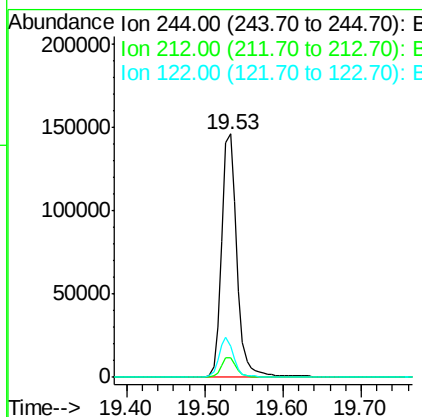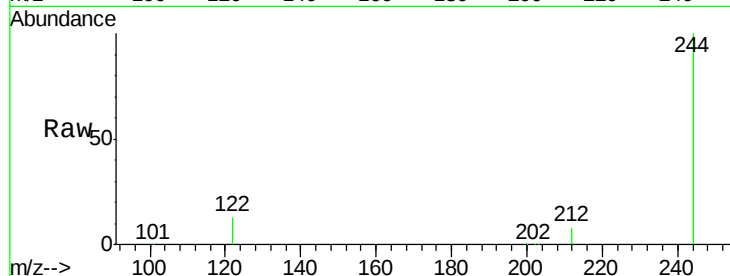

#30
 Bis(2-ethylhexyl)phthalate
 Concen: 0.20 ng
 RT: 21.00 min Scan# 2851
 Delta R.T. -0.01 min
 Lab File: BE090691.D
 Acq: 2 Sep 2015 6:13

Tgt Ion: 149 Resp: 2164
 Ion Ratio Lower Upper
 149 100
 167 23.0 20.1 30.1
 279 4.5 2.3 3.5#

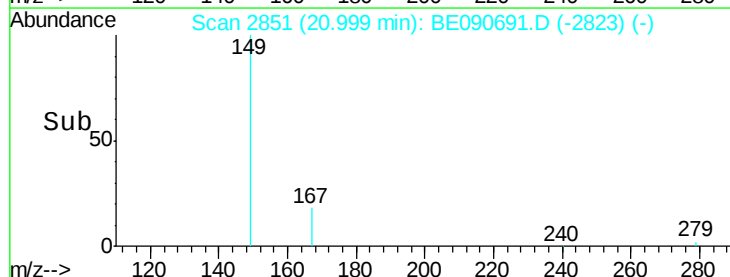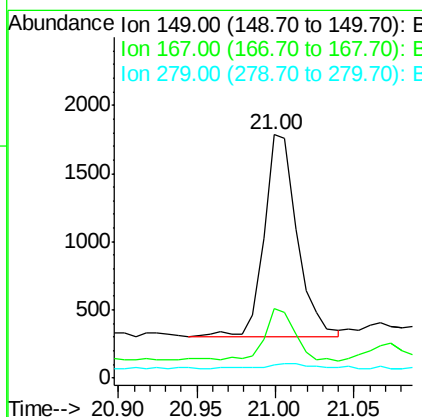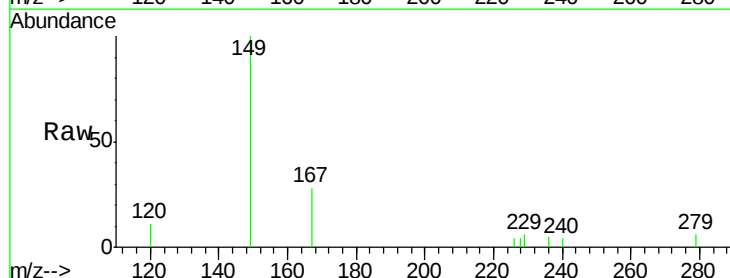

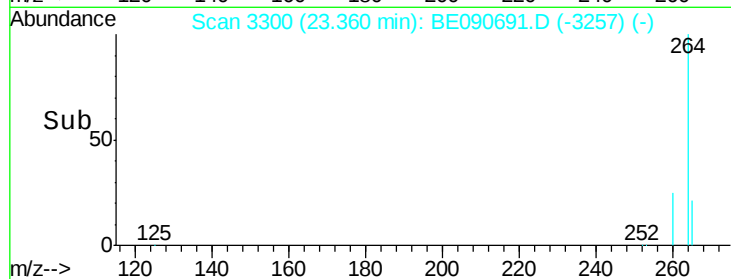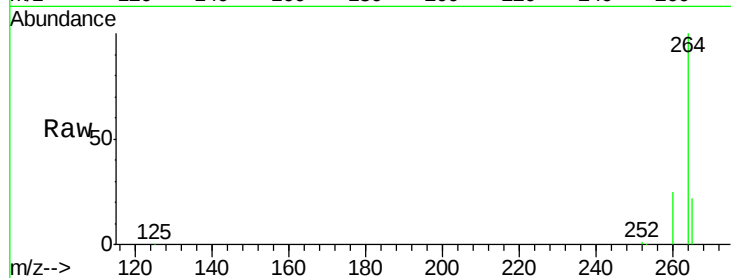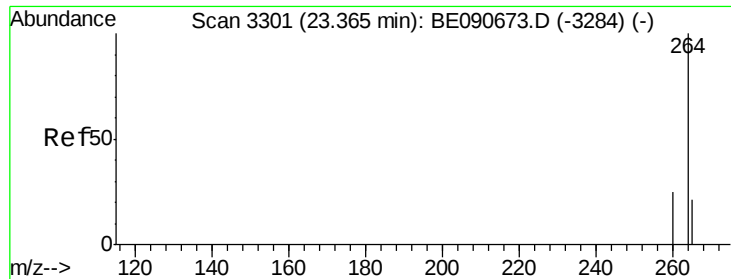

#32

Perylene-d12

Concen: 5.00 ng

RT: 23.36 min Scan# 3300

Delta R.T. -0.00 min

Lab File: BE090691.D

Acq: 2 Sep 2015 6:13

Instrument :

BNA_E

ClientSampleId :

083015-D534-F-U-S

Tgt Ion: 264 Resp: 271623

Ion Ratio Lower Upper

264 100

260 25.1 19.7 29.5

265 21.8 17.5 26.3

