


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE090115\
Data File : BE090668.D
Acq On : 1 Sep 2015 16:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 02 11:40:50 2015

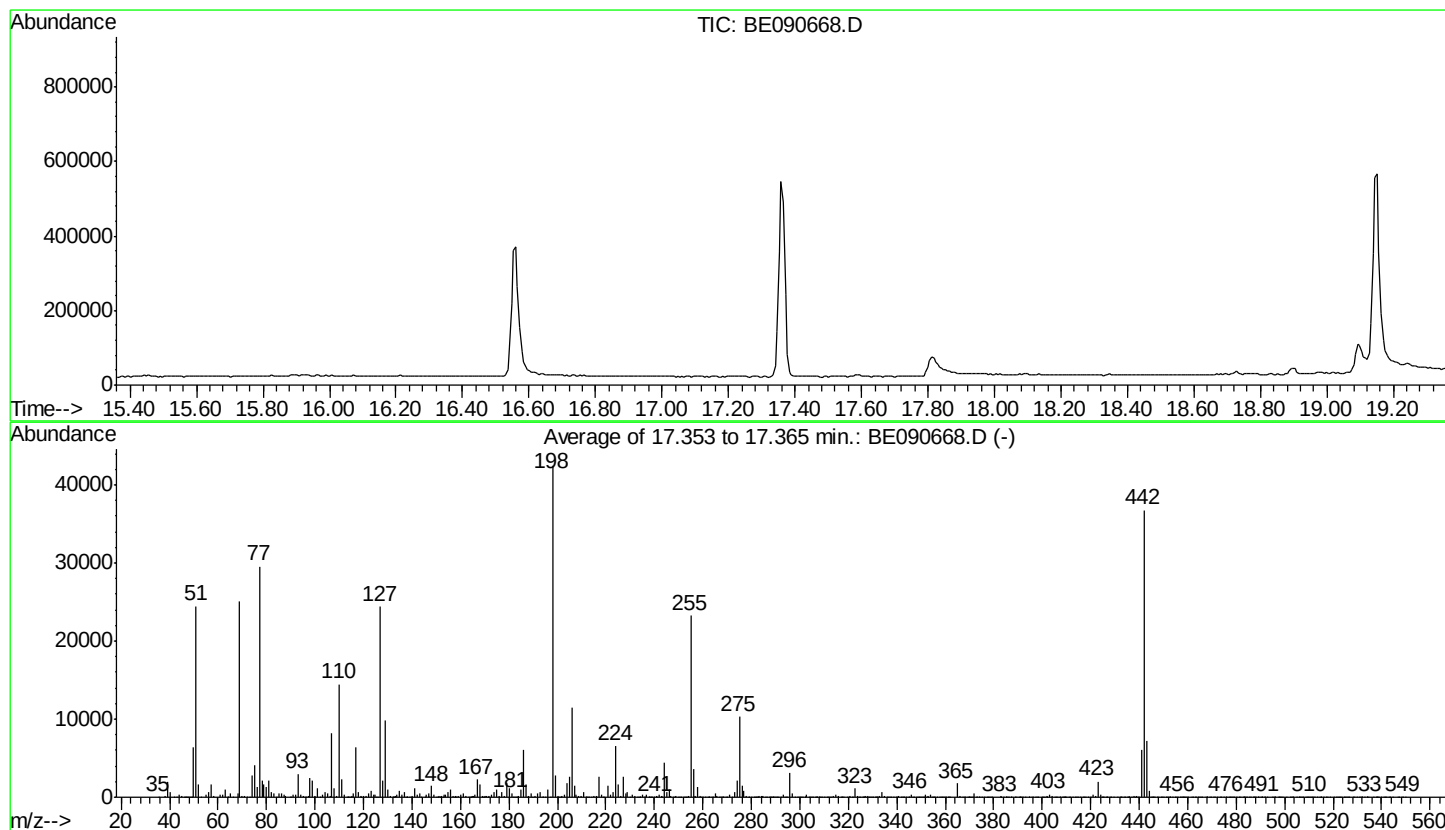

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.7	24488	PASS
68	69	0.00	2	2.0	512	PASS
69	198	0.00	100	59.2	25143	PASS
70	69	0.00	2	1.0	239	PASS
127	198	10	80	57.5	24397	PASS
197	198	0.00	2	0.1	61	PASS
198	198	100	100	100.0	42450	PASS
199	198	5	9	6.4	2713	PASS
275	198	10	60	24.2	10274	PASS
365	198	1	100	4.1	1732	PASS
441	442	0.01	24	16.3	5988	PASS
442	198	50	100	86.5	36733	PASS
443	442	15	24	19.8	7261	PASS