

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE090116\
 Data File : BE092324.D
 Acq On : 1 Sep 2016 12:07
 Operator : UM/SJ
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.1

Quant Time: Sep 02 03:16:45 2016
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 02 03:16:21 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	9388	5.00	ng	-0.02
7) Naphthalene-d8	10.95	136	44869	5.00	ng	0.00
12) Acenaphthene-d10	14.82	164	27509	5.00	ng	-0.02
18) Phenanthrene-d10	17.58	188	72712	5.00	ng	0.00
24) Chrysene-d12	21.75	240	89846	5.00	ng	0.00
31) Perylene-d12	24.12	264	97751	5.00	ng	0.00

System Monitoring Compounds						
4) 2-Fluorophenol	5.68	112	302	0.14	ng	-0.01
5) Phenol-d6	7.36	99	397	0.14	ng	0.00
8) Nitrobenzene-d5	9.34	82	495	0.17	ng	-0.02
13) 2,4,6-Tribromophenol	16.32	330	135	0.17	ng	0.00
14) 2-Fluorobiphenyl	13.45	172	1025	0.12	ng	0.00
26) Terphenyl-d14	20.19	244	1877	0.16	ng	0.00


Target Compounds						Qvalue
2) 1,4-Dioxane	3.41	88	160	0.12	ng	# 75
3) n-Nitrosodimethylamine	3.78	42	235	0.17	ng	# 84
6) bis(2-Chloroethyl)ether	7.59	93	315	0.14	ng	# 93
9) Naphthalene	11.01	128	1167	0.12	ng	# 87
10) Hexachlorobutadiene	11.30	225	183	0.12	ng	98
11) 2-Methylnaphthalene	12.64	142	736	0.12	ng	96
15) Acenaphthylene	14.53	152	5549	0.12	ng	99
16) Acenaphthene	14.88	154	1009	0.13	ng	89
17) Fluorene	15.87	166	1212	0.13	ng	99
19) Hexachlorobenzene	16.89	284	382	0.13	ng	97
20) Pentachlorophenol	17.26	266	131	0.17	ng	91
21) Phenanthrene	17.62	178	2176	0.13	ng	# 57
22) Anthracene	17.72	178	1955	0.12	ng	96
23) Fluoranthene	19.61	202	11187	0.14	ng	# 92
25) Pyrene	19.97	202	11580	0.14	ng	98
27) Benzo(a)anthracene	21.72	228	16335	0.17	ng	# 90
28) Chrysene	21.72	228	16335	0.19	ng	# 90
29) Bis(2-ethylhexyl)phthalate	21.66	149	77008	11.96	ng	# 100
30) Indeno(1,2,3-cd)pyrene	26.63	276	13209	0.15	ng	98
32) Benzo(b)fluoranthene	23.39	252	3201	0.14	ng	# 46
33) Benzo(k)fluoranthene	23.44	252	3199	0.12	ng	# 54
34) Benzo(a)pyrene	24.02	252	2988	0.13	ng	# 31
35) Dibenzo(a,h)anthracene	26.65	278	2691	0.13	ng	# 70
36) Benzo(g,h,i)perylene	27.40	276	11338	0.12	ng	# 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE090116\
Data File : BE092324.D
Acq On : 1 Sep 2016 12:07
Operator : UM/SJ
Sample : SSTDIC0.1
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTDIC0.1

Quant Time: Sep 02 03:16:45 2016
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 03:16:21 2016
Response via : Initial Calibration

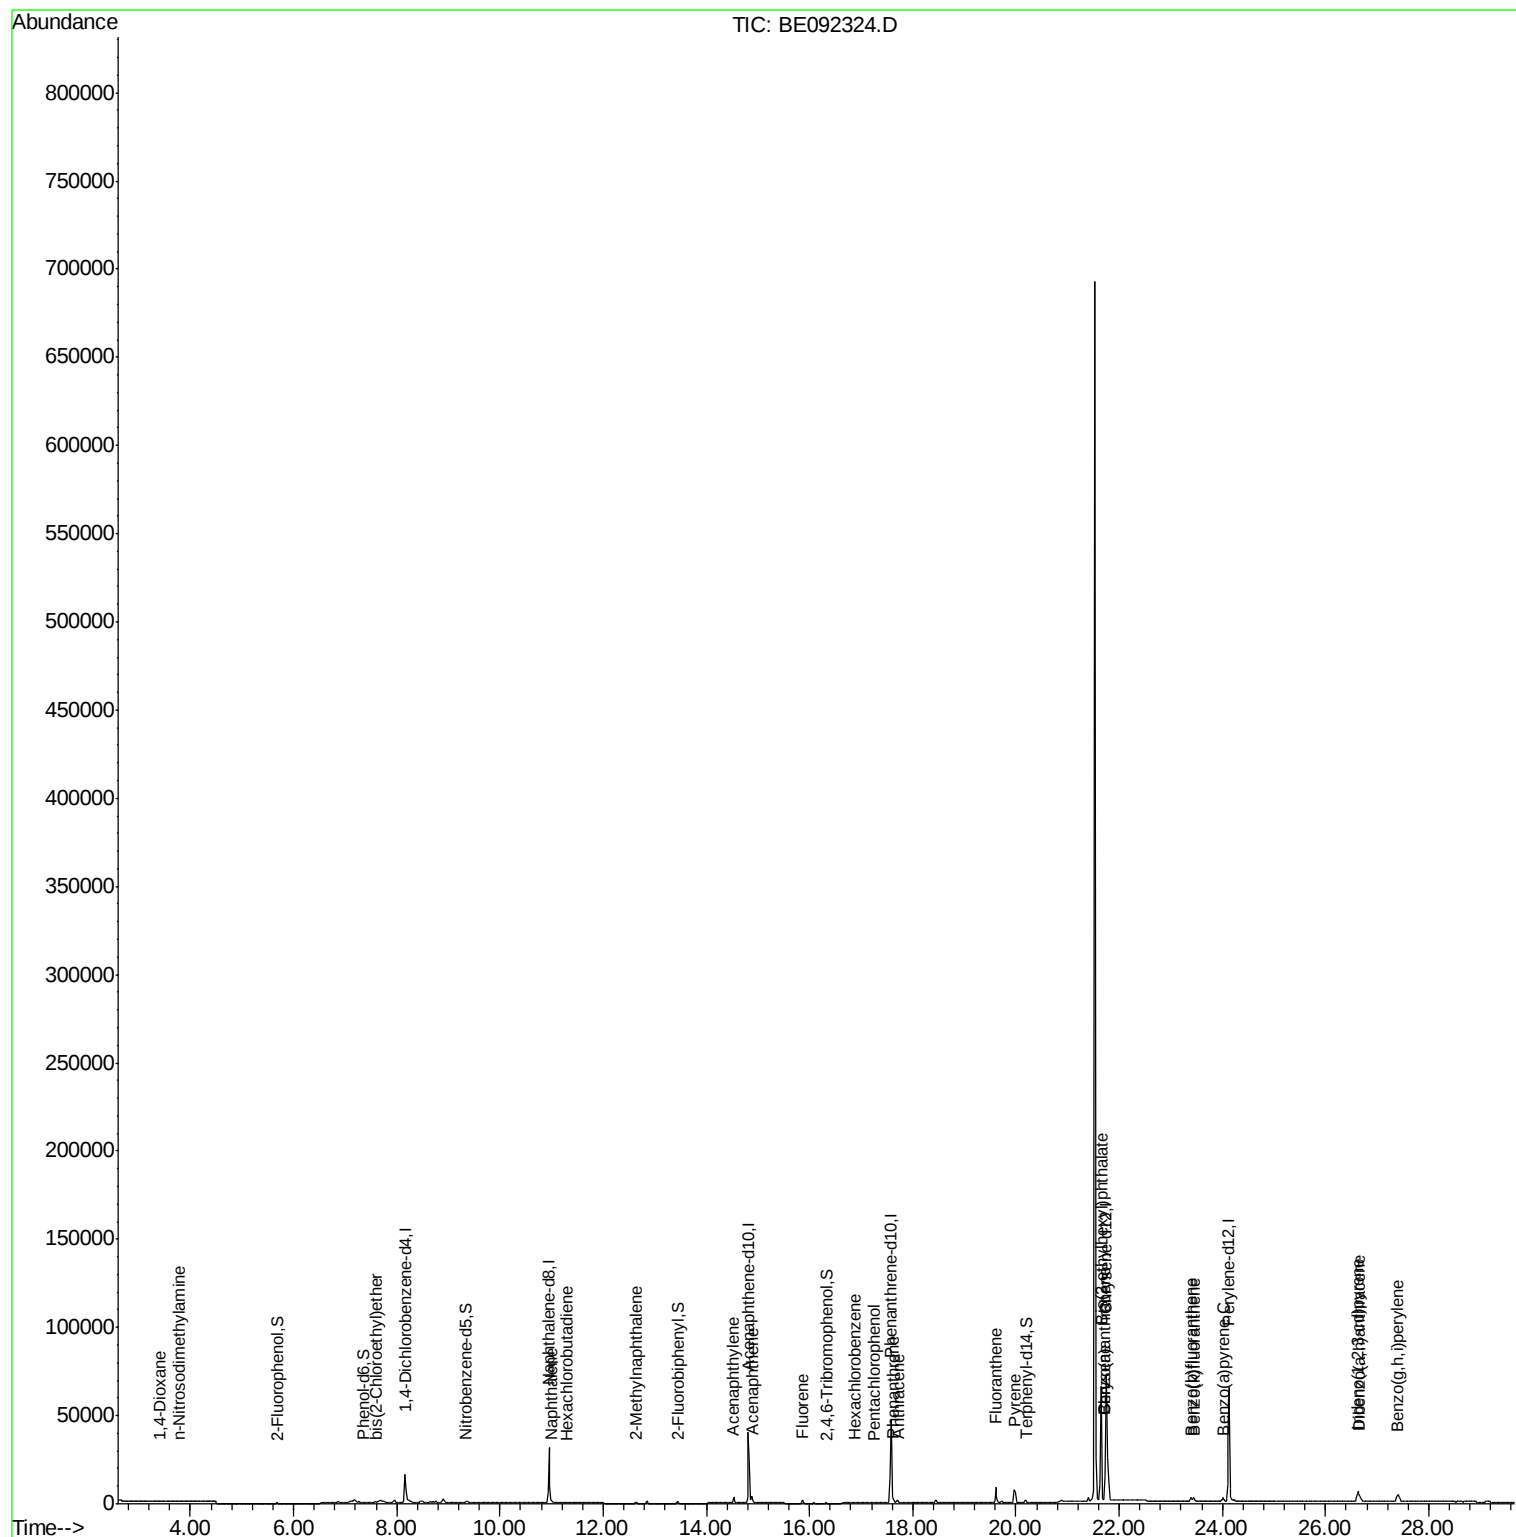

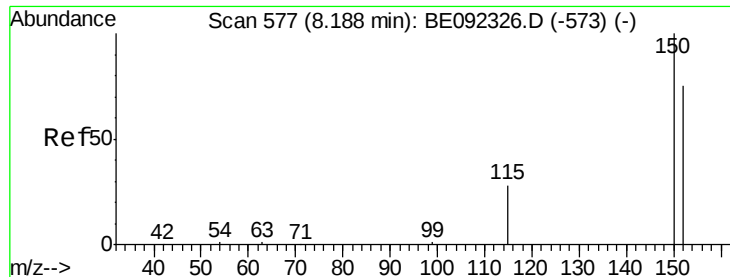

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.16 min Scan# 576

Delta R.T. -0.02 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07

Instrument :

BNA_E

ClientSampleId :

SSTDICCO.1


Tgt Ion:152 Resp: 9388

Ion Ratio Lower Upper

152 100

150 180.1 106.0 159.0#




115 85.0 31.2 46.8#

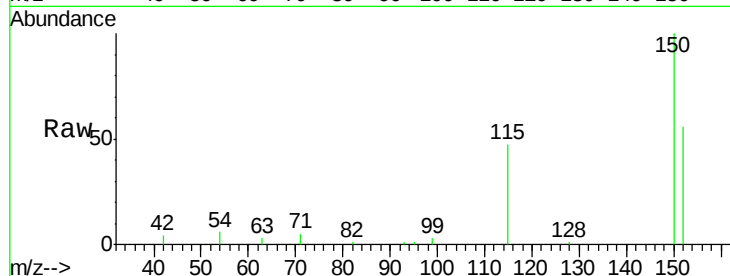

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

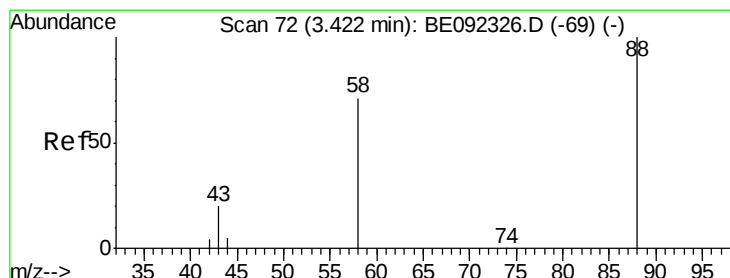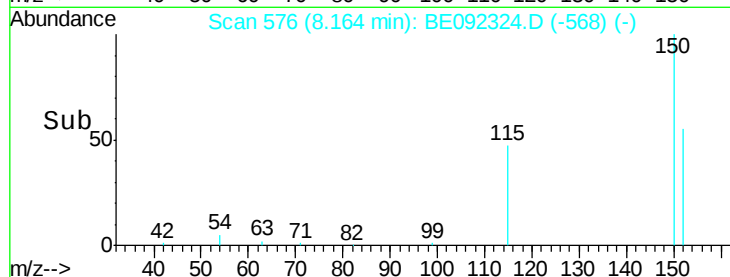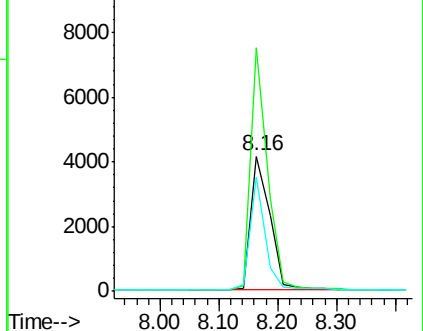

#2

1,4-Dioxane

Concen: 0.12 ng

RT: 3.41 min Scan# 71

Delta R.T. -0.01 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07


Tgt Ion: 88 Resp: 160

Ion Ratio Lower Upper

88 100

58 80.6 63.6 95.4



43 80.6 28.0 42.0#

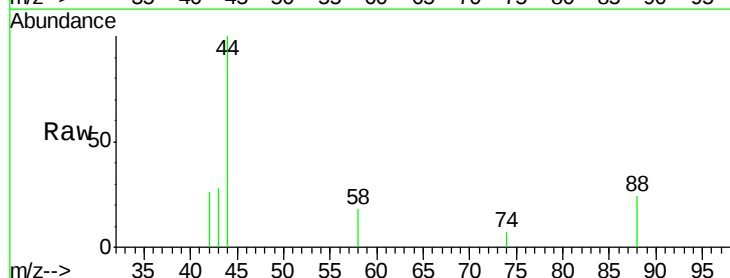


Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

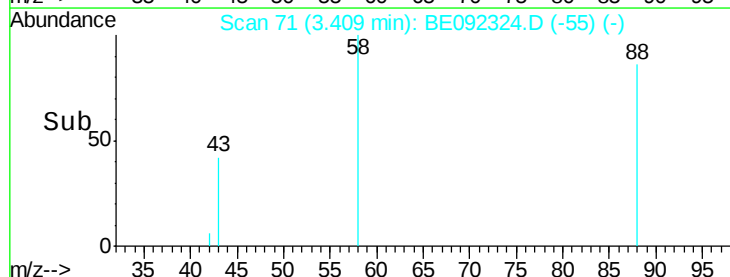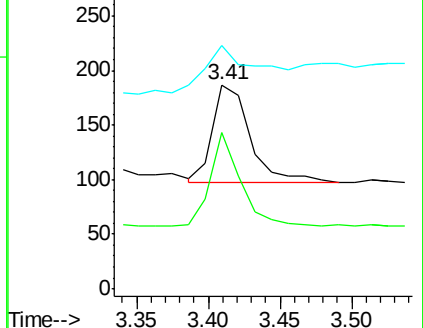







#3

n-Nitrosodimethylamine
Concen: 0.17 ng
RT: 3.78 min Scan# 103
Delta R.T. -0.01 min
Lab File: BE092324.D
Acq: 1 Sep 2016 12:07

Instrument :
BNA_E
ClientSampleId :
SSTDIC0.1




Tgt Ion: 42 Resp: 235
Ion Ratio Lower Upper
42 100
74 91.5 86.0 129.0
44 0.0 5.1 7.7#

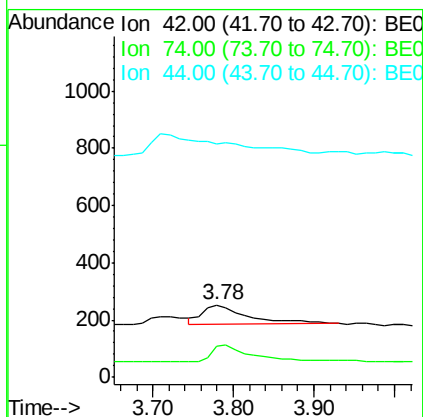


#4

2-Fluorophenol
Concen: 0.14 ng
RT: 5.68 min Scan# 364
Delta R.T. -0.01 min
Lab File: BE092324.D
Acq: 1 Sep 2016 12:07

Tgt Ion: 112 Resp: 302
Ion Ratio Lower Upper
112 100
64 67.2 53.5 80.3
63 36.8 27.9 41.9

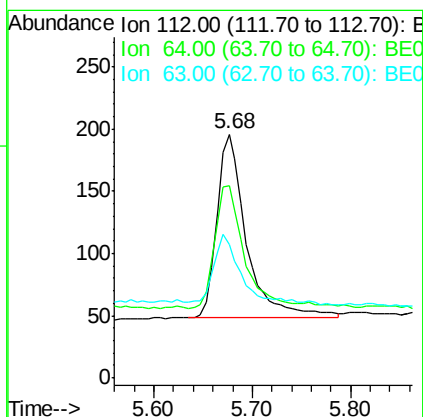

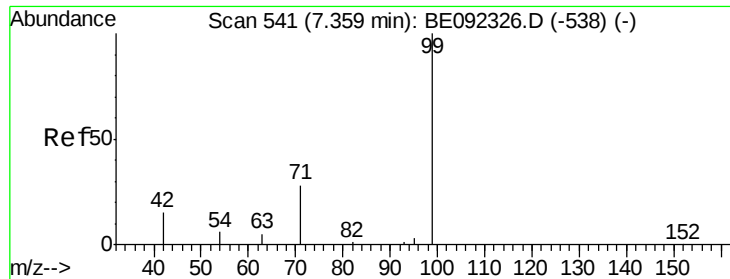

#5

Phenol-d6

Concen: 0.14 ng

RT: 7.36 min Scan# 541

Delta R.T. -0.00 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.1


Tgt Ion: 99 Resp: 397

Ion Ratio Lower Upper

99 100

42 0.0 0.0 0.0




71 0.0 30.6 45.8#

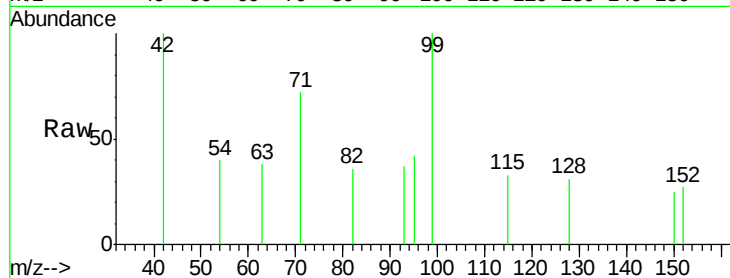

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

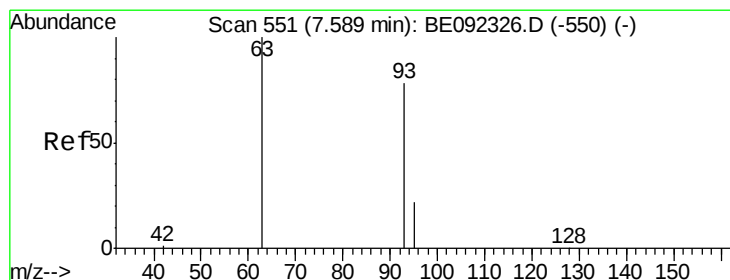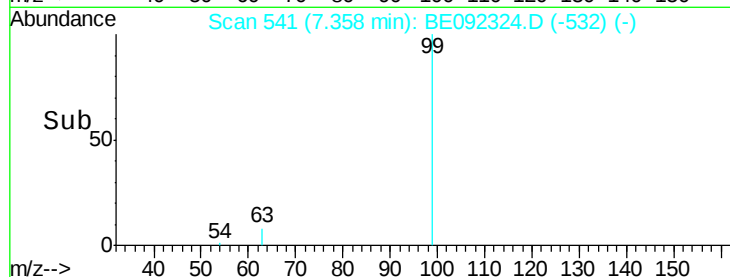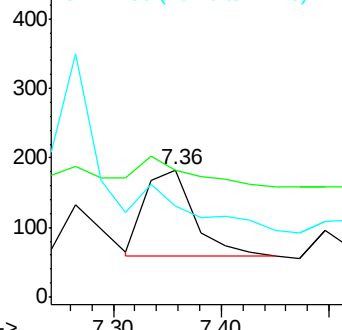

#6

bis(2-Chloroethyl)ether

Concen: 0.14 ng

RT: 7.59 min Scan# 551

Delta R.T. -0.00 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07


Tgt Ion: 93 Resp: 315

Ion Ratio Lower Upper

93 100

63 96.2 71.6 107.4



95 50.2 0.0 0.0#

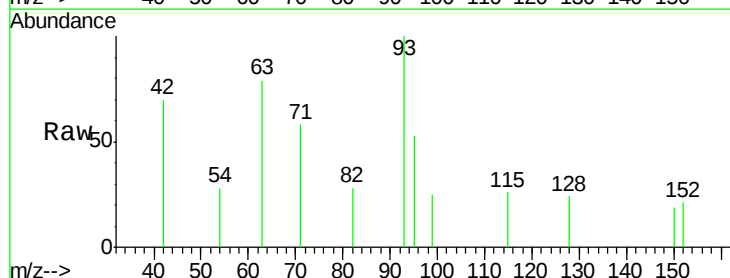


Abundance Ion 93.00 (92.70 to 93.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

Ion 95.00 (94.70 to 95.70): BE0

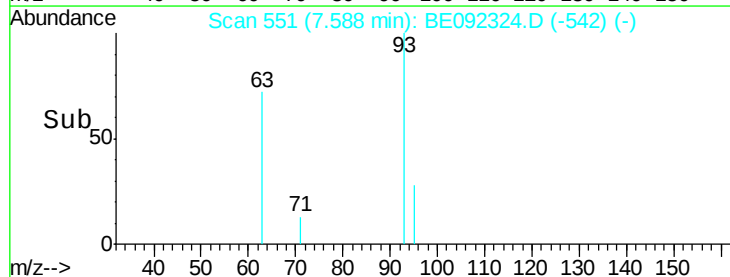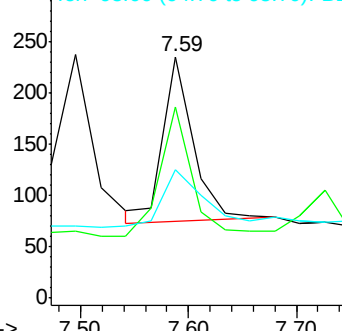



#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.95 min Scan# 708

Delta R.T. 0.00 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07


Instrument :

BNA_E

ClientSampleId :

SSTDIC0.1

Tgt Ion:	136	Resp:	44869
Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.2	12.4
54	8.4	9.6	14.4#
68	6.3	6.7	10.1#






Abundance

Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

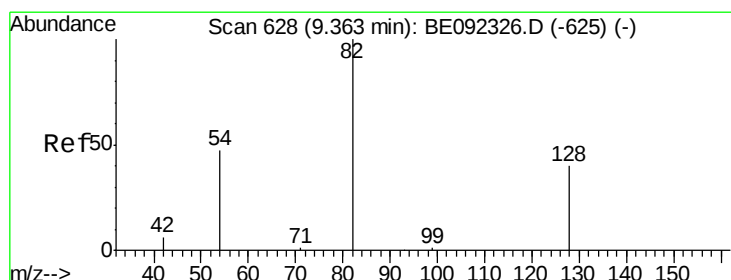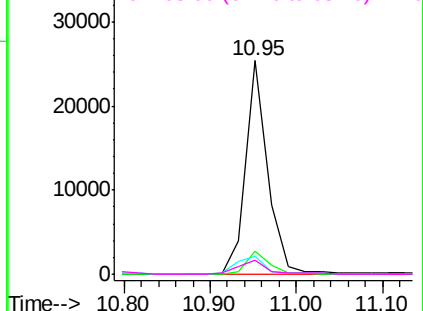

#8

Nitrobenzene-d5

Concen: 0.17 ng


RT: 9.34 min Scan# 627

Delta R.T. -0.02 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07

Tgt Ion:	82	Resp:	495
Ion	Ratio	Lower	Upper
82	100		
128	37.3	39.0	58.4#
54	76.0	44.8	67.2#






Abundance

Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0




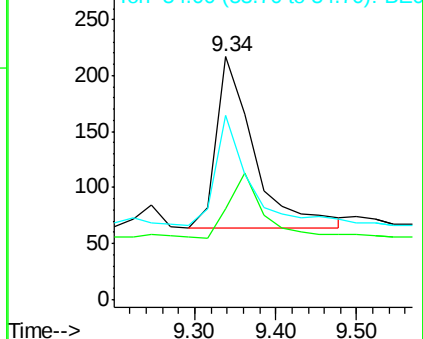




#9
Naphthalene
Concen: 0.12 ng
RT: 11.01 min Scan# 711
Delta R.T. 0.00 min
Lab File: BE092324.D
Acq: 1 Sep 2016 12:07




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.1


Tgt Ion:128 Resp: 1167
Ion Ratio Lower Upper
128 100
129 20.2 11.2 16.8#
127 19.1 11.6 17.4#

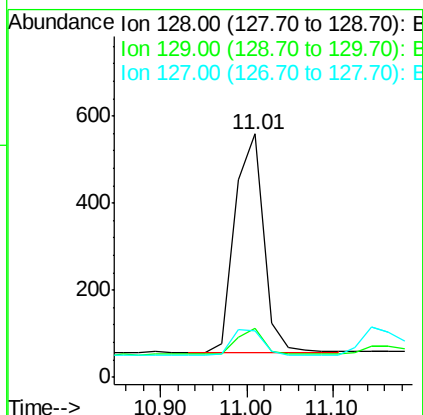

#10
Hexachlorobutadiene
Concen: 0.12 ng
RT: 11.30 min Scan# 726
Delta R.T. 0.00 min
Lab File: BE092324.D
Acq: 1 Sep 2016 12:07

Tgt Ion:225 Resp: 183
Ion Ratio Lower Upper
225 100
223 61.2 50.6 76.0
227 62.8 51.4 77.0

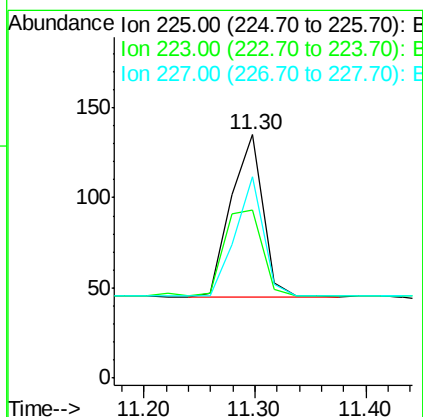

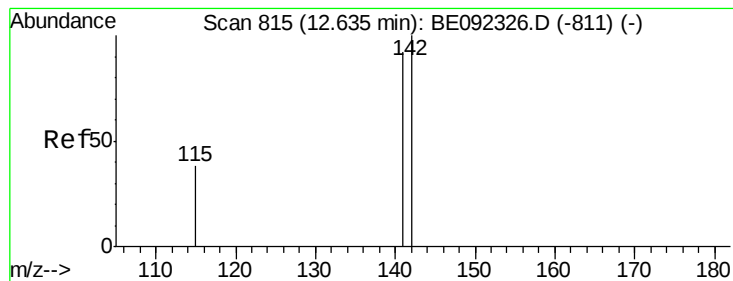

#11

2-Methylnaphthalene

Concen: 0.12 ng

RT: 12.64 min Scan# 815

Delta R.T. 0.00 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.1


Tgt Ion:142 Resp: 736

Ion Ratio Lower Upper

142 100

141 87.0 73.7 110.5




115 42.9 34.0 51.0

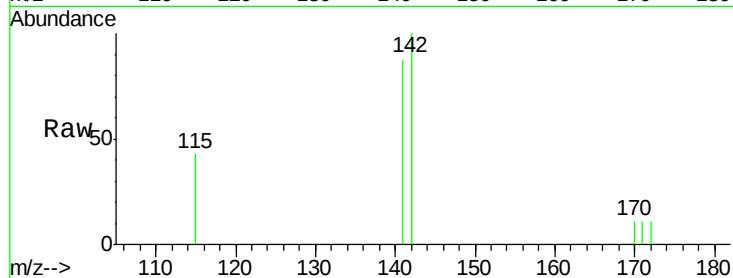

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

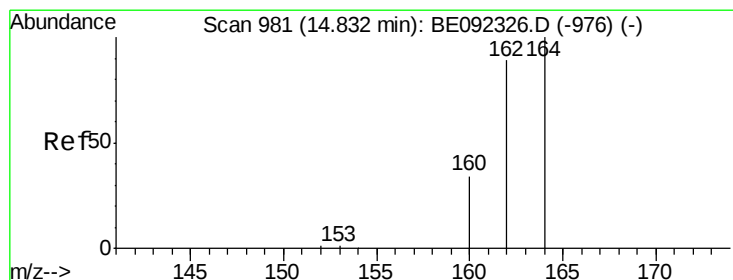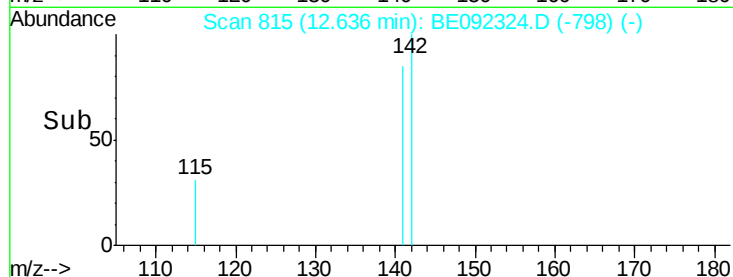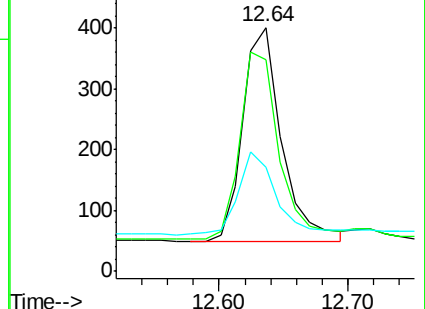

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.82 min Scan# 980

Delta R.T. -0.02 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07


Tgt Ion:164 Resp: 27509

Ion Ratio Lower Upper

164 100

162 117.5 71.4 107.0#



160 56.8 27.4 41.2#

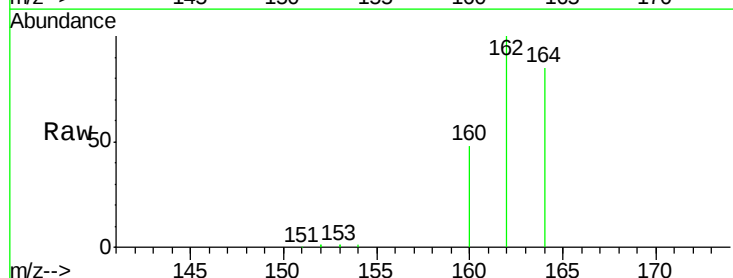


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



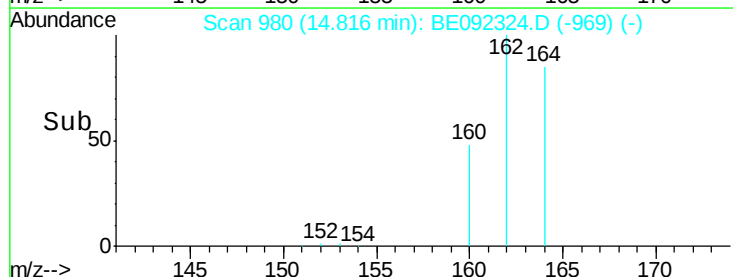
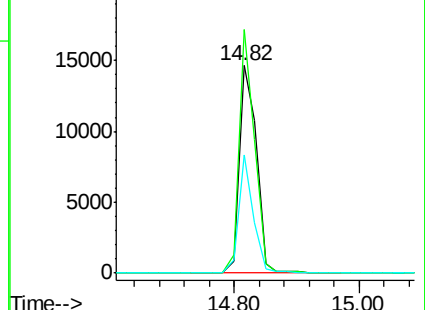


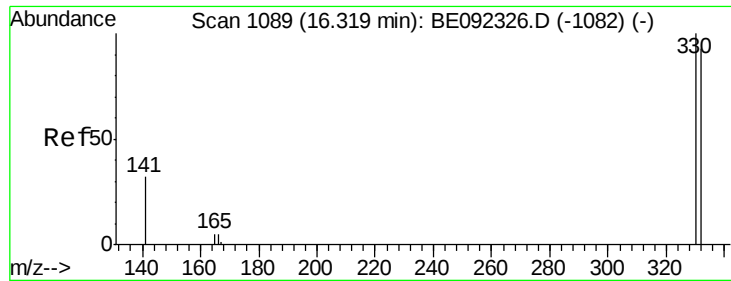

#13
 2,4,6-Tribromophenol
 Concen: 0.17 ng
 RT: 16.32 min Scan# 1089
 Delta R.T. 0.00 min
 Lab File: BE092324.D
 Acq: 1 Sep 2016 12:07




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.1


Tgt Ion: 330 Resp: 135
 Ion Ratio Lower Upper
 330 100
 332 94.1 75.4 113.0
 141 56.3 31.0 46.6#

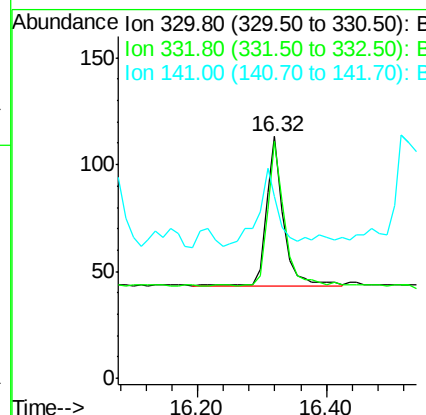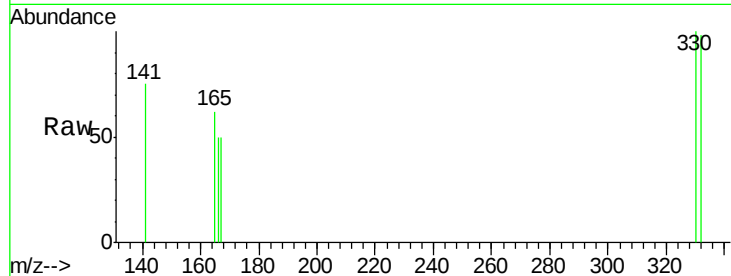

#14
 2-Fluorobiphenyl
 Concen: 0.12 ng
 RT: 13.45 min Scan# 885
 Delta R.T. 0.00 min
 Lab File: BE092324.D
 Acq: 1 Sep 2016 12:07

Tgt Ion: 172 Resp: 1025
 Ion Ratio Lower Upper
 172 100
 171 37.1 30.1 45.1
 170 25.7 21.8 32.6

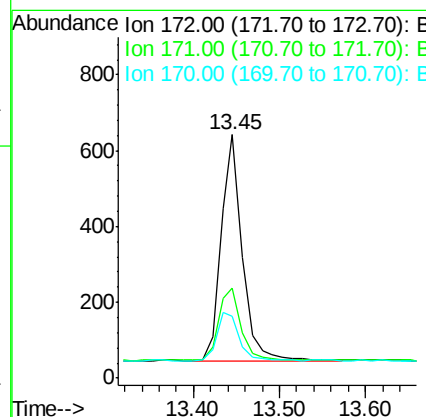

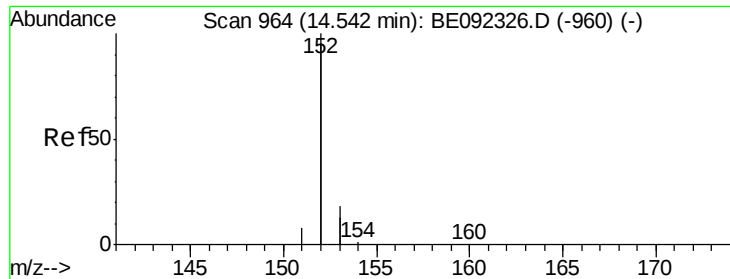

#15

Acenaphthylene

Concen: 0.12 ng

RT: 14.53 min Scan# 963

Delta R.T. -0.02 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.1


Tgt Ion:152 Resp: 5549

Ion Ratio Lower Upper

152 100

151 5.2 3.9 5.9




153 13.3 10.4 15.6

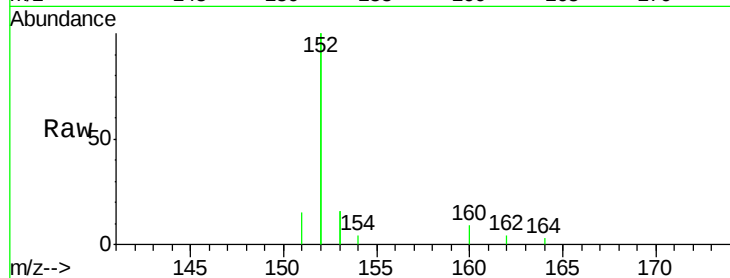

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

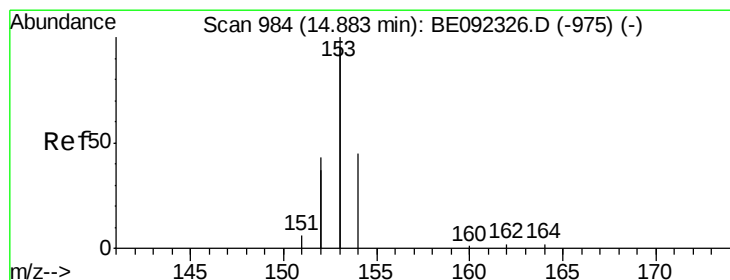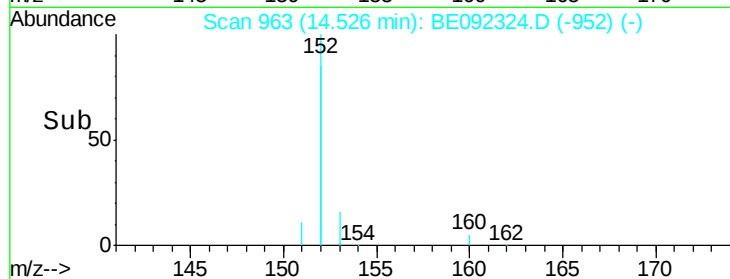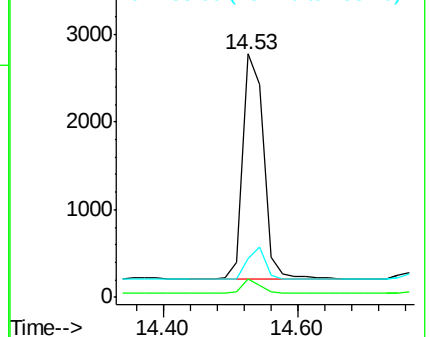

#16

Acenaphthene

Concen: 0.13 ng

RT: 14.88 min Scan# 984

Delta R.T. 0.00 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07


Tgt Ion:154 Resp: 1009

Ion Ratio Lower Upper

154 100

153 398.9 350.8 526.2



152 209.7 171.1 256.7

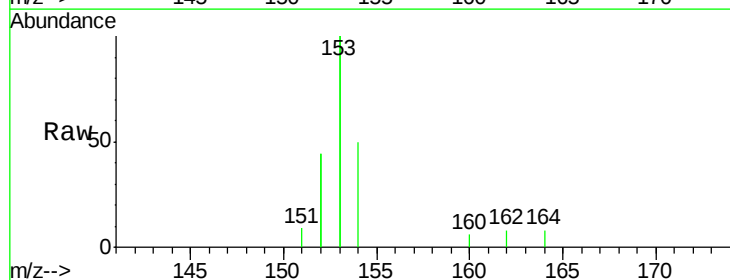


Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

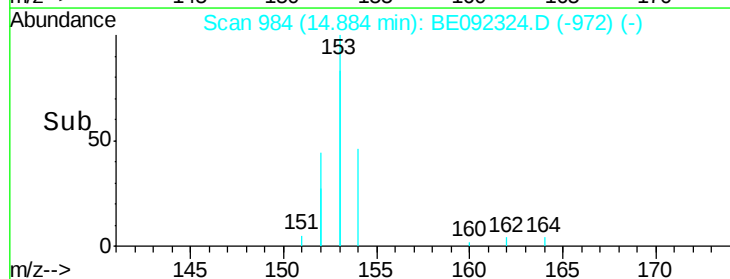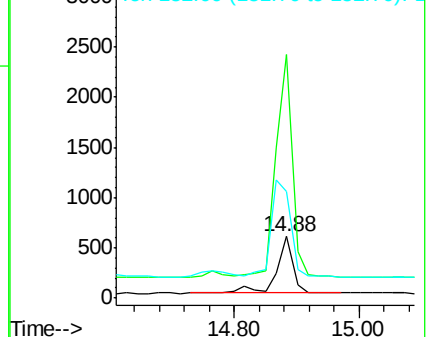

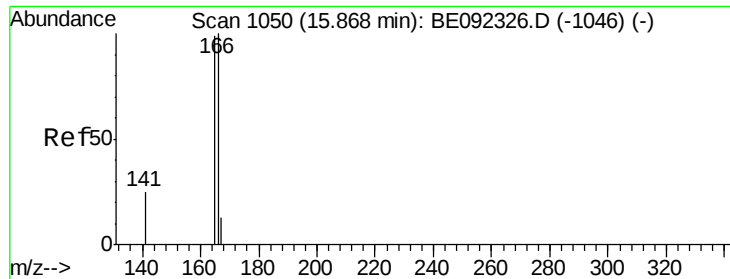

#17

Fluorene

Concen: 0.13 ng

RT: 15.87 min Scan# 1050

Delta R.T. 0.00 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.1


Tgt Ion:166 Resp: 1212

Ion Ratio Lower Upper

166 100

165 96.5 78.2 117.4


167 14.2 11.0 16.4

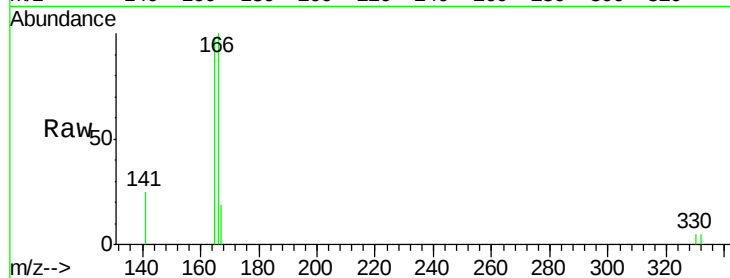



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

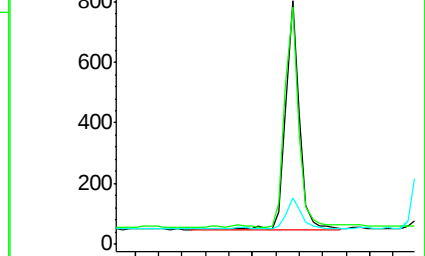

Time-->

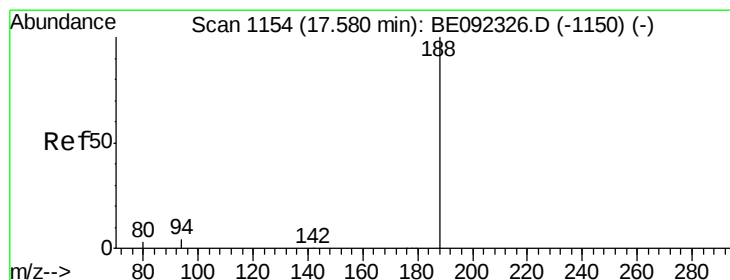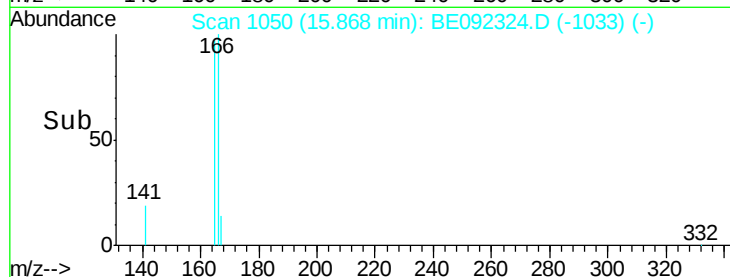

#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.58 min Scan# 1154

Delta R.T. -0.00 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07


Tgt Ion:188 Resp: 72712

Ion Ratio Lower Upper

188 100

94 4.1 3.2 4.8


80 3.4 2.6 3.8

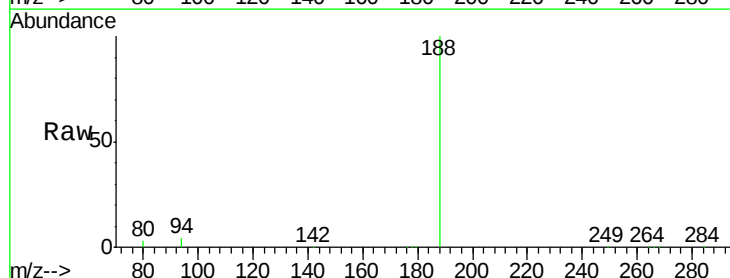


Abundance Ion 188.00 (187.70 to 188.70): E


Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

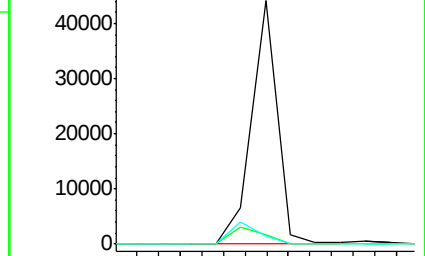

Time-->




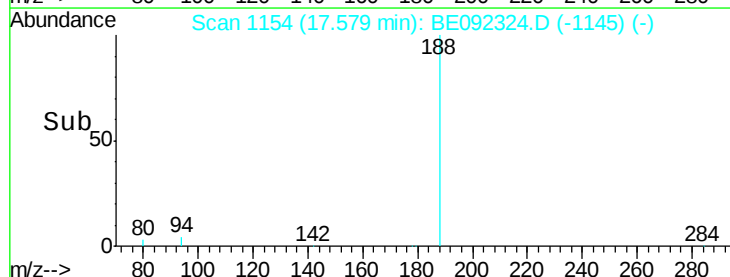




#19
Hexachlorobenzene
Concen: 0.13 ng
RT: 16.89 min Scan# 1124
Delta R.T. -0.00 min
Lab File: BE092324.D
Acq: 1 Sep 2016 12:07




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.1


Tgt Ion: 284 Resp: 382
Ion Ratio Lower Upper
284 100
142 38.7 29.1 43.7
249 36.1 27.9 41.9

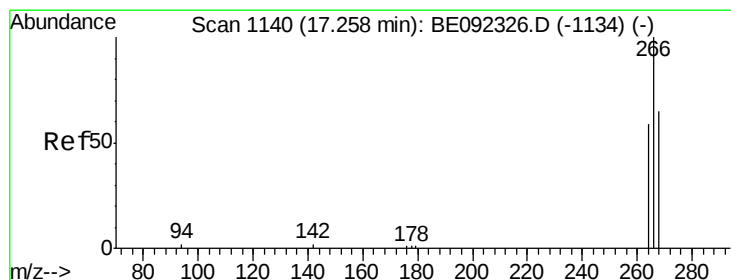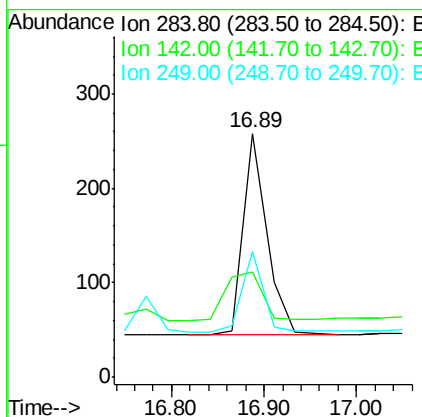

#20
Pentachlorophenol
Concen: 0.17 ng
RT: 17.26 min Scan# 1140
Delta R.T. -0.00 min
Lab File: BE092324.D
Acq: 1 Sep 2016 12:07

Tgt Ion: 266 Resp: 131
Ion Ratio Lower Upper
266 100
268 88.2 62.5 93.7
264 77.4 57.2 85.8

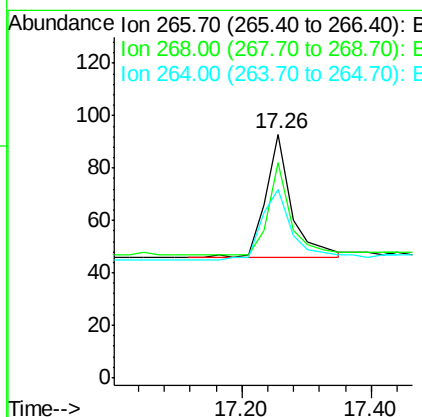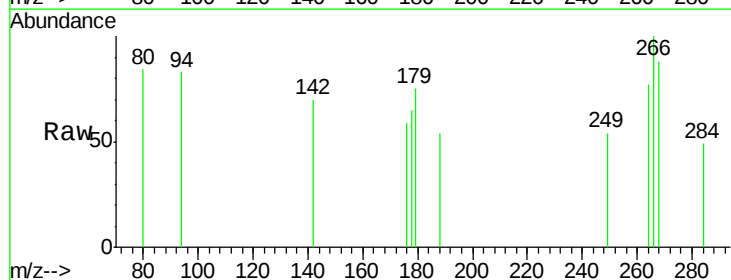



#21

Phenanthrene

Concen: 0.13 ng

RT: 17.62 min Scan# 1156

Delta R.T. 0.02 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07

Instrument :

BNA_E

ClientSampleId :

SSTDICC0.1


Tgt Ion:178 Resp: 2176

Ion Ratio Lower Upper

178 100

176 0.0 15.8 23.8#




179 19.2 0.0 0.0#



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

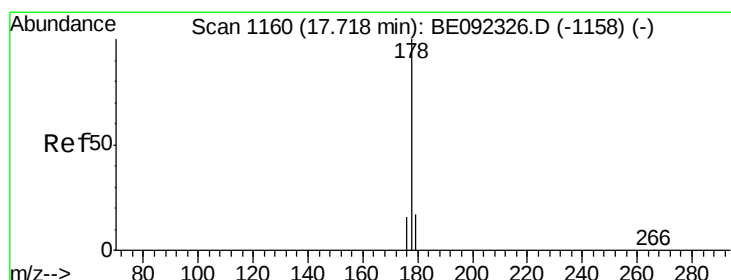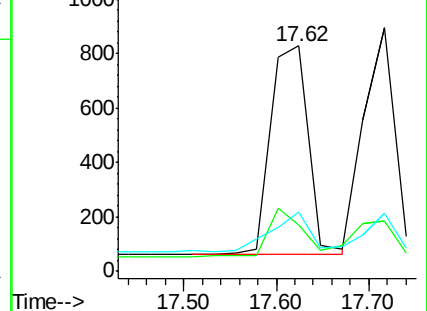

#22

Anthracene

Concen: 0.12 ng

RT: 17.72 min Scan# 1160

Delta R.T. -0.00 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07


Tgt Ion:178 Resp: 1955

Ion Ratio Lower Upper

178 100

176 21.1 15.0 22.4



179 14.6 12.2 18.2




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

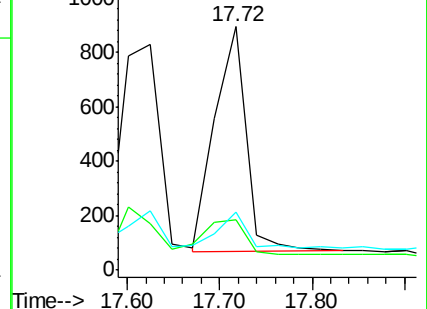

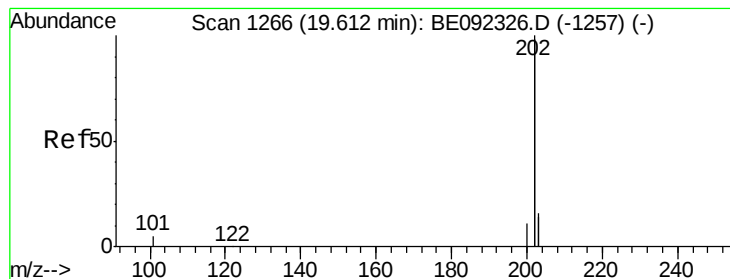

#23

Fluoranthene

Concen: 0.14 ng

RT: 19.61 min Scan# 1266

Delta R.T. -0.00 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.1


Tgt Ion:202 Resp: 11187

Ion Ratio Lower Upper

202 100

101 7.3 2.2 3.4#




203 20.0 13.7 20.5

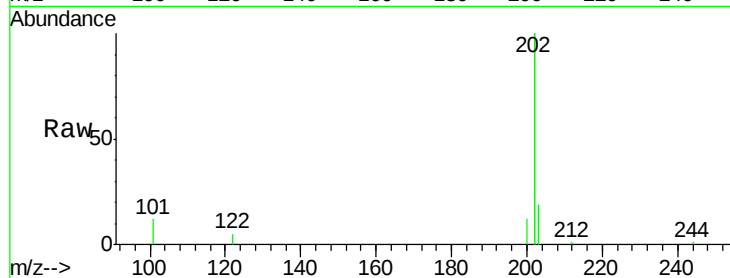

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

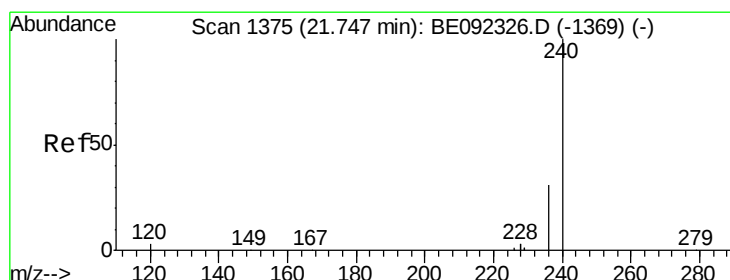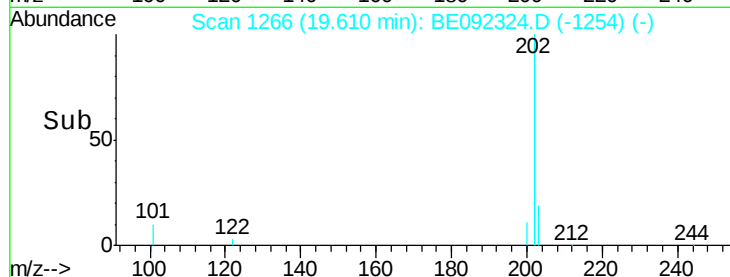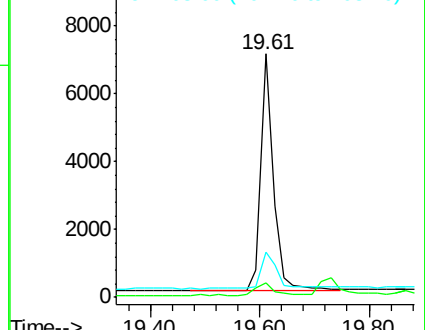

#24

Chrysene-d12

Concen: 5.00 ng

RT: 21.75 min Scan# 1375

Delta R.T. -0.00 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07


Tgt Ion:240 Resp: 89846

Ion Ratio Lower Upper

240 100

120 8.8 2.6 4.0#



236 32.8 24.6 37.0

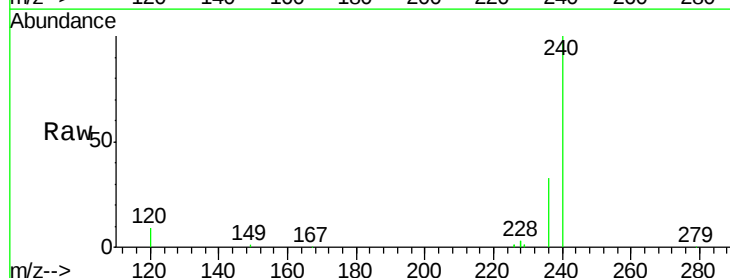


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

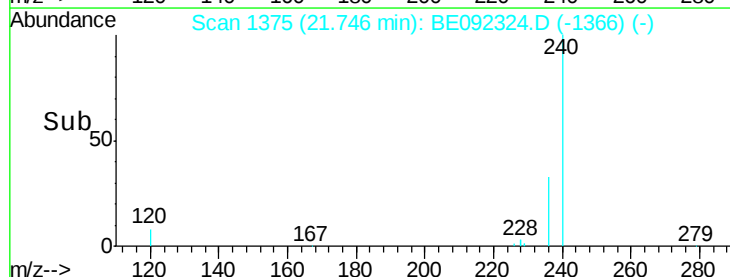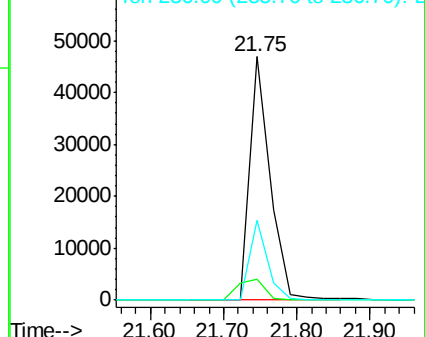



#25

Pyrene

Concen: 0.14 ng

RT: 19.97 min Scan# 1287

Delta R.T. -0.00 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.1





Tgt Ion:202 Resp: 11580

Ion Ratio Lower Upper

202 100

200 5.1 4.2 6.4

203 18.7 13.9 20.9

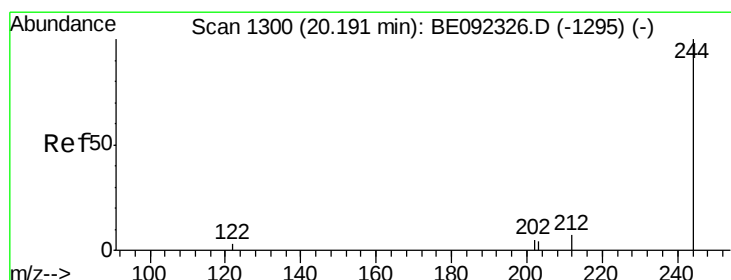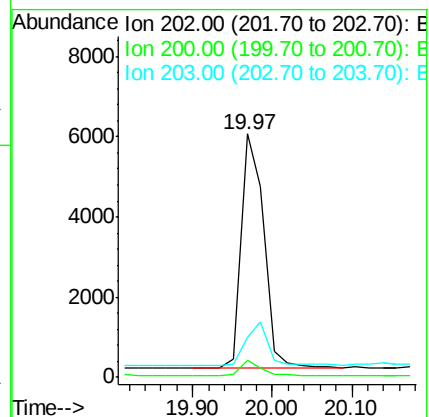

#26

Terphenyl-d14

Concen: 0.16 ng

RT: 20.19 min Scan# 1300

Delta R.T. -0.00 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07




Tgt Ion:244 Resp: 1877


Ion Ratio Lower Upper

244 100

212 10.9 6.7 10.1#

122 10.1 3.6 5.4#



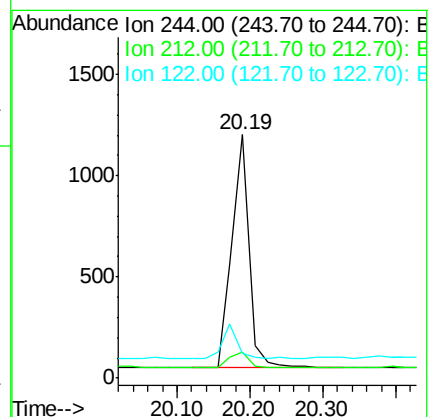





#27
Benzo(a)anthracene
Concen: 0.17 ng
RT: 21.72 min Scan# 1374
Delta R.T. -0.00 min
Lab File: BE092324.D
Acq: 1 Sep 2016 12:07




Instrument :
BNA_E
ClientSampleId :
SSTDIC0.1


Tgt Ion:228 Resp: 16335
Ion Ratio Lower Upper
228 100
226 37.9 23.6 35.4#
229 16.3 13.3 19.9

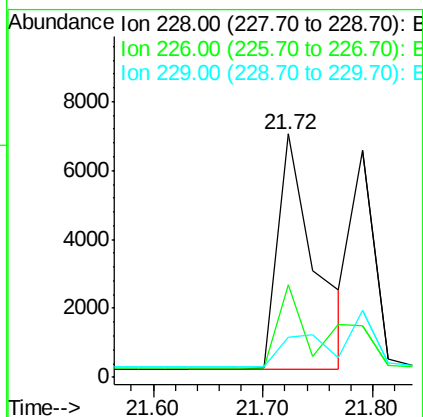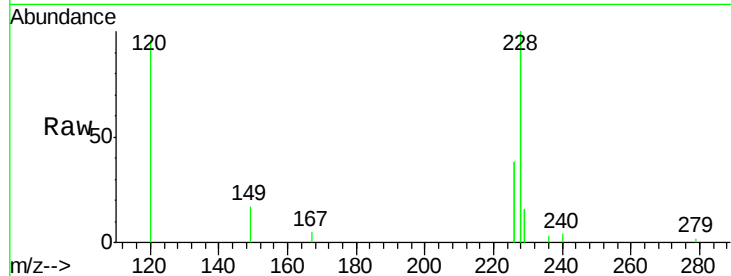

#28
Chrysene
Concen: 0.19 ng
RT: 21.72 min Scan# 1374
Delta R.T. -0.05 min
Lab File: BE092324.D
Acq: 1 Sep 2016 12:07

Tgt Ion:228 Resp: 16335
Ion Ratio Lower Upper
228 100
226 37.9 36.3 54.5
229 16.3 10.6 16.0#

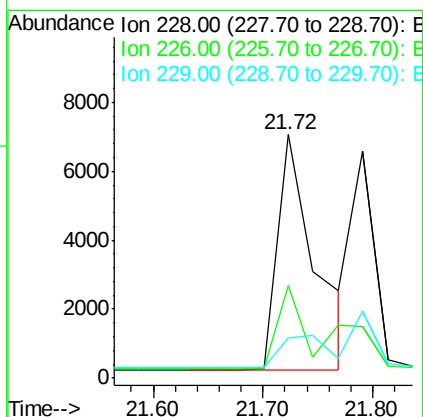



#29

Bis(2-ethylhexyl)phthalate

Concen: 11.96 ng

RT: 21.66 min Scan# 1371

Delta R.T. 0.02 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.1





Tgt Ion:149 Resp: 77008

Ion Ratio Lower Upper

149 100

167 31.3 0.0 0.0#

279 0.0 0.0 0.0

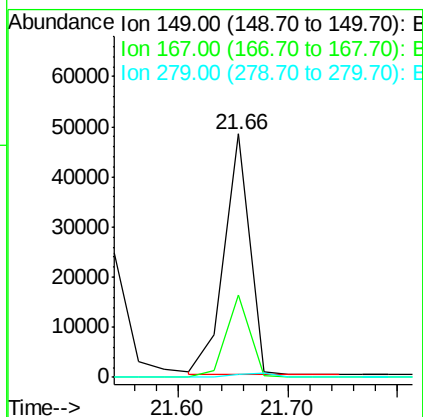

#30

Indeno(1,2,3-cd)pyrene

Concen: 0.15 ng

RT: 26.63 min Scan# 1718

Delta R.T. 0.02 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07




Tgt Ion:276 Resp: 13209


Ion Ratio Lower Upper

276 100

138 27.1 20.3 30.5

277 24.8 19.7 29.5



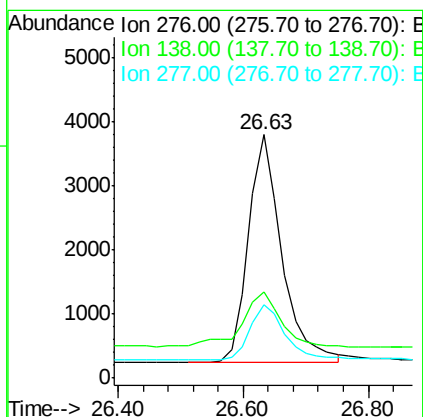



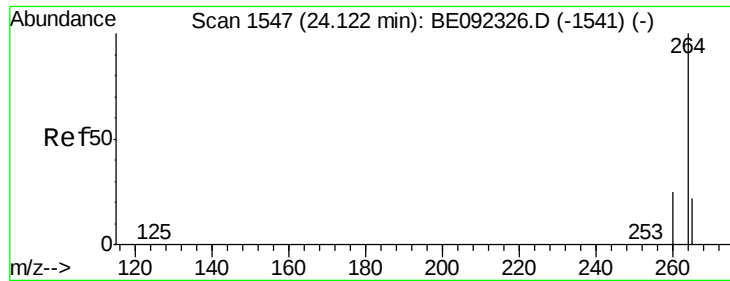

#31
Perylene-d12
 Concen: 5.00 ng
 RT: 24.12 min Scan# 1547
 Delta R.T. 0.00 min
 Lab File: BE092324.D
 Acq: 1 Sep 2016 12:07




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.1


Tgt Ion: 264 Resp: 97751
 Ion Ratio Lower Upper
 264 100
 260 26.0 20.1 30.1
 265 21.4 17.9 26.9

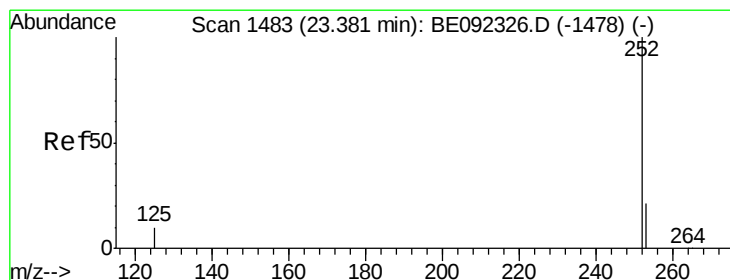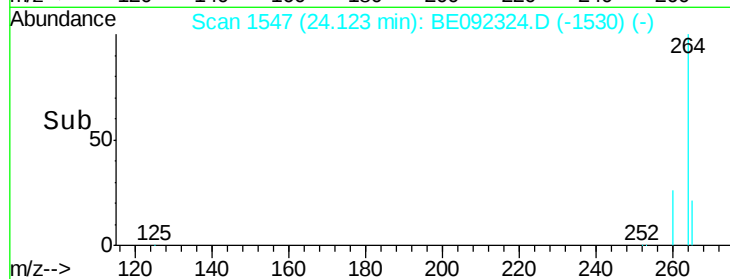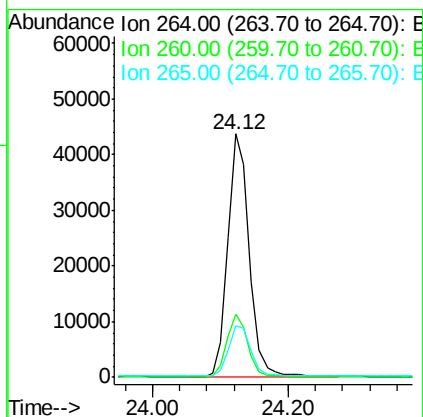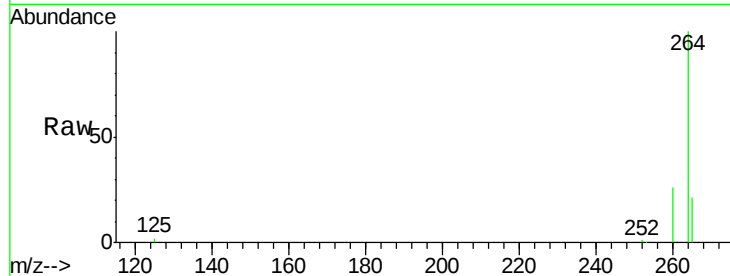

#32
Benzo(b)fluoranthene
 Concen: 0.14 ng
 RT: 23.39 min Scan# 1484
 Delta R.T. 0.01 min
 Lab File: BE092324.D
 Acq: 1 Sep 2016 12:07

Tgt Ion: 252 Resp: 3201
 Ion Ratio Lower Upper
 252 100
 253 30.1 18.7 28.1#
 125 62.8 10.5 15.7#

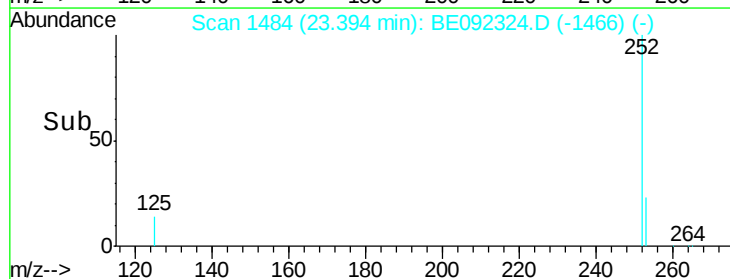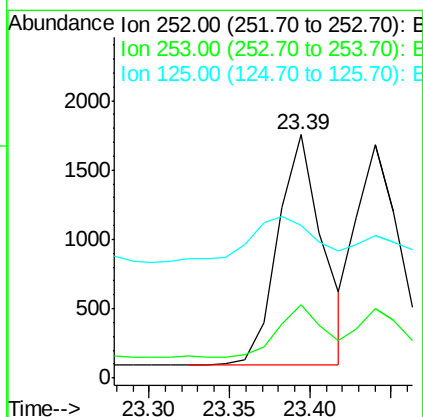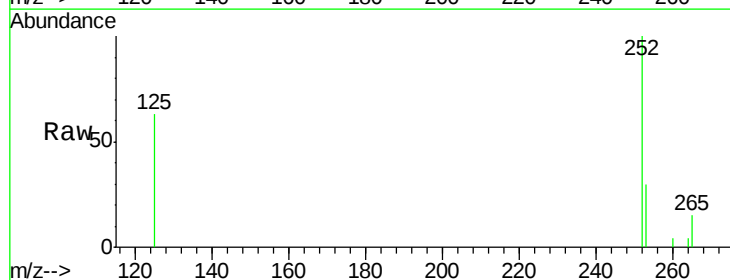



#33

Benzo(k)fluoranthene

Concen: 0.12 ng

RT: 23.44 min Scan# 1488

Delta R.T. 0.00 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07

Instrument :

BNA_E

ClientSampleId :

SSTDICC0.1


Tgt Ion:252 Resp: 3199

Ion Ratio Lower Upper

252 100

253 29.7 20.3 30.5




125 61.3 9.6 14.4#

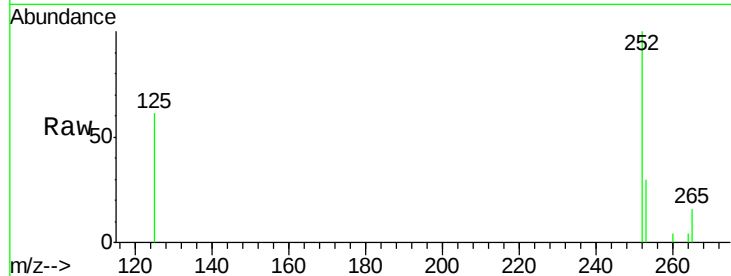

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

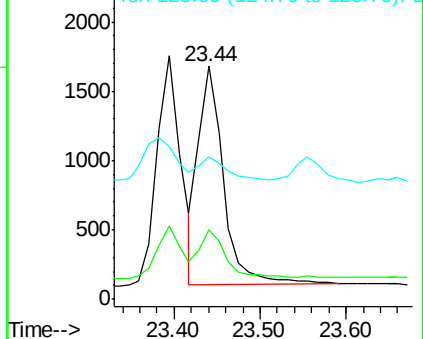

#34

Benzo(a)pyrene

Concen: 0.13 ng

RT: 24.02 min Scan# 1538

Delta R.T. 0.01 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07


Tgt Ion:252 Resp: 2988

Ion Ratio Lower Upper

252 100

253 32.7 19.0 28.6#



125 77.3 11.8 17.8#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

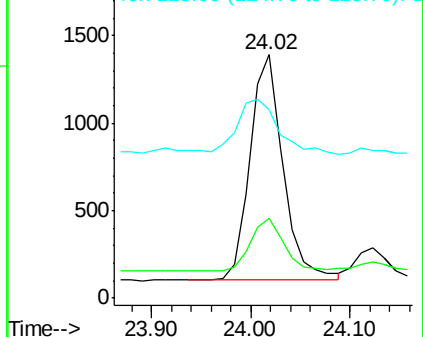



#35

Dibenzo(a,h)anthracene

Concen: 0.13 ng

RT: 26.65 min Scan# 1719

Delta R.T. -0.00 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07

Instrument :

BNA_E

ClientSampleId :

SSTDIC0.1


Tgt Ion: 278 Resp: 2691

Ion Ratio Lower Upper

278 100

139 43.4 13.8 20.8#




279 31.9 21.4 32.2

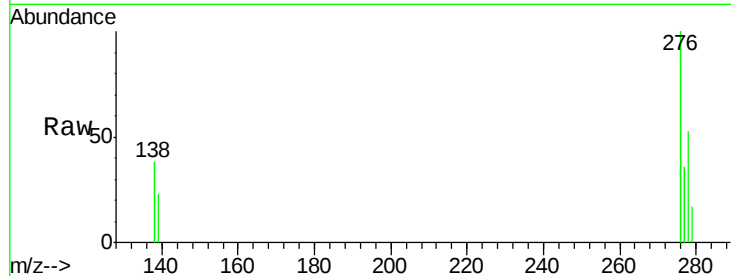

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

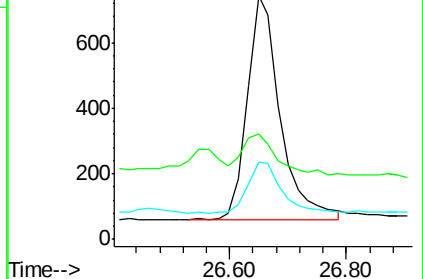

#36

Benzo(g,h,i)perylene

Concen: 0.12 ng

RT: 27.40 min Scan# 1763

Delta R.T. 0.02 min

Lab File: BE092324.D

Acq: 1 Sep 2016 12:07


Tgt Ion: 276 Resp: 11338

Ion Ratio Lower Upper

276 100

277 29.7 19.8 29.8

138 33.6 19.8 29.6#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

