
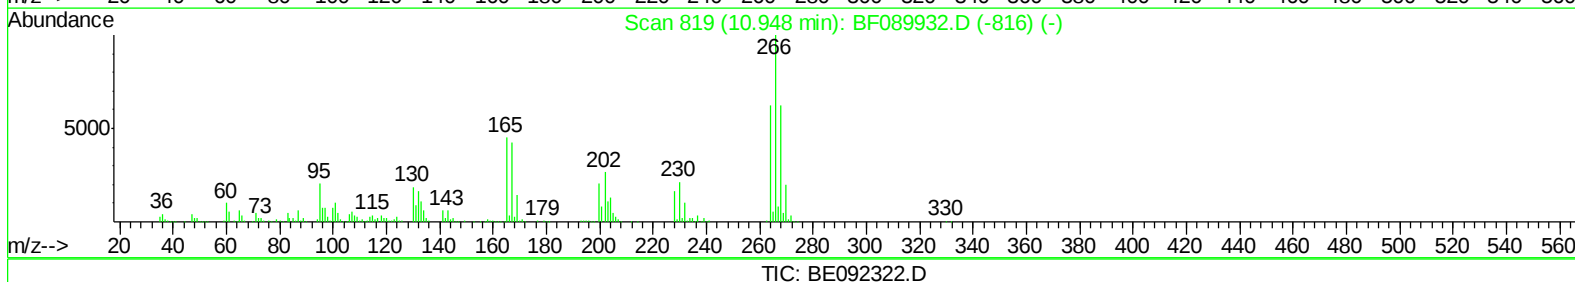
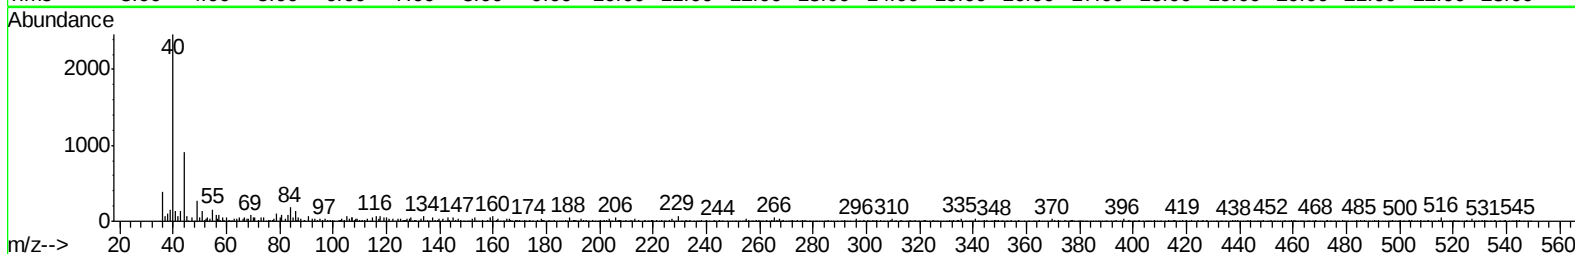


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE090116\
Data File : BE092322.D
Acq On : 1 Sep 2016 9:32
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 05:45:50 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 11:55:18 2016
Response via : Initial Calibration

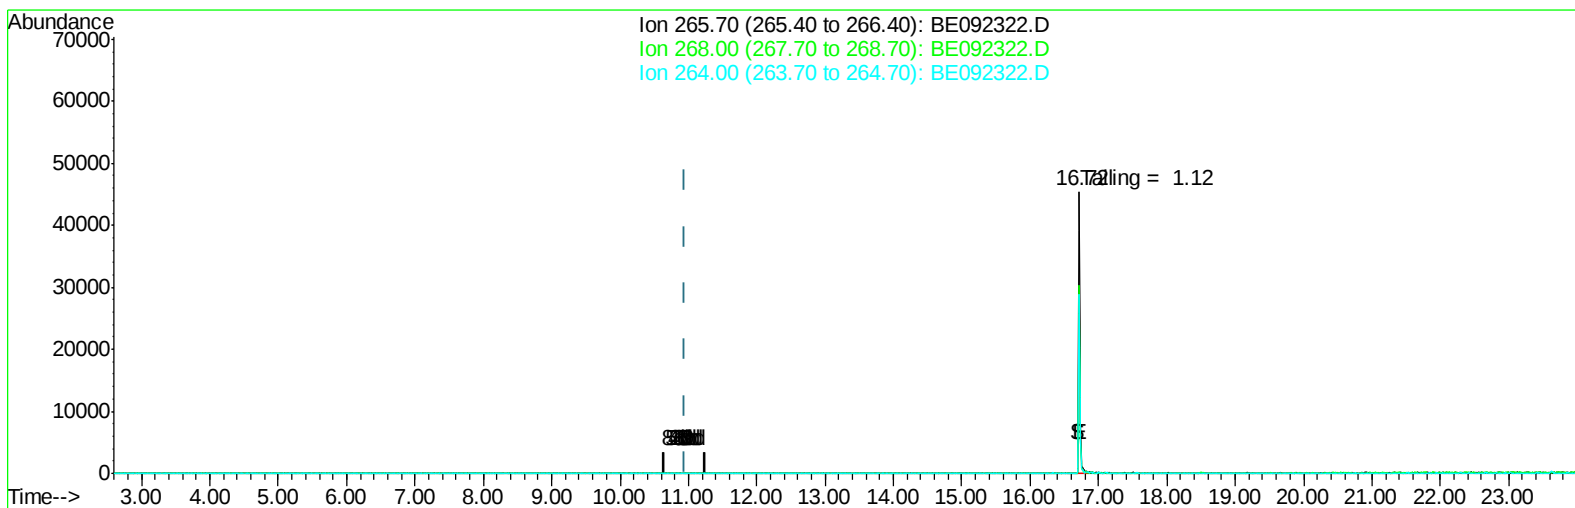




TIC: BE092322.D

(69) Pentachlorophenol (C)
10.925min (-0.022) 200.13ng
response 26

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	15.22#
264.00	63.20	19.57#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE090116\
Data File : BE092322.D
Acq On : 1 Sep 2016 9:32
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 05:45:50 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 11:55:18 2016
Response via : Initial Calibration

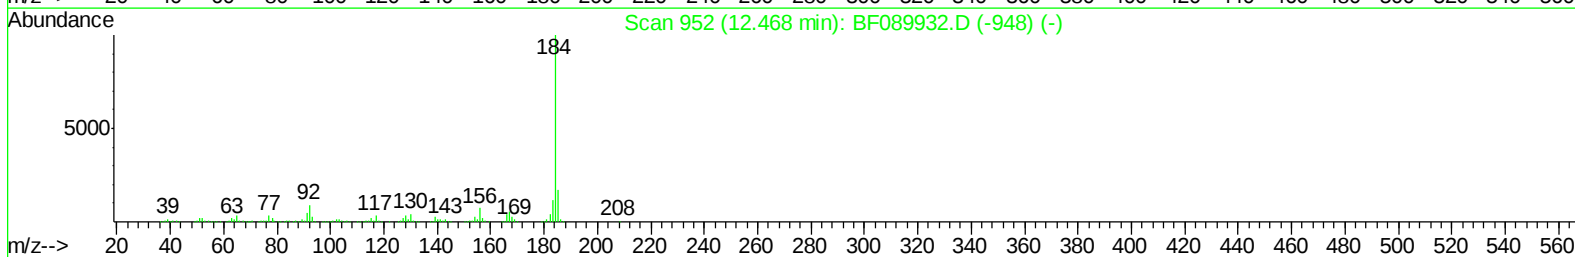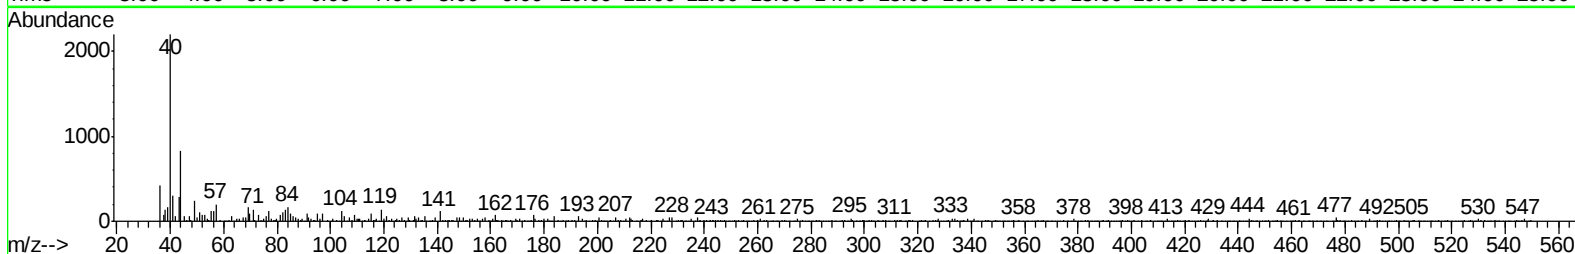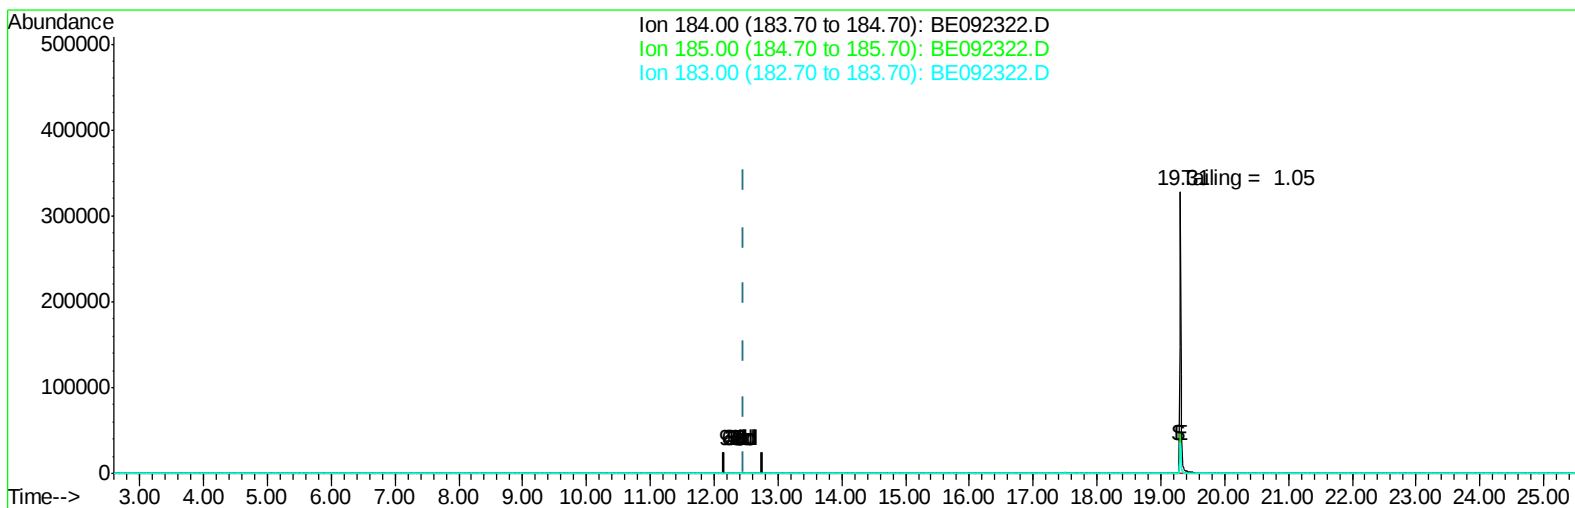

TIC: BE092322.D

(76) Benzidine

12.388min (-0.080) 62.69ng

response 38

Ion	Exp%	Act%
184.00	100	100
185.00	17.30	21.82#
183.00	12.00	0.00#
0.00	0.00	0.00