

Data Path : Z:\HPCHEM1\BNA E\DATA\BE090116\
 Data File : BE092328.D
 Acq On : 1 Sep 2016 14:33
 Operator : UM/SJ
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC1.6

Manual Integrations
 APPROVED

sohil
 9/2/2016 4:33:55 PM

Quant Time: Sep 02 03:22:09 2016
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE090116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 02 03:16:21 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.19	152	8484	5.00	ng	0.00
7) Naphthalene-d8	10.95	136	42145	5.00	ng	0.00
12) Acenaphthene-d10	14.81	164	25777	5.00	ng	-0.02
18) Phenanthrene-d10	17.58	188	65606	5.00	ng	0.00
24) Chrysene-d12	21.75	240	91855	5.00	ng	0.00
31) Perylene-d12	24.12	264	84841	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.68	112	3640	1.86	ng	-0.01
5) Phenol-d6	7.34	99	4912	1.91	ng	-0.02
8) Nitrobenzene-d5	9.34	82	4838	1.73	ng	-0.02
13) 2,4,6-Tribromophenol	16.31	330	1588	2.16	ng	-0.01
14) 2-Fluorobiphenyl	13.44	172	12741	1.59	ng	0.00
26) Terphenyl-d14	20.17	244	20099	1.62	ng	-0.02
Target Compounds						
2) 1,4-Dioxane	3.42	88	1778	1.49	ng	Qvalue 94
3) n-Nitrosodimethylamine	3.77	42	2306	1.82	ng	# 99
6) bis(2-Chloroethyl)ether	7.59	93	4196	2.09	ng	# 93
9) Naphthalene	11.01	128	14645	1.57	ng	95
10) Hexachlorobutadiene	11.30	225	2356	1.66	ng	99
11) 2-Methylnaphthalene	12.63	142	9931	1.71	ng	# 86
15) Acenaphthylene	14.53	152	72014	1.64	ng	100
16) Acenaphthene	14.88	154	11009	1.54	ng	96
17) Fluorene	15.87	166	14593	1.67	ng	99
19) Hexachlorobenzene	16.89	284	4454	1.64	ng	# 66
20) Pentachlorophenol	17.23	266	1454	2.13	ng	# 83
21) Phenanthrene	17.60	178	23543	1.52	ng	# 100
22) Anthracene	17.69	178	23578	1.65	ng	# 83
23) Fluoranthene	19.61	202	123495	1.75	ng	100
25) Pyrene	19.97	202	131774	1.55	ng	99
27) Benzo(a)anthracene	21.72	228	162518m	1.68	ng	
28) Chrysene	21.77	228	138128m	1.61	ng	
29) Bis(2-ethylhexyl)phthalate	21.63	149	14487	2.20	ng	# 100
30) Indeno(1,2,3-cd)pyrene	26.62	276	161242	1.80	ng	100
32) Benzo(b)fluoranthene	23.38	252	36241	1.81	ng	# 96
33) Benzo(k)fluoranthene	23.43	252	36108	1.58	ng	93
34) Benzo(a)pyrene	24.01	252	34225	1.69	ng	# 95
35) Dibenzo(a,h)anthracene	26.63	278	33204	1.84	ng	95
36) Benzo(g,h,i)perylene	27.38	276	136629	1.72	ng	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE090116\
Data File : BE092328.D
Acq On : 1 Sep 2016 14:33
Operator : UM/SJ
Sample : SSTDIC1.6
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
SSTDIC1.6

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:55 PM

Quant Time: Sep 02 03:22:09 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE090116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 03:16:21 2016
Response via : Initial Calibration



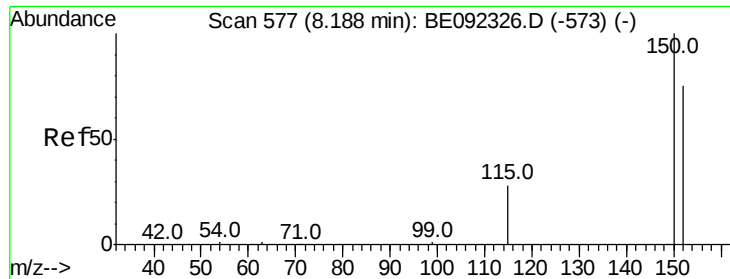

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.19 min Scan# 577

Delta R.T. -0.00 min

Lab File: BE092328.D

Acq: 1 Sep 2016 14:33

Instrument :

BNA_E





ClientSampleId :

SSTDICC1.6

Tot Ion	Ratio	Lower	Upper
152	100		
150	132.1	106.0	159.0
115	36.5	31.2	46.8

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:55 PM



#2

1,4-Dioxane

Concen: 1.49 ng




RT: 3.42 min Scan# 72


Delta R.T. -0.00 min

Lab File: BE092328.D

Acq: 1 Sep 2016 14:33

Tgt Ion	Ratio	Lower	Upper
88	100		
58	85.9	63.6	95.4
43	37.5	28.0	42.0





#3





n-Nitrosodimethylamine
 Concen: 1.82 ng
 RT: 3.77 min Scan# 102
 Delta R.T. -0.02 min
 Lab File: BE092328.D
 Acq: 1 Sep 2016 14:33

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC1.6

Tot Ion	Ratio	Lower	Upper
42	100		
74	107.8	86.0	129.0
44	7.9	5.1	7.7#

Manual Integrations
 APPROVED




sohil
 9/2/2016 4:33:55 PM




#4

2-Fluorophenol
 Concen: 1.86 ng
 RT: 5.68 min Scan# 364
 Delta R.T. -0.01 min
 Lab File: BE092328.D
 Acq: 1 Sep 2016 14:33

Tgt Ion	Ratio	Lower	Upper
112	100		
64	67.2	53.5	80.3
63	35.4	27.9	41.9





#5

Phenol-d6

Concen: 1.91 ng

RT: 7.34 min Scan# 540

Delta R.T. -0.02 min

Lab File: BE092328.D

Acq: 1 Sep 2016 14:33

Instrument :

BNA_E





ClientSampled :

SSTDICC1.6

Tot Ion	Ratio	Resp	Lower	Upper
99	100	4912		
42	24.4		0.0	0.0#
71	36.5		30.6	45.8

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:55 PM



#6

bis(2-Chloroethyl)ether

Concen: 2.09 ng




RT: 7.59 min Scan# 551


Delta R.T. -0.00 min

Lab File: BE092328.D

Acq: 1 Sep 2016 14:33

Tgt Ion	Ratio	Resp	Lower	Upper
93	100	4196		
63	82.9		71.6	107.4
95	32.4		0.0	0.0#





#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.95 min Scan# 708

Delta R.T. -0.00 min

Lab File: BE092328.D

Acq: 1 Sep 2016 14:33

Instrument :

BNA_E


ClientSampleId :

SSTDICC1.6

Tot Ion	Ratio	Resp	Lower	Upper
136	100	42145		
137	10.5		8.2	12.4
54	10.6		9.6	14.4
68	7.7		6.7	10.1

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:55 PM






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0



#8

Nitrobenzene-d5

Concen: 1.73 ng


RT: 9.34 min Scan# 627

Delta R.T. -0.02 min

Lab File: BE092328.D

Acq: 1 Sep 2016 14:33



Tgt Ion	Ratio	Resp	Lower	Upper
82	100	4838		
128	24.2		39.0	58.4#
54	58.1		44.8	67.2




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0





#9

Naphthalene

Concen: 1.57 ng

RT: 11.01 min Scan# 711

Delta R.T. -0.00 min

Lab File: BE092328.D

Acq: 1 Sep 2016 14:33

Instrument :

BNA_E


ClientSampleId :

SSTDICC1.6




Tot Ion:	128	Resp:	14645
Ion Ratio	Lower	Upper	
128	100		
129	12.2	11.2	16.8
127	12.3	11.6	17.4

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:55 PM



Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E



#10

Hexachlorobutadiene

Concen: 1.66 ng

RT: 11.30 min Scan# 726




Delta R.T. -0.00 min


Lab File: BE092328.D

Acq: 1 Sep 2016 14:33

Tgt Ion:	225	Resp:	2356
Ion Ratio	Lower	Upper	
225	100		
223	61.5	50.6	76.0
227	63.9	51.4	77.0

Abundance Ion 225.00 (224.70 to 225.70): E
Ion 223.00 (222.70 to 223.70): E
Ion 227.00 (226.70 to 227.70): E



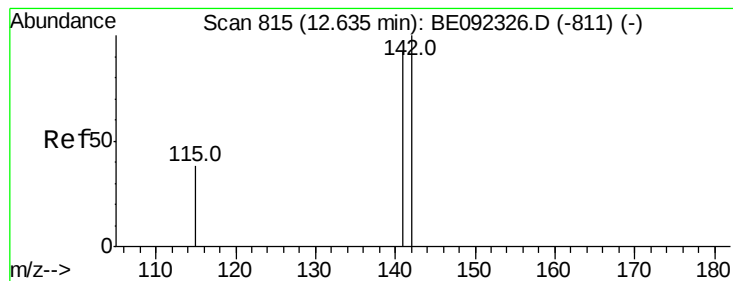

#11

2-Methylnaphthalene

Concen: 1.71 ng

RT: 12.63 min Scan# 815

Delta R.T. 0.00 min

Lab File: BE092328.D

Acq: 1 Sep 2016 14:33

Instrument :

BNA_E

ClientSampleId :





SSTDICC1.6

Tot Ion:142 Resp: 9931

Ion	Ratio	Lower	Upper
142	100		
141	81.3	73.7	110.5
115	30.6	34.0	51.0#

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:55 PM



#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.81 min Scan# 980




Delta R.T. -0.02 min


Lab File: BE092328.D

Acq: 1 Sep 2016 14:33

Tgt Ion:164 Resp: 25777

Ion	Ratio	Lower	Upper
164	100		
162	117.5	71.4	107.0#
160	59.6	27.4	41.2#









#13
 2,4,6-Tribromophenol
 Concen: 2.16 ng
 RT: 16.31 min Scan# 1088
 Delta R.T. -0.01 min
 Lab File: BE092328.D
 Acq: 1 Sep 2016 14:33

Instrument :
 BNA_E
 ClientSampled :
 SSTDICC1.6

Tot Ion:330 Resp: 1588
 Ion Ratio Lower Upper
 330 100
 332 95.5 75.4 113.0
 141 40.8 31.0 46.6




Manual Integrations
 APPROVED


sohil
 9/2/2016 4:33:55 PM



#14
 2-Fluorobiphenyl
 Concen: 1.59 ng
 RT: 13.44 min Scan# 885
 Delta R.T. 0.00 min
 Lab File: BE092328.D
 Acq: 1 Sep 2016 14:33

Tgt Ion:172 Resp: 12741
 Ion Ratio Lower Upper
 172 100
 171 32.3 30.1 45.1
 170 20.1 21.8 32.6#





#15

Acenaphthylene

Concen: 1.64 ng

RT: 14.53 min Scan# 963

Delta R.T. -0.02 min

Lab File: BE092328.D

Acq: 1 Sep 2016 14:33

Instrument :

BNA_E





ClientSampleId :

SSTDICC1.6

Tot Ion:	152	Resp:	72014
Ion Ratio	Lower	Upper	
152	100		
151	4.9	3.9	5.9
153	13.1	10.4	15.6

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:55 PM



#16

Acenaphthene

Concen: 1.54 ng




RT: 14.88 min Scan# 984


Delta R.T. -0.00 min

Lab File: BE092328.D

Acq: 1 Sep 2016 14:33

Tgt Ion:	154	Resp:	11009
Ion Ratio	Lower	Upper	
154	100		
153	448.9	350.8	526.2
152	221.0	171.1	256.7









#17
Fluorene
 Concen: 1.67 ng
 RT: 15.87 min Scan# 1050
 Delta R.T. 0.00 min
 Lab File: BE092328.D
 Acq: 1 Sep 2016 14:33

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC1.6

Tot Ion	Ratio	Lower	Upper
166	100		
165	98.8	78.2	117.4
167	13.5	11.0	16.4




Manual Integrations
 APPROVED


sohil
 9/2/2016 4:33:55 PM



#18
Phenanthrene-d10
 Concen: 5.00 ng
 RT: 17.58 min Scan# 1154
 Delta R.T. -0.00 min
 Lab File: BE092328.D
 Acq: 1 Sep 2016 14:33

Tgt Ion	Ratio	Lower	Upper
188	100		
94	3.8	3.2	4.8
80	3.1	2.6	3.8









#19
Hexachlorobenzene
Concen: 1.64 ng
RT: 16.89 min Scan# 1124
Delta R.T. -0.00 min
Lab File: BE092328.D
Acq: 1 Sep 2016 14:33

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

Tot Ion	Ratio	Lower	Upper
284	100		
142	0.0	29.1	43.7#
249	32.1	27.9	41.9




Manual Integrations
APPROVED


sohil
9/2/2016 4:33:55 PM



#20
Pentachlorophenol
Concen: 2.13 ng
RT: 17.23 min Scan# 1139
Delta R.T. -0.03 min
Lab File: BE092328.D
Acq: 1 Sep 2016 14:33

Tgt Ion	Ratio	Lower	Upper
266	100		
268	54.8	62.5	93.7#
264	77.5	57.2	85.8









#21
Phenanthrene
Concen: 1.52 ng
RT: 17.60 min Scan# 1155
Delta R.T. -0.00 min
Lab File: BE092328.D
Acq: 1 Sep 2016 14:33

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

Tot Ion	Ratio	Lower	Upper
178	100		
176	19.9	15.8	23.8
179	0.0	0.0	0.0




Manual Integrations
APPROVED


sohil
9/2/2016 4:33:55 PM



#22
Anthracene
Concen: 1.65 ng
RT: 17.69 min Scan# 1159
Delta R.T. -0.03 min
Lab File: BE092328.D
Acq: 1 Sep 2016 14:33

Tgt Ion	Ratio	Lower	Upper
178	100		
176	19.1	15.0	22.4
179	0.0	12.2	18.2#





#23

Fluoranthene

Concen: 1.75 ng

RT: 19.61 min Scan# 1266

Delta R.T. -0.00 min

Lab File: BE092328.D

Acq: 1 Sep 2016 14:33

Instrument :

BNA_E





ClientSampled :

SSTDICC1.6

Tot Ion:	202	Resp:	123495
Ion Ratio	Lower	Upper	
202	100		
101	2.8	2.2	3.4
203	17.1	13.7	20.5

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:55 PM



#24

Chrysene-d12

Concen: 5.00 ng




RT: 21.75 min Scan# 1375


Delta R.T. -0.00 min

Lab File: BE092328.D

Acq: 1 Sep 2016 14:33

Tgt Ion:	240	Resp:	91855
Ion Ratio	Lower	Upper	
240	100		
120	2.2	2.6	4.0#
236	28.4	24.6	37.0









#25
Pvrene
Concen: 1.55 ng
RT: 19.97 min Scan# 1287
Delta R.T. -0.00 min
Lab File: BE092328.D
Acq: 1 Sep 2016 14:33

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

Tot Ion	Ratio	Resp	Lower	Upper
202	100	131774		
200	5.3		4.2	6.4
203	17.1		13.9	20.9




Manual Integrations
APPROVED


sohil
9/2/2016 4:33:55 PM



#26
Terphenyl-d14
Concen: 1.62 ng
RT: 20.17 min Scan# 1299
Delta R.T. -0.02 min
Lab File: BE092328.D
Acq: 1 Sep 2016 14:33

Tgt Ion	Ratio	Resp	Lower	Upper
244	100	20099		
212	9.9		6.7	10.1
122	18.1		3.6	5.4









#27
Benzo(a)anthracene
Concen: 1.68 ng m
RT: 21.72 min Scan# 1374
Delta R.T. -0.00 min
Lab File: BE092328.D
Acq: 1 Sep 2016 14:33

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

Tot Ion	Ratio	Lower	Upper
228	100		
226	25.3	23.6	35.4
229	17.5	13.3	19.9




Manual Integrations
APPROVED


sohil
9/2/2016 4:33:55 PM



#28
Chrysene
Concen: 1.61 ng m
RT: 21.77 min Scan# 1376
Delta R.T. -0.00 min
Lab File: BE092328.D
Acq: 1 Sep 2016 14:33

Tgt Ion	Ratio	Lower	Upper
228	100		
226	43.0	36.3	54.5
229	11.9	10.6	16.0









#29
 Bis(2-ethylhexyl)phthalate
 Concen: 2.20 ng
 RT: 21.63 min Scan# 1370
 Delta R.T. -0.00 min
 Lab File: BE092328.D
 Acq: 1 Sep 2016 14:33

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC1.6

Tot Ion	Ratio	Resp	Lower	Upper
149	100	14487		
167	0.0	0.0	0.0	0.0
279	0.0	0.0	0.0	0.0




Manual Integrations
 APPROVED


sohil
 9/2/2016 4:33:55 PM



#30
 Indeno(1,2,3-cd)pyrene
 Concen: 1.80 ng
 RT: 26.62 min Scan# 1717
 Delta R.T. 0.00 min
 Lab File: BE092328.D
 Acq: 1 Sep 2016 14:33

Tgt Ion	Ratio	Resp	Lower	Upper
276	100	161242		
138	25.2	20.3	30.5	
277	24.9	19.7	29.5	









#31
Pervlene-d12
Concen: 5.00 ng
RT: 24.12 min Scan# 1547
Delta R.T. 0.00 min
Lab File: BE092328.D
Acq: 1 Sep 2016 14:33

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.2	20.1	30.1
265	22.4	17.9	26.9




Manual Integrations
APPROVED


sohil
9/2/2016 4:33:55 PM



#32
Benzo(b)fluoranthene
Concen: 1.81 ng
RT: 23.38 min Scan# 1483
Delta R.T. 0.00 min
Lab File: BE092328.D
Acq: 1 Sep 2016 14:33

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.5	18.7	28.1
125	9.9	10.5	15.7









#33
Benzo(k)fluoranthene
Concen: 1.58 ng
RT: 23.43 min Scan# 1487
Delta R.T. -0.01 min
Lab File: BE092328.D
Acq: 1 Sep 2016 14:33

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

Tot Ion	Ratio	Lower	Upper
252	100		
253	21.6	20.3	30.5
125	10.1	9.6	14.4




Manual Integrations
APPROVED


sohil
9/2/2016 4:33:55 PM



#34
Benzo(a)pyrene
Concen: 1.69 ng
RT: 24.01 min Scan# 1537
Delta R.T. 0.00 min
Lab File: BE092328.D
Acq: 1 Sep 2016 14:33

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.3	19.0	28.6
125	11.2	11.8	17.8





#35

Dibenzo(a,h)anthracene

Concen: 1.84 ng

RT: 26.63 min Scan# 1718

Delta R.T. -0.02 min

Lab File: BE092328.D

Acq: 1 Sep 2016 14:33

Instrument :

BNA_E





ClientSampleId :

SSTDICC1.6

Tot Ion:	278	Resp:	33204
Ion Ratio	Lower	Upper	
278	100		
139	15.6	13.8	20.8
279	24.2	21.4	32.2

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:55 PM



#36

Benzo(g,h,i)perylene

Concen: 1.72 ng

RT: 27.38 min Scan# 1762

Delta R.T. 0.00 min

Lab File: BE092328.D

Acq: 1 Sep 2016 14:33

Tgt Ion:	276	Resp:	136629
Ion Ratio	Lower	Upper	
276	100		
277	24.7	19.8	29.8
138	20.0	19.8	29.6

