

Data Path : Z:\HPCHEM1\BNA E\DATA\BE090116\
 Data File : BE092329.D
 Acq On : 1 Sep 2016 15:20
 Operator : UM/SJ
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2

Manual Integrations
 APPROVED

sohil
 9/2/2016 4:33:58 PM

Quant Time: Sep 02 03:22:46 2016
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE090116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 02 03:16:21 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	9662	5.00	ng	-0.02
7) Naphthalene-d8	10.95	136	47825	5.00	ng	0.00
12) Acenaphthene-d10	14.82	164	29758	5.00	ng	-0.02
18) Phenanthrene-d10	17.58	188	71106	5.00	ng	0.00
24) Chrysene-d12	21.75	240	104739	5.00	ng	0.00
31) Perylene-d12	24.12	264	92786	5.00	ng	0.00

System Monitoring Compounds						
4) 2-Fluorophenol	5.67	112	7812	3.50	ng	-0.02
5) Phenol-d6	7.34	99	11235	3.83	ng	-0.02
8) Nitrobenzene-d5	9.34	82	11552	3.64	ng	-0.02
13) 2,4,6-Tribromophenol	16.31	330	3655	4.30	ng	-0.01
14) 2-Fluorobiphenyl	13.44	172	26923	2.91	ng	0.00
26) Terphenyl-d14	20.17	244	41701	2.95	ng	-0.02

Target Compounds				Qvalue		
2) 1,4-Dioxane	3.41	88	3664	2.69	ng	94
3) n-Nitrosodimethylamine	3.76	42	5184	3.58	ng	98
6) bis(2-Chloroethyl)ether	7.59	93	9167	4.01	ng	# 88
9) Naphthalene	11.01	128	30963	2.93	ng	# 94
10) Hexachlorobutadiene	11.30	225	4806	2.99	ng	100
11) 2-Methylnaphthalene	12.62	142	21137	3.21	ng	96
15) Acenaphthylene	14.53	152	154007	3.03	ng	100
16) Acenaphthene	14.88	154	23559	2.85	ng	98
17) Fluorene	15.87	166	31069	3.08	ng	99
19) Hexachlorobenzene	16.89	284	9589	3.26	ng	# 66
20) Pentachlorophenol	17.23	266	3930	5.31	ng	# 86
21) Phenanthrene	17.60	178	51297	3.05	ng	# 99
22) Anthracene	17.69	178	52922	3.42	ng	98
23) Fluoranthene	19.61	202	257582	3.36	ng	99
25) Pyrene	19.97	202	281551	2.91	ng	100
27) Benzo(a)anthracene	21.72	228	345973m	3.13	ng	
28) Chrysene	21.77	228	273862m	2.80	ng	
29) Bis(2-ethylhexyl)phthalate	21.63	149	30769	4.10	ng	# 100
30) Indeno(1,2,3-cd)pyrene	26.62	276	332477	3.25	ng	100
32) Benzo(b)fluoranthene	23.38	252	74725	3.41	ng	# 95
33) Benzo(k)fluoranthene	23.43	252	73782	2.95	ng	93
34) Benzo(a)pyrene	24.01	252	72114	3.25	ng	# 95
35) Dibenzo(a,h)anthracene	26.63	278	68088	3.45	ng	94
36) Benzo(g,h,i)perylene	27.38	276	278471	3.20	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE090116\
Data File : BE092329.D
Acq On : 1 Sep 2016 15:20
Operator : UM/SJ
Sample : SSTDICC3.2
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:58 PM

Quant Time: Sep 02 03:22:46 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE090116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 03:16:21 2016
Response via : Initial Calibration





#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.16 min Scan# 576

Delta R.T. -0.02 min

Lab File: BE092329.D

Acq: 1 Sep 2016 15:20

Instrument :

BNA_E


ClientSampled :

SSTDICC3.2




Tot Ion	Ratio	Lower	Upper
152	100		
150	181.6	106.0	159.0#
115	86.5	31.2	46.8#

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:58 PM



Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E



#2

1,4-Dioxane

Concen: 2.69 ng


RT: 3.41 min Scan# 71

Delta R.T. -0.01 min



Lab File: BE092329.D


Acq: 1 Sep 2016 15:20

Tgt Ion	Ratio	Lower	Upper
88	100		
58	86.3	63.6	95.4
43	37.0	28.0	42.0



Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0





#3





n-Nitrosodimethylamine
Concen: 3.58 ng
RT: 3.76 min Scan# 101
Delta R.T. -0.04 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
42	100		
74	105.3	86.0	129.0
44	6.2	5.1	7.7

Manual Integrations
APPROVED




sohil
9/2/2016 4:33:58 PM




#4

2-Fluorophenol
Concen: 3.50 ng
RT: 5.67 min Scan# 363
Delta R.T. -0.02 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Tgt Ion	Ratio	Lower	Upper
112	100		
64	67.1	53.5	80.3
63	36.0	27.9	41.9





#5

Phenol-d6

Concen: 3.83 ng

RT: 7.34 min Scan# 540

Delta R.T. -0.02 min

Lab File: BE092329.D

Acq: 1 Sep 2016 15:20

Instrument :

BNA_E





ClientSampleId :

SSTDICC3.2

Tot Ion:	99	Resp:	11235
Ion Ratio	Lower	Upper	
99	100		
42	0.0	0.0	0.0
71	32.7	30.6	45.8

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:58 PM



#6

bis(2-Chloroethyl)ether

Concen: 4.01 ng




RT: 7.59 min Scan# 551


Delta R.T. 0.00 min

Lab File: BE092329.D

Acq: 1 Sep 2016 15:20

Tgt Ion:	93	Resp:	9167
Ion Ratio	Lower	Upper	
93	100		
63	77.9	71.6	107.4
95	33.0	0.0	0.0#





#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.95 min Scan# 708

Delta R.T. 0.00 min

Lab File: BE092329.D

Acq: 1 Sep 2016 15:20

Instrument :

BNA_E





ClientSampleId :

SSTDICC3.2

Tot Ion	Ratio	Resp	Lower	Upper
136	100			
137	10.8	8.2	12.4	
54	8.6	9.6	14.4	
68	6.4	6.7	10.1	

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:58 PM



#8

Nitrobenzene-d5

Concen: 3.64 ng




RT: 9.34 min Scan# 627


Delta R.T. -0.02 min

Lab File: BE092329.D

Acq: 1 Sep 2016 15:20

Tgt Ion	Ratio	Resp	Lower	Upper
82	100			
128	37.7	39.0	58.4	
54	43.8	44.8	67.2	





#9

Naphthalene

Concen: 2.93 ng

RT: 11.01 min Scan# 711

Delta R.T. 0.00 min

Lab File: BE092329.D

Acq: 1 Sep 2016 15:20

Instrument :

BNA_E





ClientSampleId :

SSTDICC3.2

Tot Ion:	128	Resp:	30963
Ion Ratio	Lower	Upper	
128	100		
129	12.3	11.2	16.8
127	11.6	11.6	17.4#

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:58 PM



#10

Hexachlorobutadiene

Concen: 2.99 ng




RT: 11.30 min Scan# 726


Delta R.T. 0.00 min

Lab File: BE092329.D

Acq: 1 Sep 2016 15:20

Tgt Ion:	225	Resp:	4806
Ion Ratio	Lower	Upper	
225	100		
223	62.9	50.6	76.0
227	64.1	51.4	77.0



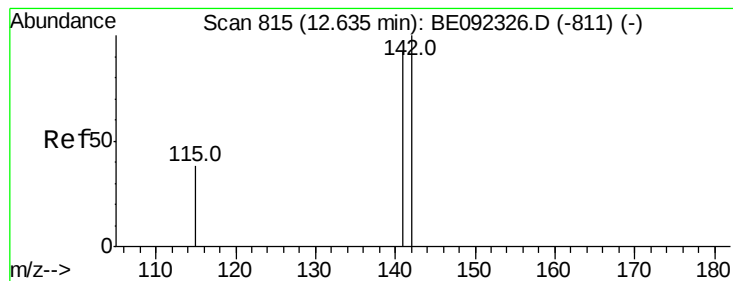





#11
2-Methylnaphthalene
Concen: 3.21 ng
RT: 12.62 min Scan# 814
Delta R.T. -0.01 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
142	100		
141	89.7	73.7	110.5
115	37.3	34.0	51.0




Manual Integrations
APPROVED


sohil
9/2/2016 4:33:58 PM



#12
Acenaphthene-d10
Concen: 5.00 ng
RT: 14.82 min Scan# 980
Delta R.T. -0.02 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Tgt Ion	Ratio	Lower	Upper
164	100		
162	111.8	71.4	107.0#
160	52.6	27.4	41.2#









#13
 2,4,6-Tribromophenol
 Concen: 4.30 ng
 RT: 16.31 min Scan# 1088
 Delta R.T. -0.01 min
 Lab File: BE092329.D
 Acq: 1 Sep 2016 15:20

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.5	75.4	113.0
141	40.2	31.0	46.6




Manual Integrations
 APPROVED


sohil
 9/2/2016 4:33:58 PM



#14
 2-Fluorobiphenyl
 Concen: 2.91 ng
 RT: 13.44 min Scan# 885
 Delta R.T. 0.00 min
 Lab File: BE092329.D
 Acq: 1 Sep 2016 15:20

Tgt Ion	Ratio	Lower	Upper
172	100		
171	29.7	30.1	45.1#
170	17.7	21.8	32.6#









#15
Acenaphthylene
Concen: 3.03 ng
RT: 14.53 min Scan# 963
Delta R.T. -0.02 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
152	100		
151	4.9	3.9	5.9
153	13.1	10.4	15.6




Manual Integrations
APPROVED


sohil
9/2/2016 4:33:58 PM



#16
Acenaphthene
Concen: 2.85 ng
RT: 14.88 min Scan# 984
Delta R.T. 0.00 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Tgt Ion	Ratio	Lower	Upper
154	100		
153	442.0	350.8	526.2
152	216.9	171.1	256.7









#17
Fluorene
 Concen: 3.08 ng
 RT: 15.87 min Scan# 1050
 Delta R.T. 0.00 min
 Lab File: BE092329.D
 Acq: 1 Sep 2016 15:20

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
166	100		
165	99.1	78.2	117.4
167	13.4	11.0	16.4




Manual Integrations
 APPROVED


sohil
 9/2/2016 4:33:58 PM



#18
Phenanthrene-d10
 Concen: 5.00 ng
 RT: 17.58 min Scan# 1154
 Delta R.T. -0.00 min
 Lab File: BE092329.D
 Acq: 1 Sep 2016 15:20

Tgt Ion	Ratio	Lower	Upper
188	100		
94	3.2	3.2	4.8
80	2.5	2.6	3.8






#19
Hexachlorobenzene
Concen: 3.26 ng
RT: 16.89 min Scan# 1124
Delta R.T. -0.00 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2




Tot Ion	Ratio	Lower	Upper
284	100		
142	0.0	29.1	43.7#
249	31.3	27.9	41.9

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:58 PM






Abundance Ion 283.80 (283.50 to 284.50): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E




#20
Pentachlorophenol
Concen: 5.31 ng
RT: 17.23 min Scan# 1139
Delta R.T. -0.02 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Tgt Ion	Ratio	Lower	Upper
266	100		
268	57.5	62.5	93.7#
264	67.8	57.2	85.8

Abundance Ion 265.70 (265.40 to 266.40): E
Ion 268.00 (267.70 to 268.70): E
Ion 264.00 (263.70 to 264.70): E



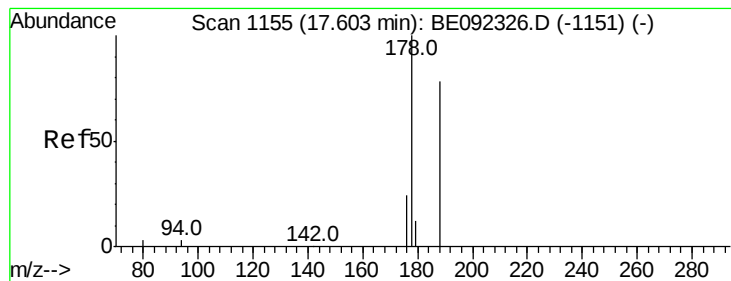

#21

Phenanthrene

Concen: 3.05 ng

RT: 17.60 min Scan# 1155

Delta R.T. -0.00 min

Lab File: BE092329.D

Acq: 1 Sep 2016 15:20

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2

Tot Ion:178 Resp: 51297

Ion Ratio Lower Upper

178 100





176 20.1 15.8 23.8

179 15.1 0.0 0.0#

Manual Integrations
APPROVED

sohil

9/2/2016 4:33:58 PM

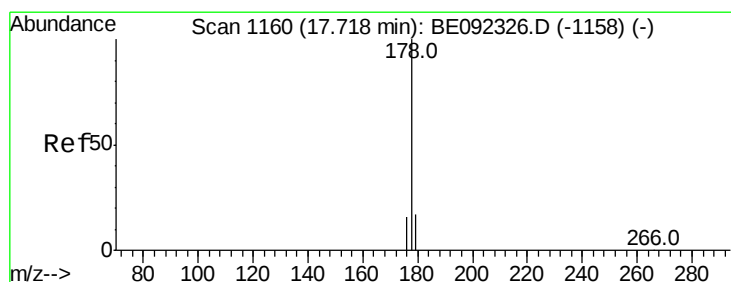

#22

Anthracene

Concen: 3.42 ng

RT: 17.69 min Scan# 1159

Delta R.T. -0.02 min

Lab File: BE092329.D

Acq: 1 Sep 2016 15:20




Tgt Ion:178 Resp: 52922


Ion Ratio Lower Upper

178 100

176 19.7 15.0 22.4

179 14.8 12.2 18.2





#23

Fluoranthene

Concen: 3.36 ng

RT: 19.61 min Scan# 1266

Delta R.T. 0.00 min

Lab File: BE092329.D

Acq: 1 Sep 2016 15:20

Instrument :

BNA_E





ClientSampleId :

SSTDICC3.2

Tot Ion:	202	Resp:	257582
Ion Ratio	Lower	Upper	
202	100		
101	2.9	2.2	3.4
203	17.5	13.7	20.5

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:58 PM



#24

Chrysene-d12

Concen: 5.00 ng




RT: 21.75 min Scan# 1375


Delta R.T. -0.00 min

Lab File: BE092329.D

Acq: 1 Sep 2016 15:20

Tgt Ion:	240	Resp:	104739
Ion Ratio	Lower	Upper	
240	100		
120	2.2	2.6	4.0#
236	28.8	24.6	37.0









#25
Pvrene
Concen: 2.91 ng
RT: 19.97 min Scan# 1287
Delta R.T. 0.00 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Instrument :
BNA_E
ClientSampled :
SSTDICC3.2

Tot Ion	Ratio	Resp Lower	Upper
202	100		
200	5.3	4.2	6.4
203	17.1	13.9	20.9




Manual Integrations
APPROVED


sohil
9/2/2016 4:33:58 PM



#26
Terphenyl-d14
Concen: 2.95 ng
RT: 20.17 min Scan# 1299
Delta R.T. -0.02 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Tgt Ion	Ratio	Resp Lower	Upper
244	100		
212	9.4	6.7	10.1
122	11.9	3.6	5.4#





#27

Benzo(a)anthracene

Concen: 3.13 ng m

RT: 21.72 min Scan# 1374

Delta R.T. -0.00 min

Lab File: BE092329.D





Acq: 1 Sep 2016 15:20

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
228	100		
226	25.9	23.6	35.4
229	16.5	13.3	19.9

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:58 PM



#28

Chrysene

Concen: 2.80 ng m




RT: 21.77 min Scan# 1376


Delta R.T. -0.00 min

Lab File: BE092329.D

Acq: 1 Sep 2016 15:20

Tgt Ion	Ratio	Lower	Upper
228	100		
226	41.7	36.3	54.5
229	12.4	10.6	16.0









#29
 Bis(2-ethylhexyl)phthalate
 Concen: 4.10 ng
 RT: 21.63 min Scan# 1370
 Delta R.T. -0.00 min
 Lab File: BE092329.D
 Acq: 1 Sep 2016 15:20

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2

Tot Ion	Ratio	Resp Lower	Resp Upper
149	100		
167	0.0	0.0	0.0
279	0.0	0.0	0.0




Manual Integrations
 APPROVED


sohil
 9/2/2016 4:33:58 PM



#30
 Indeno(1,2,3-cd)pyrene
 Concen: 3.25 ng
 RT: 26.62 min Scan# 1717
 Delta R.T. -0.00 min
 Lab File: BE092329.D
 Acq: 1 Sep 2016 15:20

Tgt Ion	Ratio	Resp Lower	Resp Upper
276	100		
138	25.1	20.3	30.5
277	24.7	19.7	29.5









#31
Pervlene-d12
Concen: 5.00 ng
RT: 24.12 min Scan# 1547
Delta R.T. 0.00 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.3	20.1	30.1
265	23.1	17.9	26.9




Manual Integrations
APPROVED


sohil
9/2/2016 4:33:58 PM



#32
Benzo(b)fluoranthene
Concen: 3.41 ng
RT: 23.38 min Scan# 1483
Delta R.T. 0.00 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.0	18.7	28.1
125	9.7	10.5	15.7









#33
Benzo(k)fluoranthene
Concen: 2.95 ng
RT: 23.43 min Scan# 1487
Delta R.T. -0.01 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
252	100		
253	21.5	20.3	30.5
125	9.8	9.6	14.4




Manual Integrations
APPROVED


sohil
9/2/2016 4:33:58 PM



#34
Benzo(a)pyrene
Concen: 3.25 ng
RT: 24.01 min Scan# 1537
Delta R.T. 0.00 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.7	19.0	28.6
125	10.6	11.8	17.8









#35
Dibenzo(a,h)anthracene
Concen: 3.45 ng
RT: 26.63 min Scan# 1718
Delta R.T. -0.02 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
278	100		
139	14.3	13.8	20.8
279	23.7	21.4	32.2

Manual Integrations
APPROVED

sohil
9/2/2016 4:33:58 PM



#36
Benzo(g,h,i)perylene
Concen: 3.20 ng
RT: 27.38 min Scan# 1762
Delta R.T. -0.00 min
Lab File: BE092329.D
Acq: 1 Sep 2016 15:20

Tgt Ion	Ratio	Lower	Upper
276	100		
277	24.3	19.8	29.8
138	20.7	19.8	29.6

