

Data Path : Z:\HPCHEM1\BNA E\DATA\BE090116\
 Data File : BE092339.D
 Acq On : 1 Sep 2016 21:27
 Operator : UM/SJ
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC0.4EC

Manual Integrations
 APPROVED

sohil
 9/2/2016 4:34:16 PM

Quant Time: Sep 02 11:13:11 2016
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE090116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 02 11:02:43 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.19	152	7720	5.00	ng	0.00
7) Naphthalene-d8	10.95	136	36894	5.00	ng	0.00
12) Acenaphthene-d10	14.81	164	22718	5.00	ng	-0.02
18) Phenanthrene-d10	17.58	188	55685	5.00	ng	0.00
24) Chrysene-d12	21.75	240	82603	5.00	ng	0.00
31) Perylene-d12	24.12	264	76903	5.00	ng	0.00

System Monitoring Compounds						
4) 2-Fluorophenol	5.69	112	777	0.38	ng	0.00
5) Phenol-d6	7.36	99	929	0.33	ng	0.00
8) Nitrobenzene-d5	9.36	82	896	0.33	ng	0.00
13) 2,4,6-Tribromophenol	16.32	330	298	0.34	ng	0.00
14) 2-Fluorobiphenyl	13.45	172	2783	0.40	ng	0.00
26) Terphenyl-d14	20.19	244	4290	0.38	ng	0.00

Target Compounds						Qvalue
2) 1,4-Dioxane	3.42	88	497	0.45	ng	97
3) n-Nitrosodimethylamine	3.79	42	409	0.36	ng	# 95
6) bis(2-Chloroethyl)ether	7.61	93	777	0.43	ng	# 5
9) Naphthalene	11.01	128	3489	0.43	ng	100
10) Hexachlorobutadiene	11.30	225	549	0.42	ng	99
11) 2-Methylnaphthalene	12.65	142	2220	0.41	ng	93
15) Acenaphthylene	14.54	152	16131	0.41	ng	100
16) Acenaphthene	14.88	154	2677	0.42	ng	99
17) Fluorene	15.87	166	3299	0.41	ng	100
19) Hexachlorobenzene	16.89	284	1042	0.43	ng	# 67
20) Pentachlorophenol	17.26	266	238	0.37	ng	100
21) Phenanthrene	17.60	178	5886	0.43	ng	# 100
22) Anthracene	17.72	178	5289	0.40	ng	100
23) Fluoranthene	19.61	202	27914	0.41	ng	99
25) Pyrene	19.97	202	29595	0.39	ng	100
27) Benzo(a)anthracene	21.72	228	37090m	0.40	ng	
28) Chrysene	21.77	228	34982m	0.45	ng	
29) Bis(2-ethylhexyl)phthalate	21.63	149	2709	0.31	ng	# 56
30) Indeno(1,2,3-cd)pyrene	26.62	276	36914	0.41	ng	100
32) Benzo(b)fluoranthene	23.38	252	7895	0.38	ng	99
33) Benzo(k)fluoranthene	23.43	252	8836	0.44	ng	96
34) Benzo(a)pyrene	24.01	252	8050	0.41	ng	99
35) Dibenzo(a,h)anthracene	26.63	278	7500	0.40	ng	97
36) Benzo(g,h,i)perylene	27.38	276	31686	0.41	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE090116\
Data File : BE092339.D
Acq On : 1 Sep 2016 21:27
Operator : UM/SJ
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

sohil
9/2/2016 4:34:16 PM

Quant Time: Sep 02 11:13:11 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE090116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 11:02:43 2016
Response via : Initial Calibration

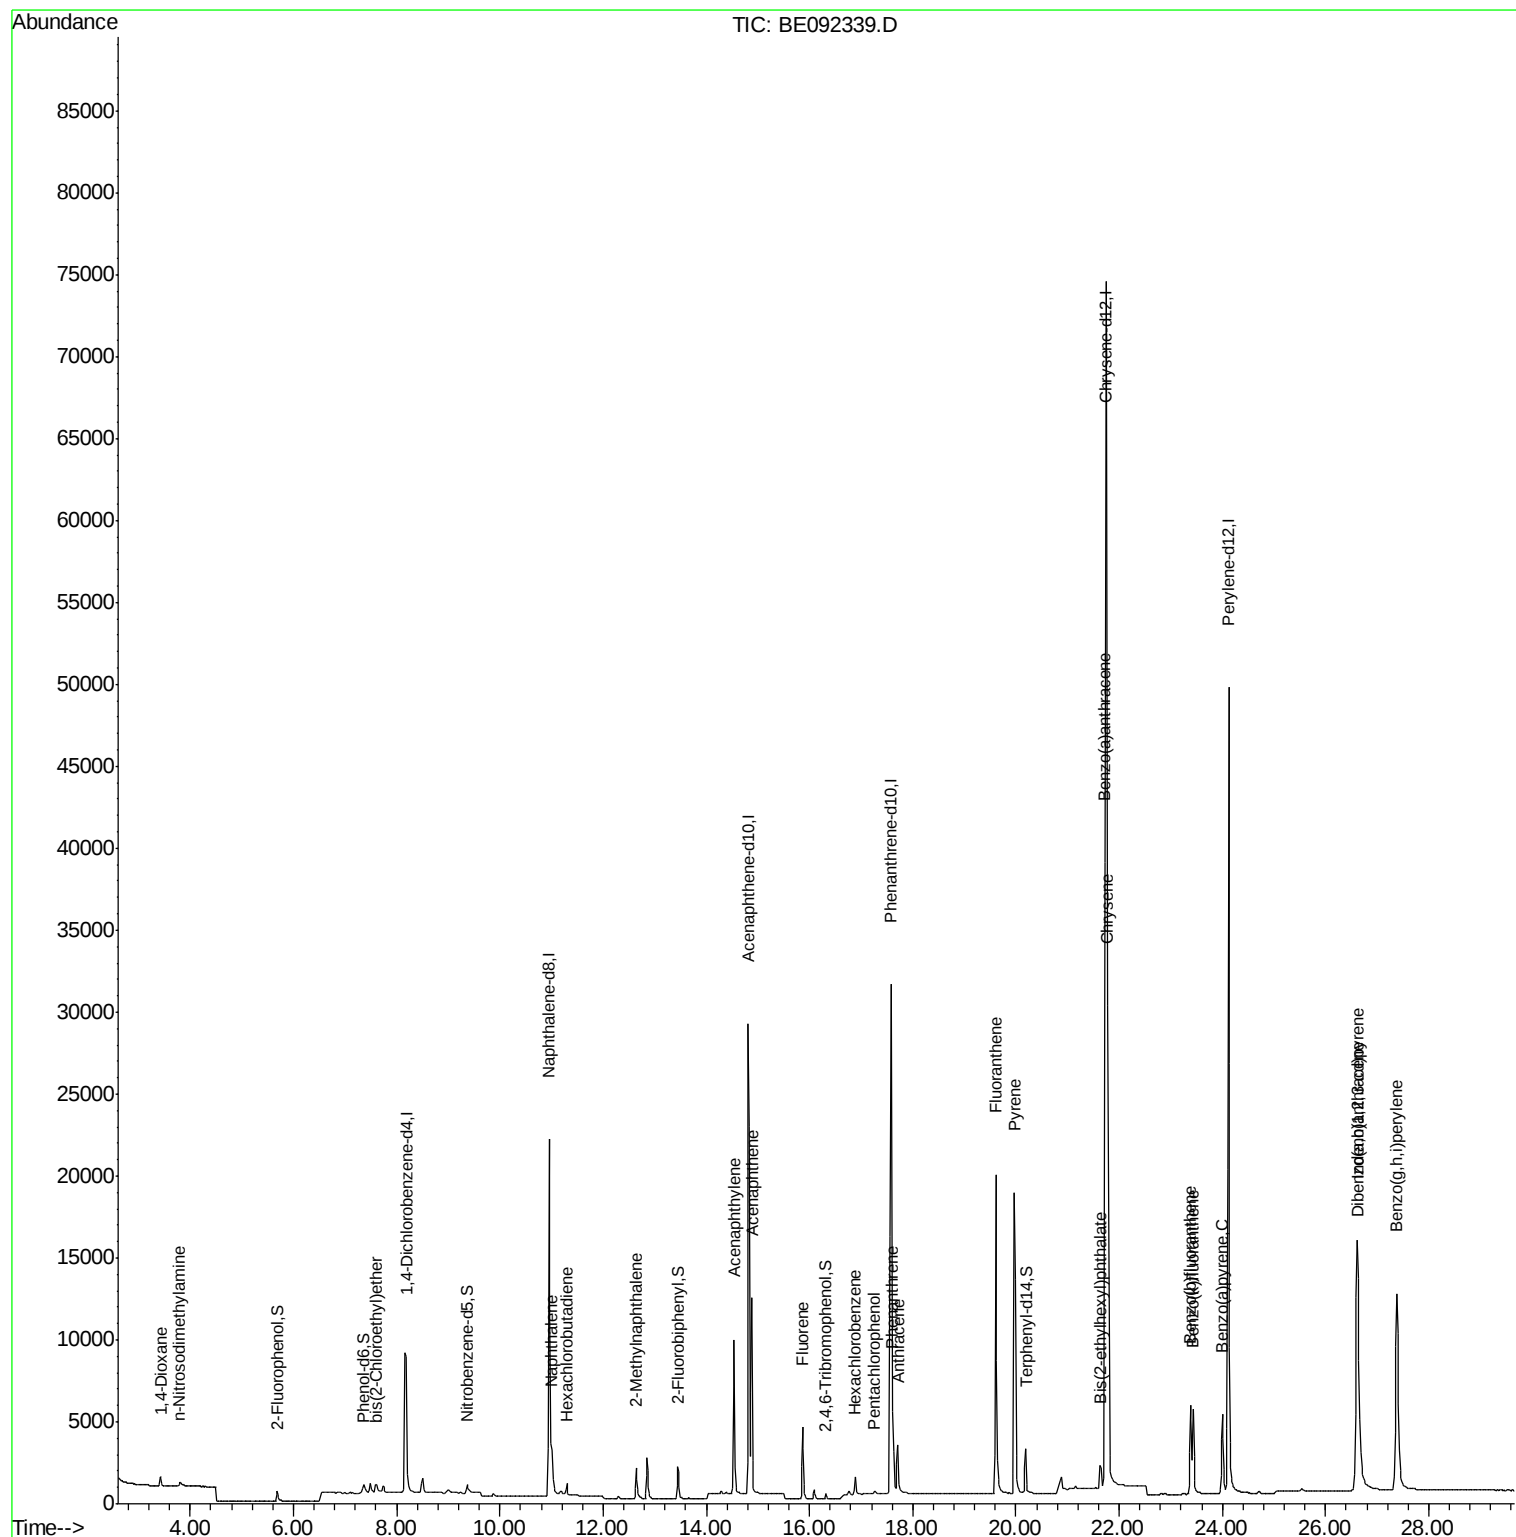

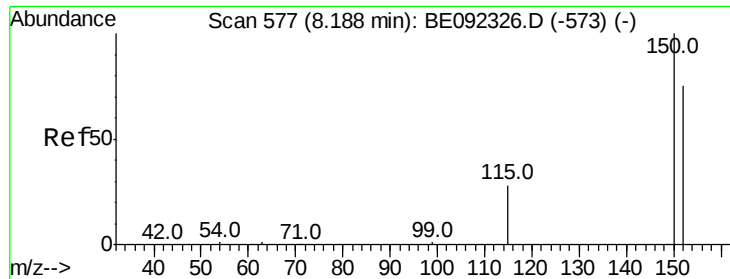

#1





1,4-Dichlorobenzene-d4
Concen: 5.00 ng
RT: 8.19 min Scan# 577
Delta R.T. -0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tot Ion	Ratio	Lower	Upper
152	100		
150	133.0	106.0	159.0
115	39.1	31.2	46.8

Manual Integrations
APPROVED




sohil
9/2/2016 4:34:16 PM

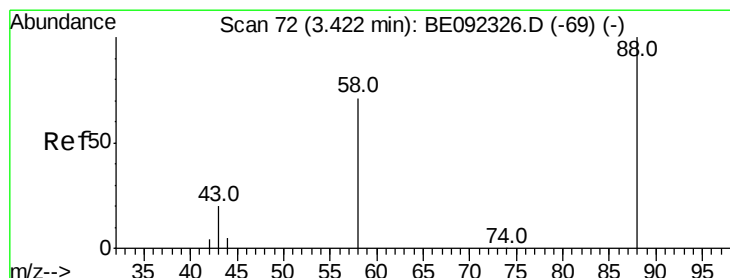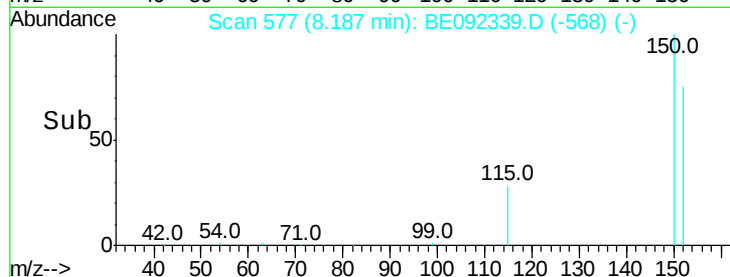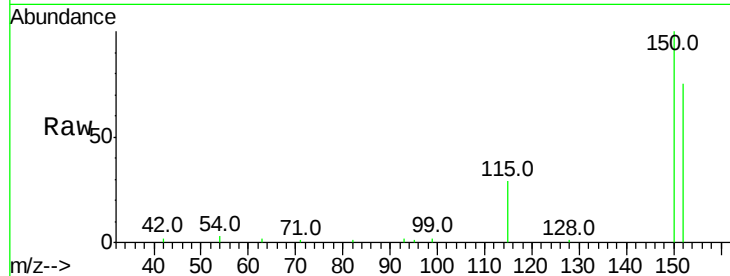


#2

1,4-Dioxane
Concen: 0.45 ng
RT: 3.42 min Scan# 72
Delta R.T. 0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Tgt Ion	Ratio	Lower	Upper
88	100		
58	77.5	63.6	95.4
43	32.2	28.0	42.0

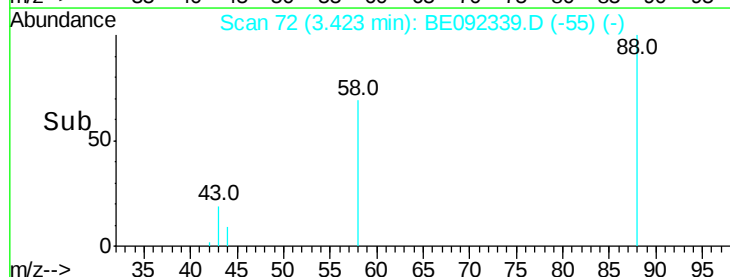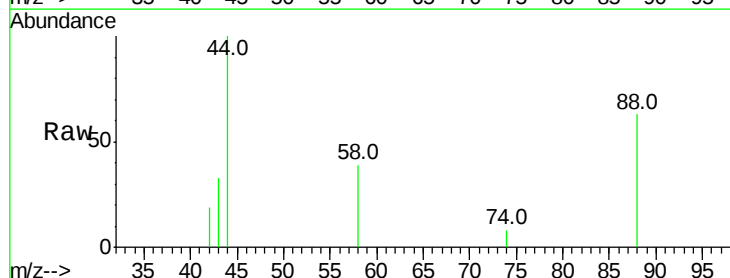



#3





n-Nitrosodimethylamine
Concen: 0.36 ng
RT: 3.79 min Scan# 104
Delta R.T. 0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tot Ion	Ratio	Lower	Upper
42	100		
74	111.7	86.0	129.0
44	15.2	5.1	7.7#

Manual Integrations
APPROVED




sohil
9/2/2016 4:34:16 PM




#4

2-Fluorophenol
Concen: 0.38 ng
RT: 5.69 min Scan# 366
Delta R.T. -0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Tgt Ion	Ratio	Lower	Upper
112	100		
64	66.5	53.5	80.3
63	33.8	27.9	41.9





#5

Phenol-d6

Concen: 0.33 ng

RT: 7.36 min Scan# 541

Delta R.T. -0.00 min

Lab File: BE092339.D

Acq: 1 Sep 2016 21:27

Instrument :

BNA_E





ClientSampleId :

SSTDCCC0.4EC

Tot Ion:	99	Resp:	929
Ion	Ratio	Lower	Upper
99	100		
42	0.0	0.0	0.0
71	35.5	30.6	45.8

Manual Integrations
APPROVED

sohil
9/2/2016 4:34:16 PM

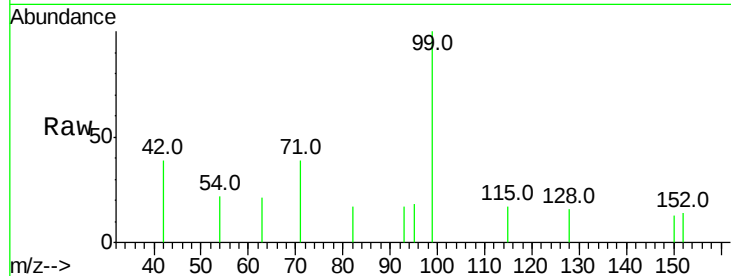

#6

bis(2-Chloroethyl)ether

Concen: 0.43 ng




RT: 7.61 min Scan# 552


Delta R.T. 0.02 min

Lab File: BE092339.D

Acq: 1 Sep 2016 21:27

Tgt Ion:	93	Resp:	777
Ion	Ratio	Lower	Upper
93	100		
63	0.0	71.6	107.4#
95	32.2	0.0	0.0#





#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.95 min Scan# 708

Delta R.T. 0.00 min

Lab File: BE092339.D

Acq: 1 Sep 2016 21:27

Instrument :

BNA_E





ClientSampleId :

SSTDCCC0.4EC

Tot Ion	Ratio	Lower	Upper
136	100		
137	10.5	8.2	12.4
54	10.7	9.6	14.4
68	7.7	6.7	10.1

Manual Integrations
APPROVED

sohil
9/2/2016 4:34:16 PM

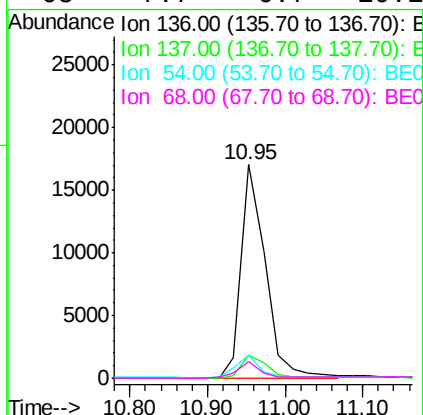

#8

Nitrobenzene-d5

Concen: 0.33 ng




RT: 9.36 min Scan# 628


Delta R.T. -0.00 min

Lab File: BE092339.D

Acq: 1 Sep 2016 21:27

Tgt Ion	Ratio	Lower	Upper
82	100		
128	44.7	39.0	58.4
54	58.8	44.8	67.2

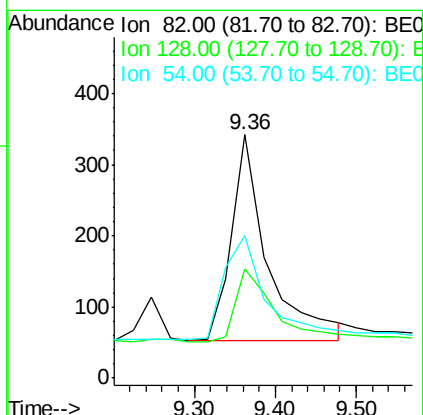







#9
Naphthalene
Concen: 0.43 ng
RT: 11.01 min Scan# 711
Delta R.T. 0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tot Ion	128	Resp	3489
Ion	Ratio	Lower	Upper
128	100		
129	13.9	11.2	16.8
127	14.5	11.6	17.4




Manual Integrations
APPROVED


sohil
9/2/2016 4:34:16 PM



#10
Hexachlorobutadiene
Concen: 0.42 ng
RT: 11.30 min Scan# 726
Delta R.T. 0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Tgt Ion	225	Resp	549
Ion	Ratio	Lower	Upper
225	100		
223	62.1	50.6	76.0
227	65.0	51.4	77.0



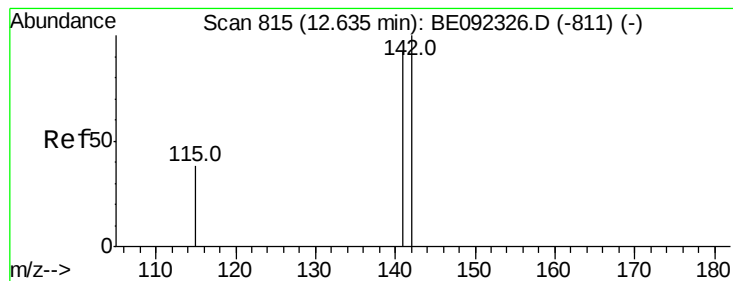





#11
2-Methylnaphthalene
Concen: 0.41 ng
RT: 12.65 min Scan# 816
Delta R.T. 0.01 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tot Ion	Ratio	Lower	Upper
142	100		
141	86.2	73.7	110.5
115	37.8	34.0	51.0




Manual Integrations
APPROVED


sohil
9/2/2016 4:34:16 PM

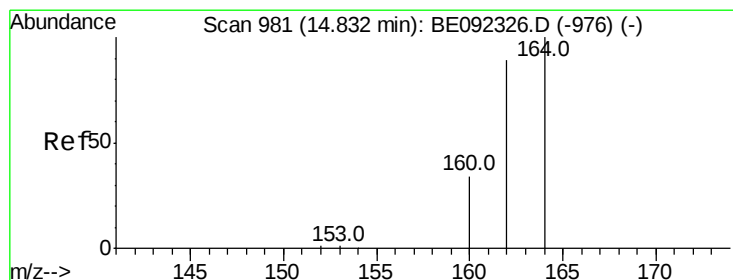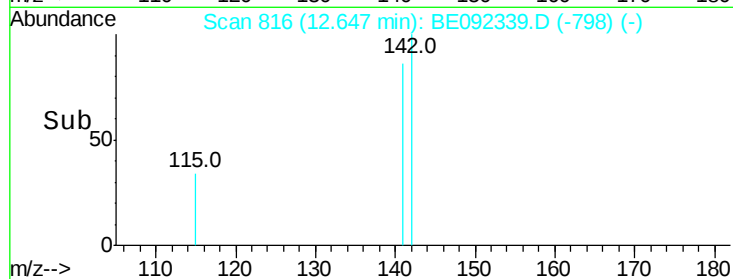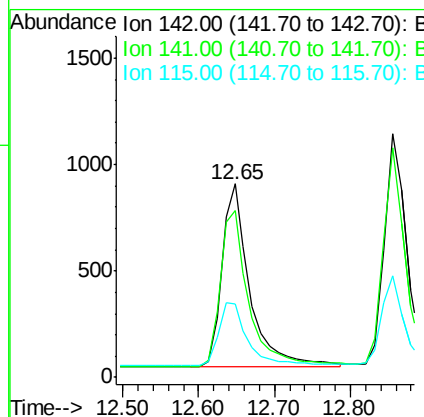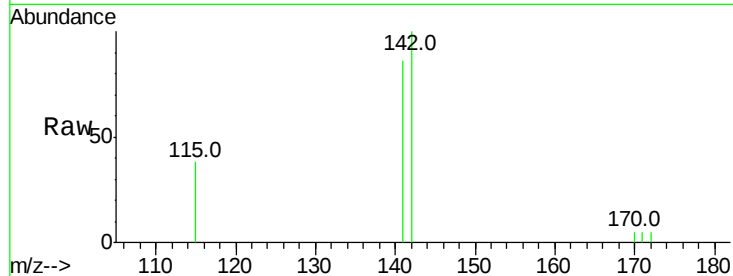

#12
Acenaphthene-d10
Concen: 5.00 ng
RT: 14.81 min Scan# 980
Delta R.T. -0.02 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Tgt Ion	Ratio	Lower	Upper
164	100		
162	117.8	71.4	107.0#
160	59.6	27.4	41.2#

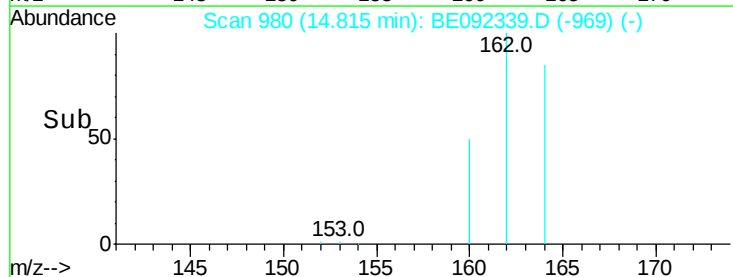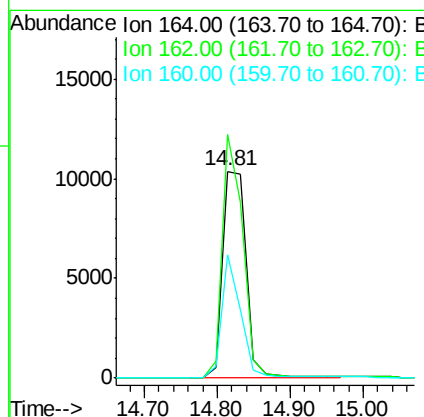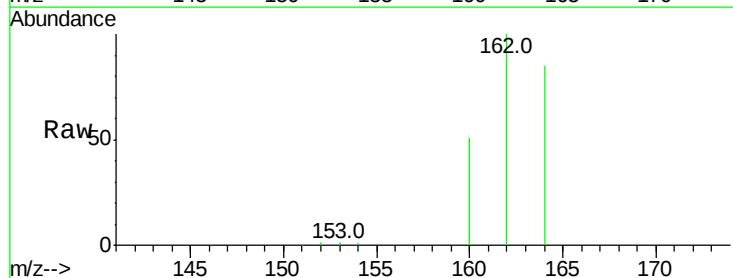

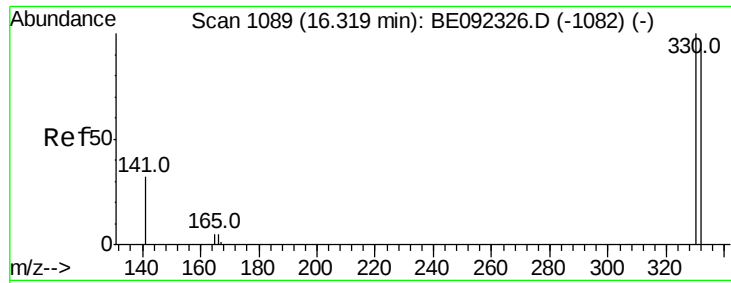





#13
 2,4,6-Tribromophenol
 Concen: 0.34 ng
 RT: 16.32 min Scan# 1089
 Delta R.T. -0.00 min
 Lab File: BE092339.D
 Acq: 1 Sep 2016 21:27

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC0.4EC

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.3	75.4	113.0
141	41.6	31.0	46.6




Manual Integrations
 APPROVED


sohil
 9/2/2016 4:34:16 PM

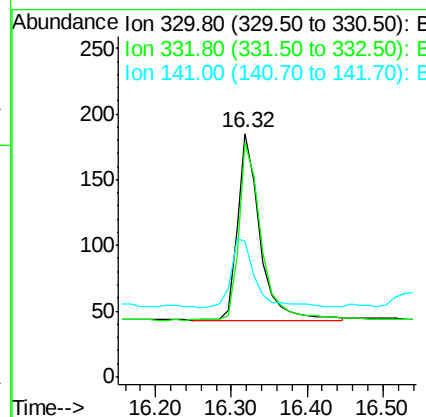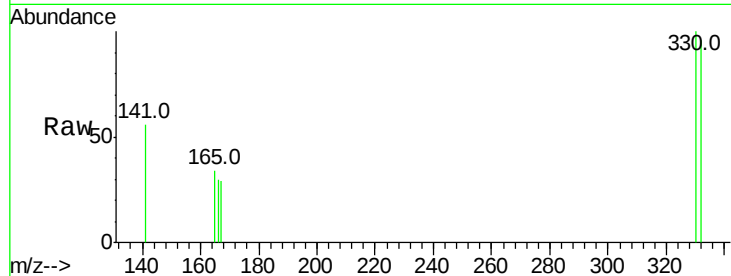

#14
 2-Fluorobiphenyl
 Concen: 0.40 ng
 RT: 13.45 min Scan# 885
 Delta R.T. 0.00 min
 Lab File: BE092339.D
 Acq: 1 Sep 2016 21:27

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.7	30.1	45.1
170	27.6	21.8	32.6

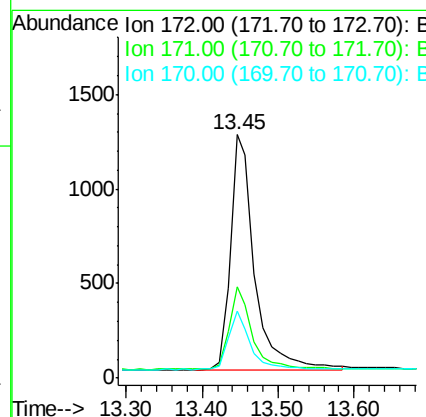







#15
Acenaphthylene
Concen: 0.41 ng
RT: 14.54 min Scan# 964
Delta R.T. -0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tot Ion	Ratio	Lower	Upper
152	100		
151	4.9	3.9	5.9
153	13.1	10.4	15.6




Manual Integrations
APPROVED


sohil
9/2/2016 4:34:16 PM

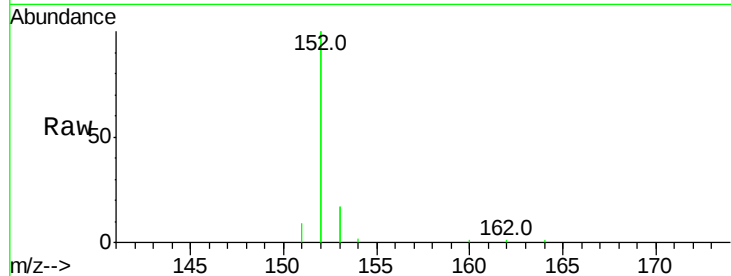

#16
Acenaphthene
Concen: 0.42 ng
RT: 14.88 min Scan# 984
Delta R.T. -0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Tgt Ion	Ratio	Lower	Upper
154	100		
153	435.9	350.8	526.2
152	217.2	171.1	256.7









#17
Fluorene
Concen: 0.41 ng
RT: 15.87 min Scan# 1050
Delta R.T. -0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tot Ion	Ratio	Lower	Upper
166	100		
165	97.3	78.2	117.4
167	13.5	11.0	16.4




Manual Integrations
APPROVED


sohil
9/2/2016 4:34:16 PM

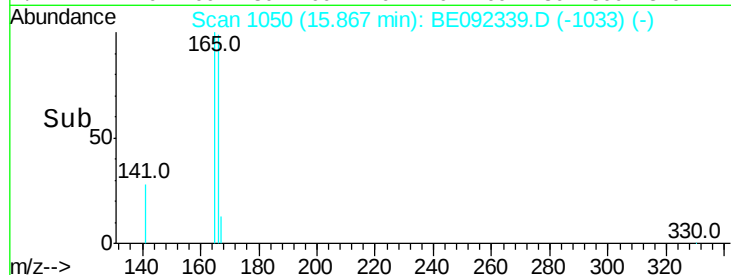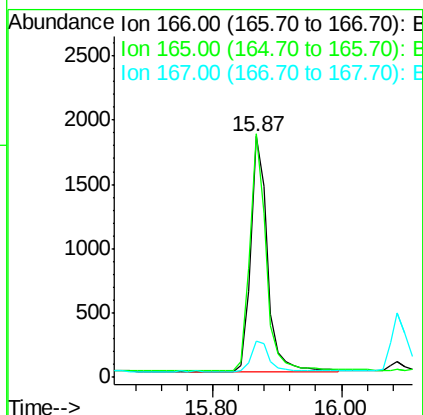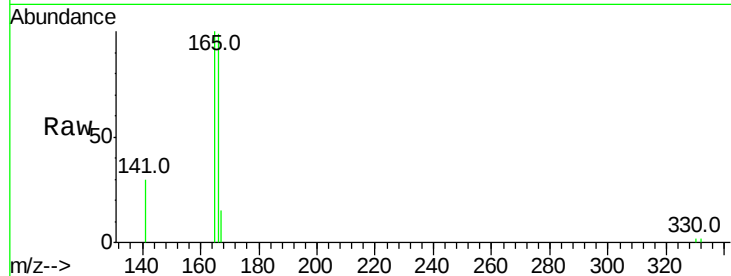

#18
Phenanthrene-d10
Concen: 5.00 ng
RT: 17.58 min Scan# 1154
Delta R.T. -0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Tgt Ion	Ratio	Lower	Upper
188	100		
94	3.5	3.2	4.8
80	2.9	2.6	3.8

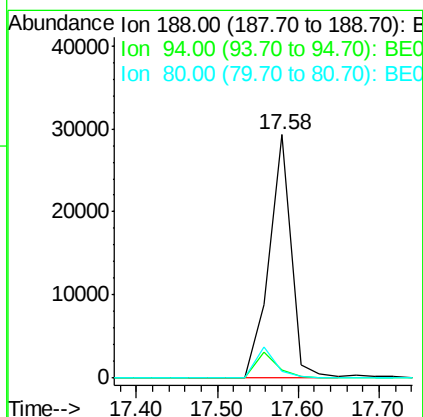







#19
Hexachlorobenzene
Concen: 0.43 ng
RT: 16.89 min Scan# 1124
Delta R.T. -0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tot Ion	Ratio	Lower	Upper
284	100		
142	0.0	29.1	43.7#
249	33.3	27.9	41.9




Manual Integrations
APPROVED


sohil
9/2/2016 4:34:16 PM

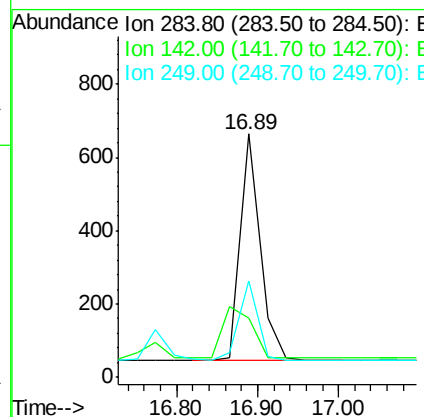

#20
Pentachlorophenol
Concen: 0.37 ng
RT: 17.26 min Scan# 1140
Delta R.T. 0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Tgt Ion	Ratio	Lower	Upper
266	100		
268	78.6	62.5	93.7
264	71.4	57.2	85.8

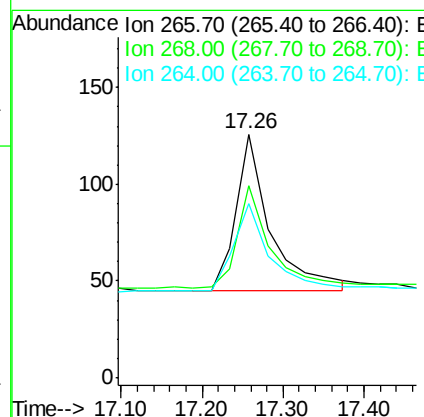

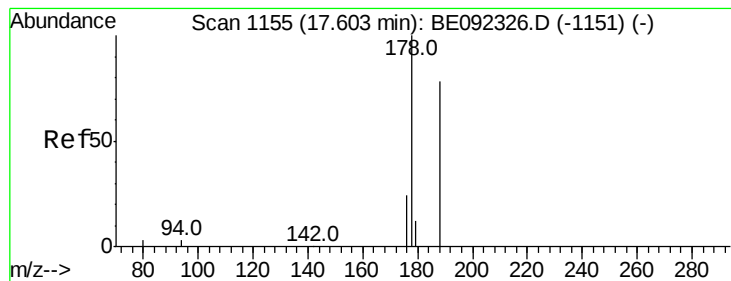

#21

Phenanthrene

Concen: 0.43 ng

RT: 17.60 min Scan# 1155

Delta R.T. -0.00 min

Lab File: BE092339.D

Acq: 1 Sep 2016 21:27

Instrument :

BNA_E

ClientSampleId :

SSTDCCC0.4EC

Tot Ion:178 Resp: 5886

Ion Ratio Lower Upper

178 100





176 20.0 15.8 23.8

179 15.8 0.0 0.0#

Manual Integrations
APPROVED

sohil

9/2/2016 4:34:16 PM

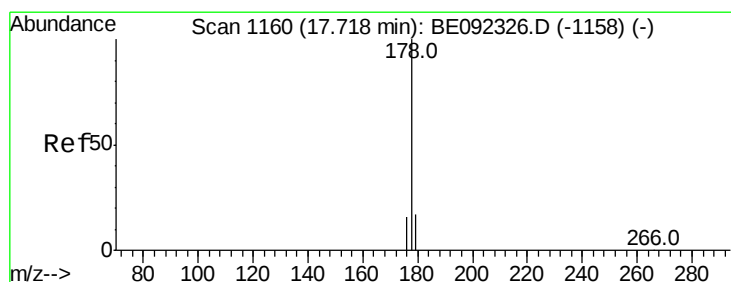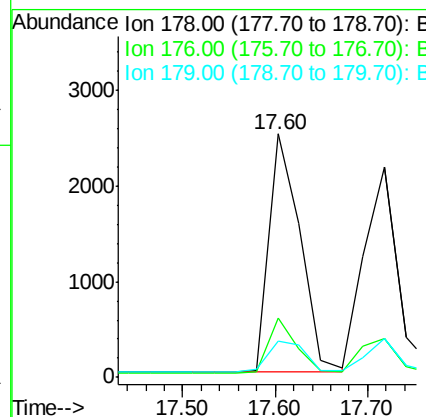

#22

Anthracene

Concen: 0.40 ng

RT: 17.72 min Scan# 1160

Delta R.T. -0.00 min

Lab File: BE092339.D

Acq: 1 Sep 2016 21:27




Tgt Ion:178 Resp: 5289


Ion Ratio Lower Upper

178 100

176 18.8 15.0 22.4

179 14.8 12.2 18.2

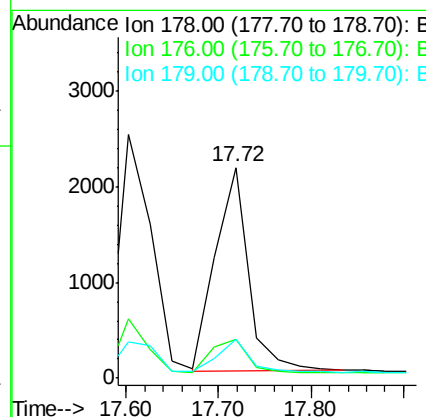

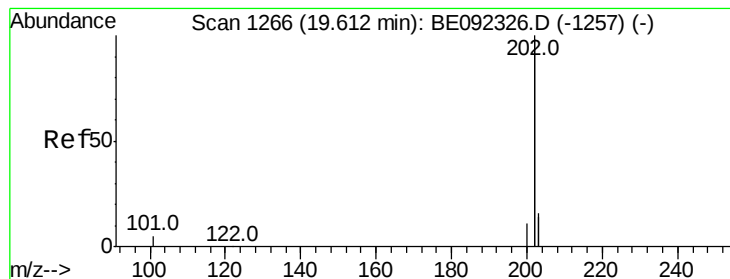

#23

Fluoranthene

Concen: 0.41 ng

RT: 19.61 min Scan# 1266

Delta R.T. -0.00 min

Lab File: BE092339.D

Acq: 1 Sep 2016 21:27

Instrument :

BNA_E


ClientSampleId :

SSTDCCC0.4EC




Tot Ion:	202	Resp:	27914
Ion Ratio	Lower	Upper	
202	100		
101	2.8	2.2	3.4
203	17.4	13.7	20.5

Manual Integrations
APPROVED

sohil
9/2/2016 4:34:16 PM

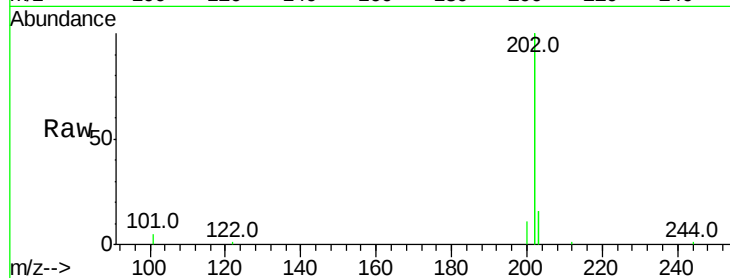

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E

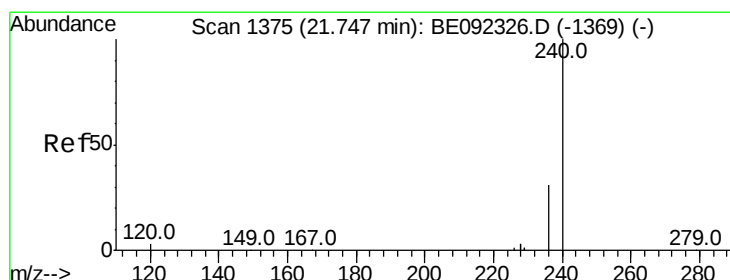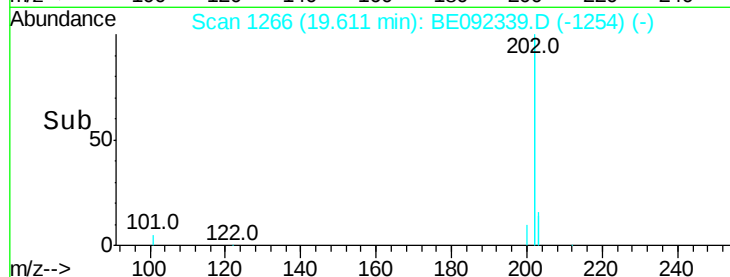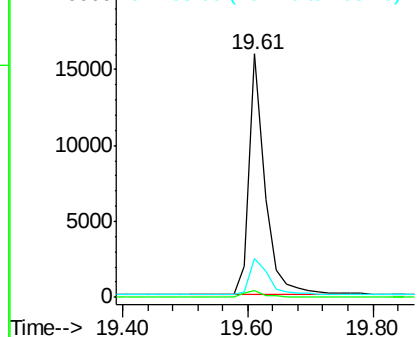

#24

Chrysene-d12

Concen: 5.00 ng

RT: 21.75 min Scan# 1375




Delta R.T. -0.00 min


Lab File: BE092339.D

Acq: 1 Sep 2016 21:27

Tgt Ion:	240	Resp:	82603
Ion Ratio	Lower	Upper	
240	100		
120	2.8	2.6	4.0
236	28.2	24.6	37.0

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

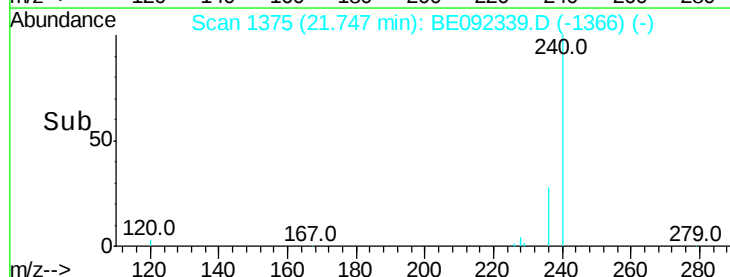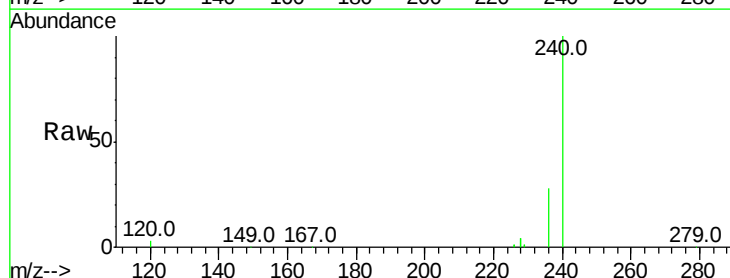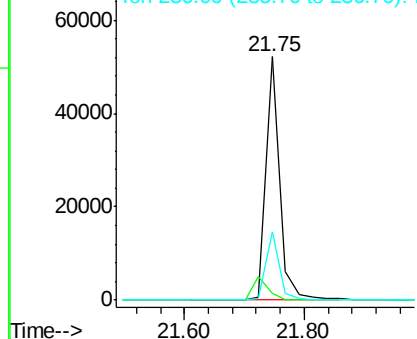







#25
Pvrene
Concen: 0.39 ng
RT: 19.97 min Scan# 1287
Delta R.T. -0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tot Ion	Ratio	Resp Lower	Upper
202	100		
200	5.3	4.2	6.4
203	17.5	13.9	20.9




Manual Integrations
APPROVED


sohil
9/2/2016 4:34:16 PM

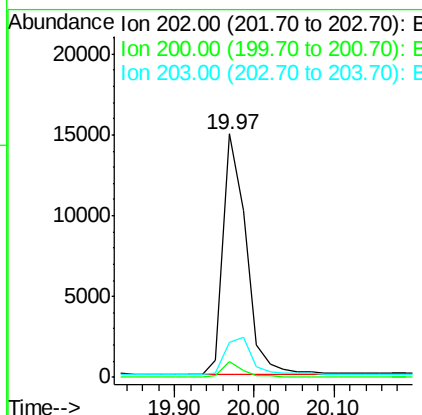

#26
Terphenyl-d14
Concen: 0.38 ng
RT: 20.19 min Scan# 1300
Delta R.T. -0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Tgt Ion	Ratio	Resp Lower	Upper
244	100		
212	8.9	6.7	10.1
122	5.7	3.6	5.4#

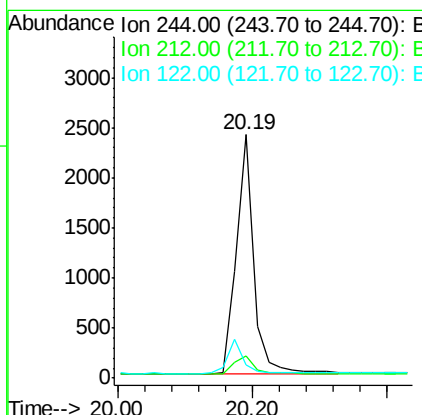



#27

Benzo(a)anthracene

Concen: 0.40 ng m

RT: 21.72 min Scan# 1374

Delta R.T. -0.00 min

Lab File: BE092339.D





Acq: 1 Sep 2016 21:27

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tot Ion	Ion	Ratio	Lower	Upper
228	100			
226	27.7	23.6	35.4	
229	17.1	13.3	19.9	

Manual Integrations
APPROVED

sohil
9/2/2016 4:34:16 PM

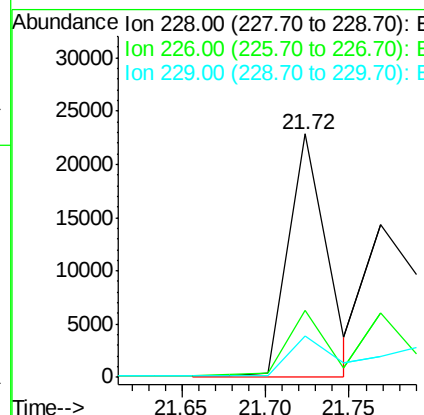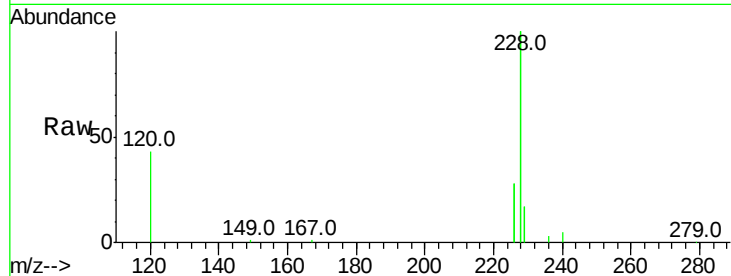

#28

Chrysene

Concen: 0.45 ng m




RT: 21.77 min Scan# 1376


Delta R.T. -0.00 min

Lab File: BE092339.D

Acq: 1 Sep 2016 21:27

Tgt Ion	Ion	Ratio	Lower	Upper
228	100			
226	42.4	36.3	54.5	
229	13.4	10.6	16.0	

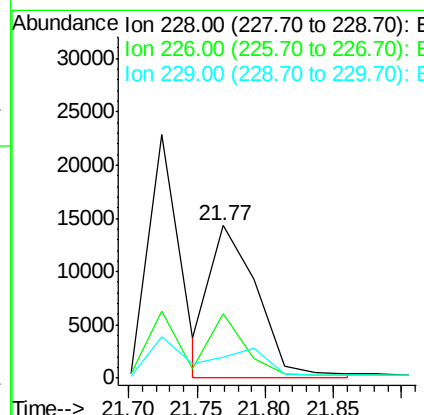







#29
 Bis(2-ethylhexyl)phthalate
 Concen: 0.31 ng
 RT: 21.63 min Scan# 1370
 Delta R.T. 0.00 min
 Lab File: BE092339.D
 Acq: 1 Sep 2016 21:27

Instrument :
 BNA_E
 ClientSampleId :
 SSTCCCC0.4EC

Tot Ion	Ratio	Lower	Upper
149	100		
167	0.0	16.0	24.0#
279	0.0	16.0	24.0#




Manual Integrations
 APPROVED


sohil
 9/2/2016 4:34:16 PM

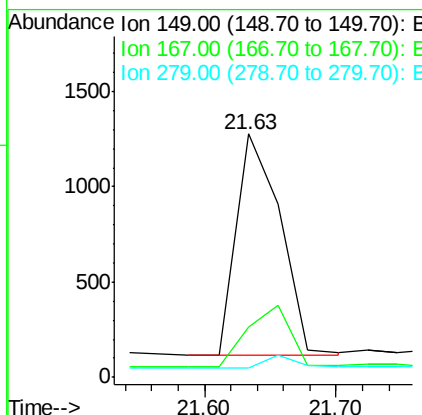

#30
 Indeno(1,2,3-cd)pyrene
 Concen: 0.41 ng
 RT: 26.62 min Scan# 1717
 Delta R.T. -0.00 min
 Lab File: BE092339.D
 Acq: 1 Sep 2016 21:27

Tgt Ion	Ratio	Lower	Upper
276	100		
138	25.5	20.3	30.5
277	24.8	19.7	29.5



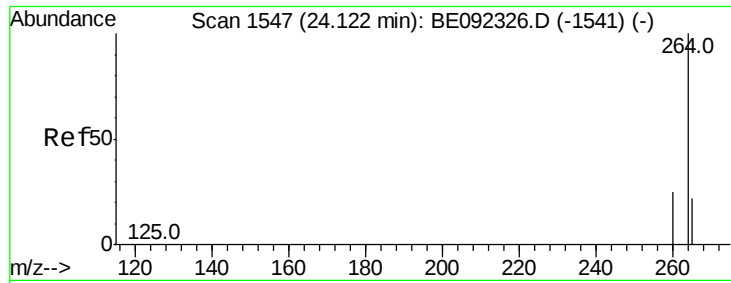





#31
Pervlene-d12
Concen: 5.00 ng
RT: 24.12 min Scan# 1547
Delta R.T. -0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.6	20.1	30.1
265	22.8	17.9	26.9




Manual Integrations
APPROVED


sohil
9/2/2016 4:34:16 PM

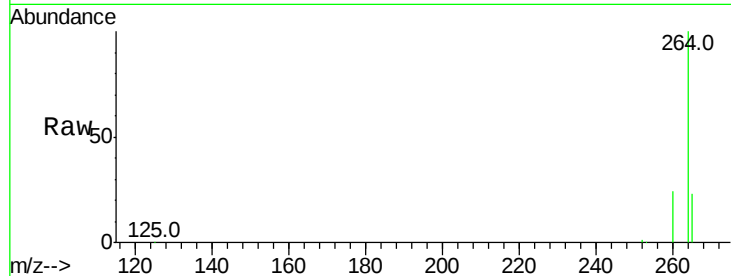

#32
Benzo(b)fluoranthene
Concen: 0.38 ng
RT: 23.38 min Scan# 1483
Delta R.T. -0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.8	18.7	28.1
125	12.6	10.5	15.7









#33
Benzo(k)fluoranthene
Concen: 0.44 ng
RT: 23.43 min Scan# 1487
Delta R.T. -0.01 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.9	20.3	30.5
125	12.3	9.6	14.4




Manual Integrations
APPROVED


sohil
9/2/2016 4:34:16 PM

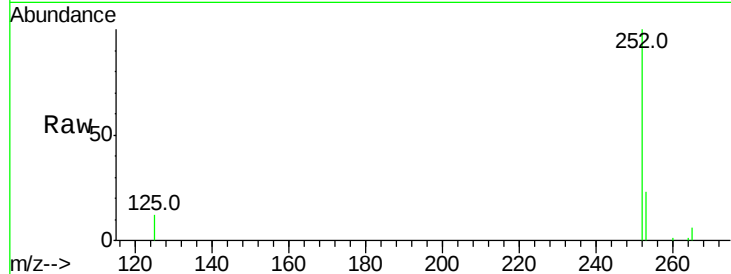

#34
Benzo(a)pyrene
Concen: 0.41 ng
RT: 24.01 min Scan# 1537
Delta R.T. -0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.9	19.0	28.6
125	13.9	11.8	17.8









#35
Dibenzo(a,h)anthracene
Concen: 0.40 ng
RT: 26.63 min Scan# 1718
Delta R.T. -0.02 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tot Ion	Ratio	Lower	Upper
278	100		
139	19.4	13.8	20.8
279	25.5	21.4	32.2

Manual Integrations
APPROVED

sohil
9/2/2016 4:34:16 PM



#36
Benzo(g,h,i)perylene
Concen: 0.41 ng
RT: 27.38 min Scan# 1762
Delta R.T. -0.00 min
Lab File: BE092339.D
Acq: 1 Sep 2016 21:27

Tgt Ion	Ratio	Lower	Upper
276	100		
277	25.3	19.8	29.8
138	23.9	19.8	29.6

