


Data Path : Z:\HPCHEM1\BNA E\Data\BE090116\
 Data File : BE092322.D
 Acq On : 1 Sep 2016 9:32
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 02 11:02:43 2016

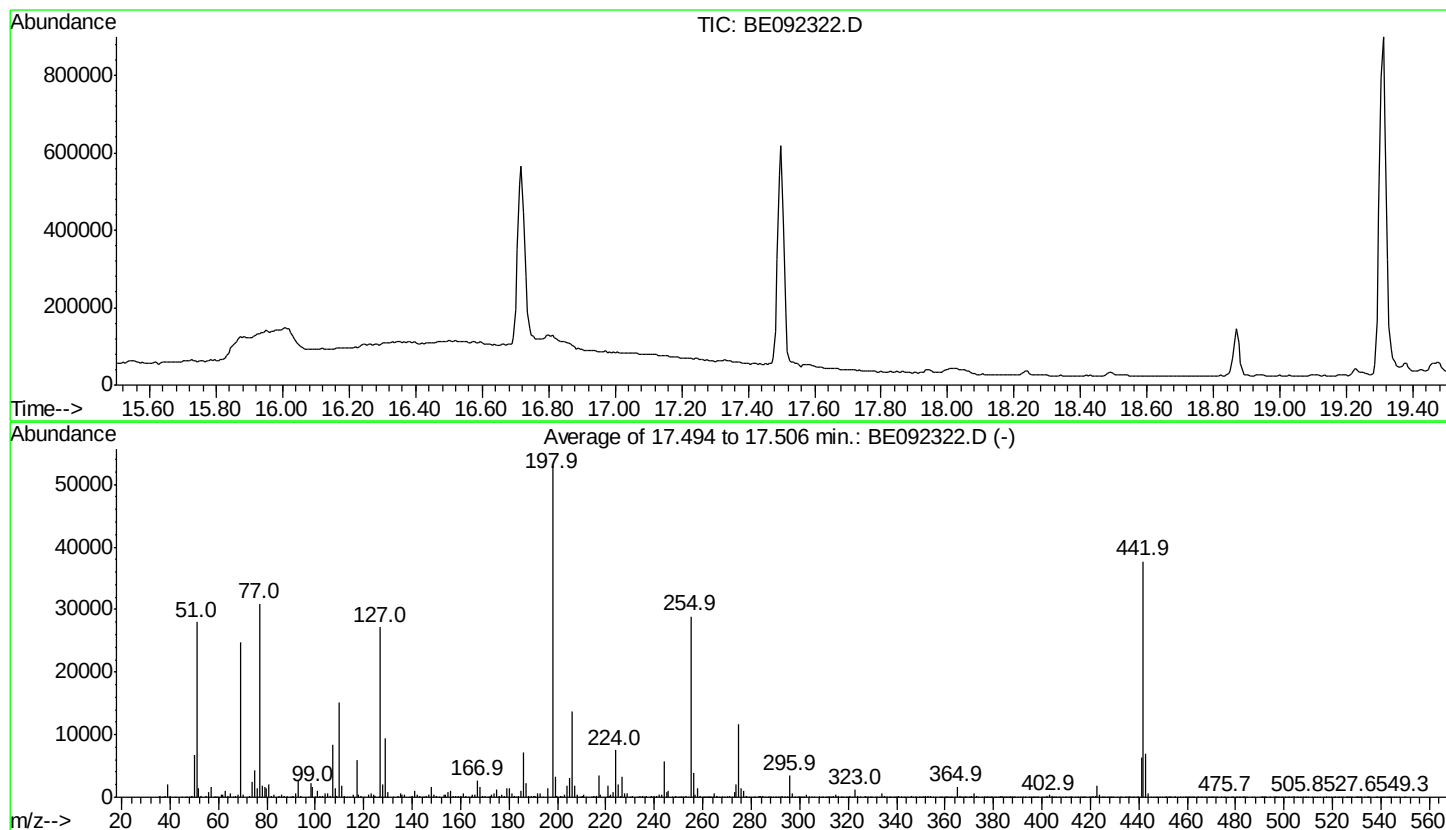

AutoFind: Scans 2537, 2538, 2539; Background Corrected with Scan 2527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.9	28024	PASS
68	69	0.00	2	1.7	412	PASS
69	198	0.00	100	46.6	24708	PASS
70	69	0.00	2	1.4	339	PASS
127	198	10	80	51.2	27141	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53005	PASS
199	198	5	9	6.3	3347	PASS
275	198	10	60	22.1	11697	PASS
365	198	1	100	3.1	1658	PASS
441	442	0.01	24	16.7	6307	PASS
442	198	50	100	71.1	37691	PASS
443	442	15	24	18.6	6999	PASS