
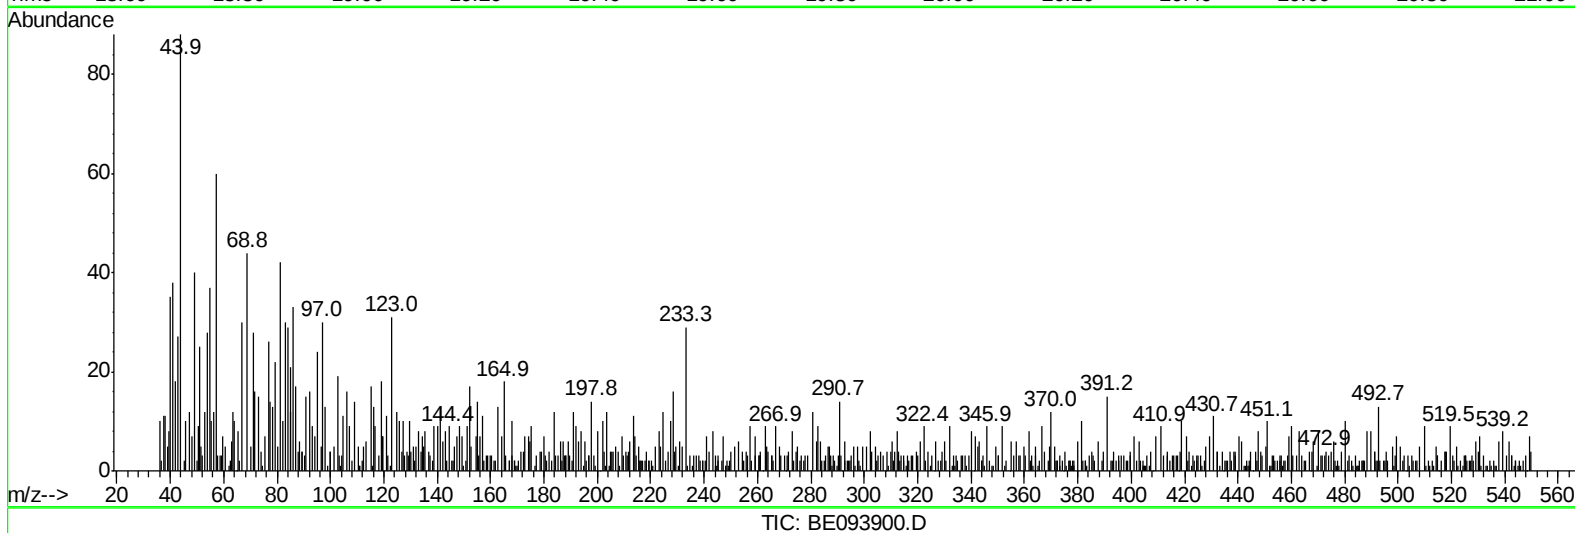


Data Path : Z:\HPCHEM1\BNA E\DATA\BE090117\
Data File : BE093900.D
Acq On : 1 Sep 2017 13:52
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 02:02:07 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

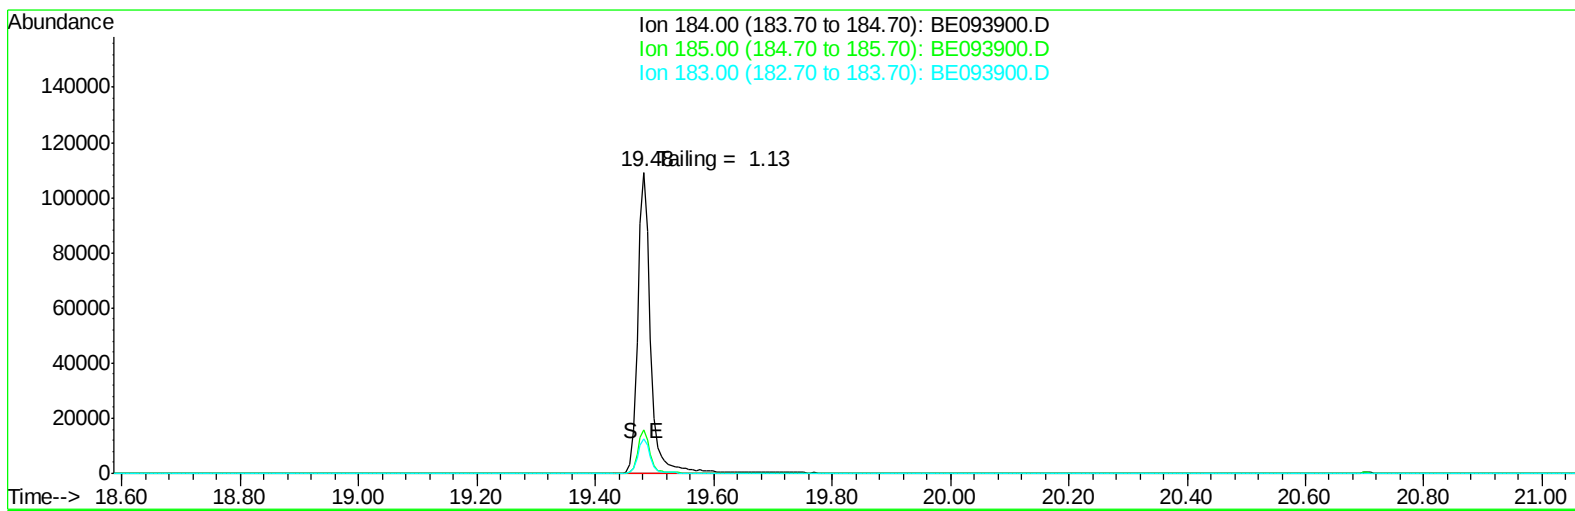

(76) Benzidine



12.608min (+0.010) 30.50ng

response 8

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	20.00
183.00	12.20	13.33
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE090117\
Data File : BE093900.D
Acq On : 1 Sep 2017 13:52
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 02:02:07 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

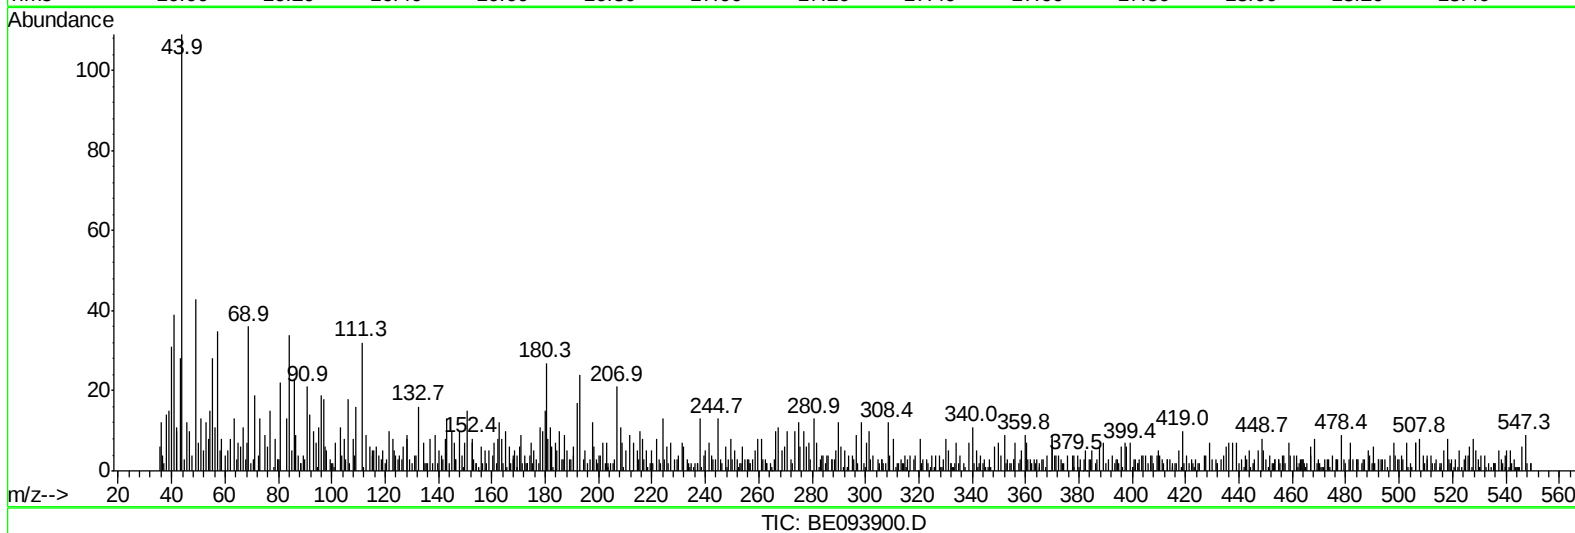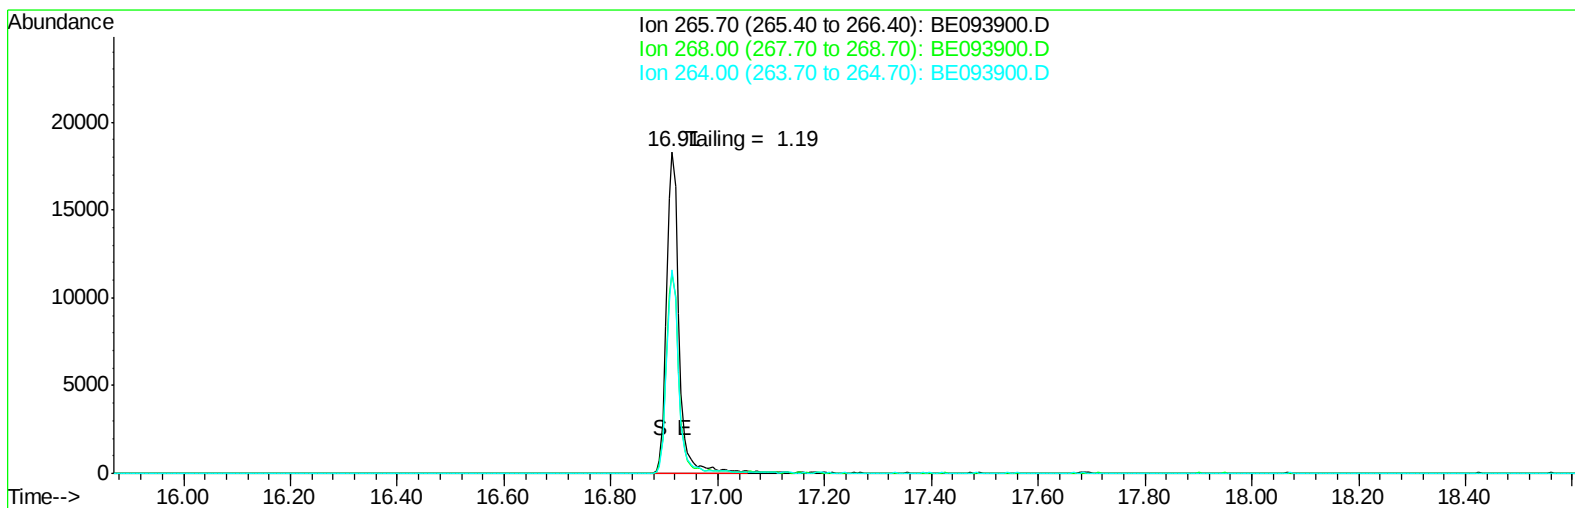

TIC: BE093900.D

(69) Pentachlorophenol (C)

11.098min (+0.029) 324.08ng

response 6

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	0.00#
264.00	64.60	15.38#
0.00	0.00	0.00