


Data Path : Z:\HPCHEM1\BNA_E\Data\BE090117\
 Data File : BE093900.D
 Acq On : 1 Sep 2017 13:52
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE082617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 01 16:31:36 2017

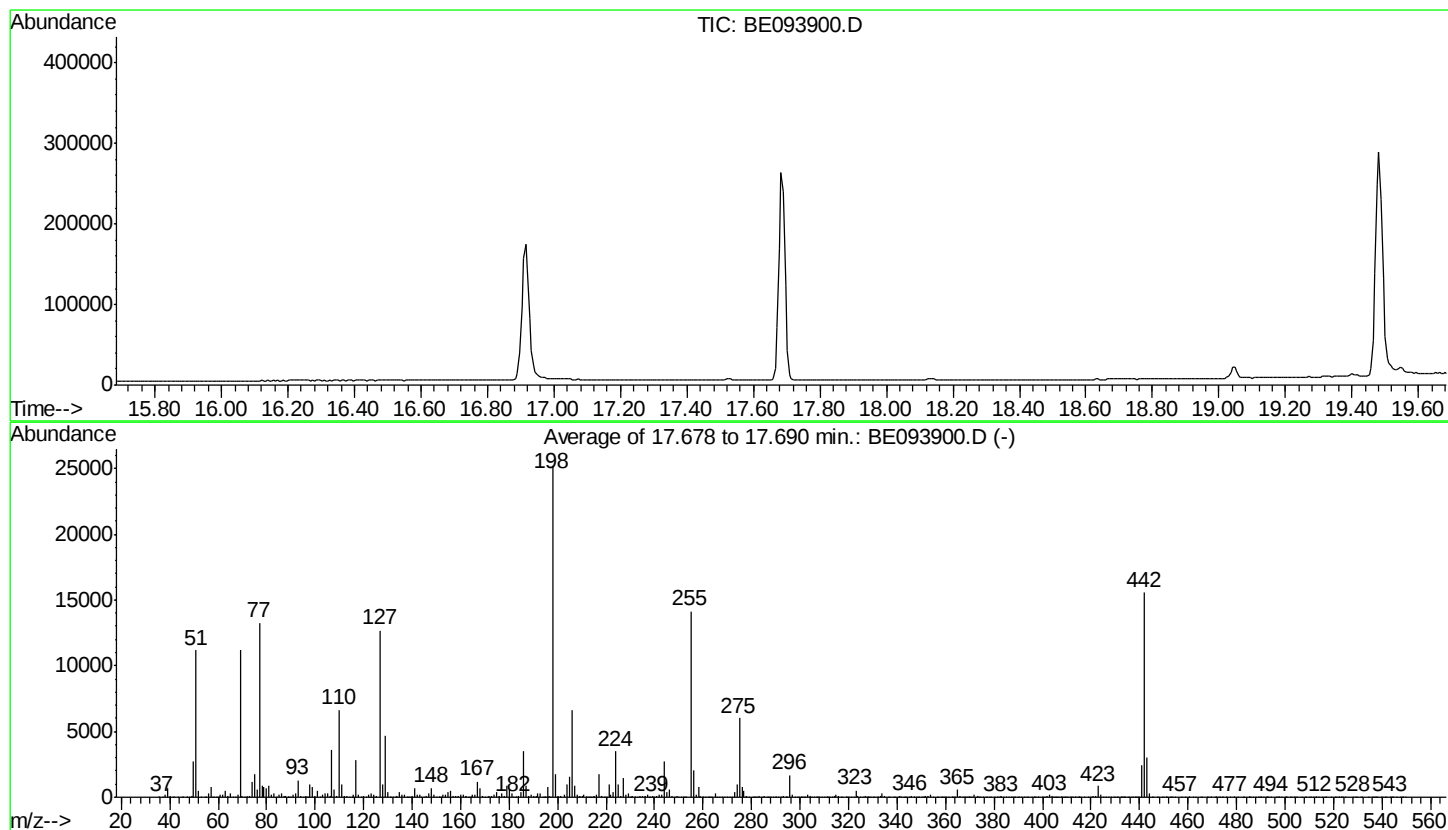

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2562

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	11186	PASS
68	69	0.00	2	1.4	154	PASS
69	198	0.00	100	44.2	11155	PASS
70	69	0.00	2	0.5	52	PASS
127	198	10	80	50.4	12705	PASS
197	198	0.00	2	0.2	53	PASS
198	198	100	100	100.0	25219	PASS
199	198	5	9	6.9	1732	PASS
275	198	10	60	23.8	5996	PASS
365	198	1	100	2.2	566	PASS
441	442	0.01	24	15.8	2466	PASS
442	198	50	100	61.7	15563	PASS
443	442	15	24	19.6	3045	PASS