
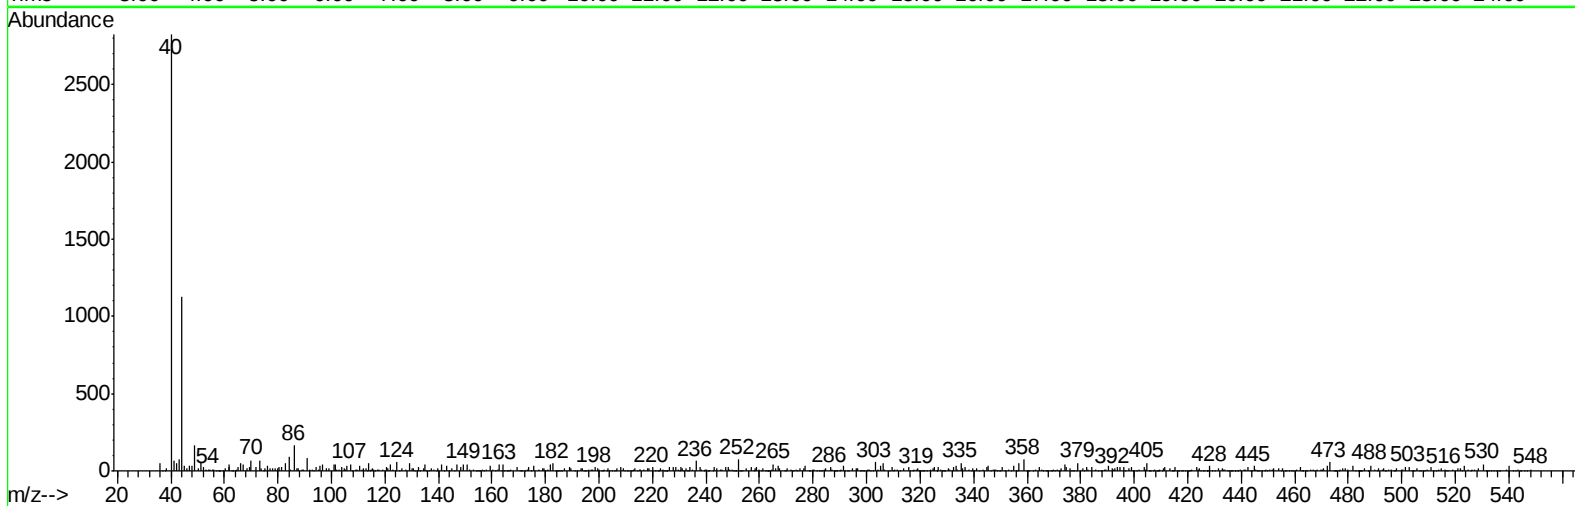


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE090215\
Data File : BE090703.D
Acq On : 2 Sep 2015 14:19
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 11:37:23 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-BE070114.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 02 05:40:44 2014
Response via : Initial Calibration

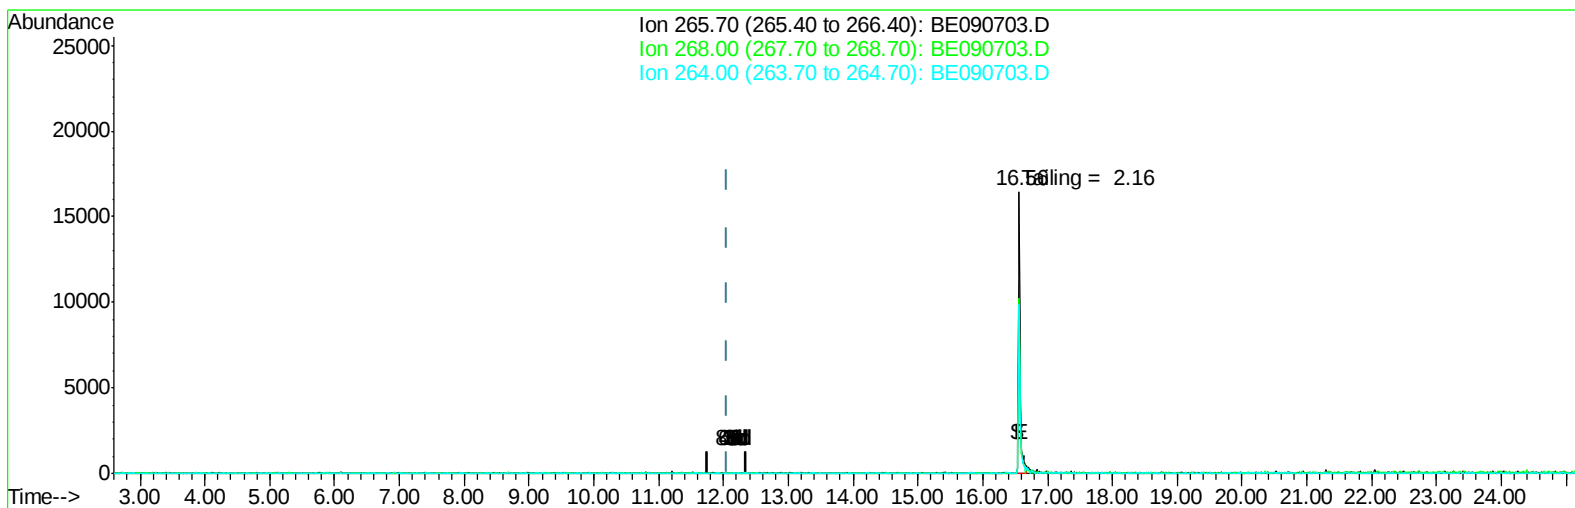

TIC: BE090703.D

(69) Pentachlorophenol (C)



12.153min (+0.090) 73.51ng

response 9

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	0.00#
264.00	62.10	73.33
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE090215\
Data File : BE090703.D
Acq On : 2 Sep 2015 14:19
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 11:37:23 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-BE070114.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 02 05:40:44 2014
Response via : Initial Calibration

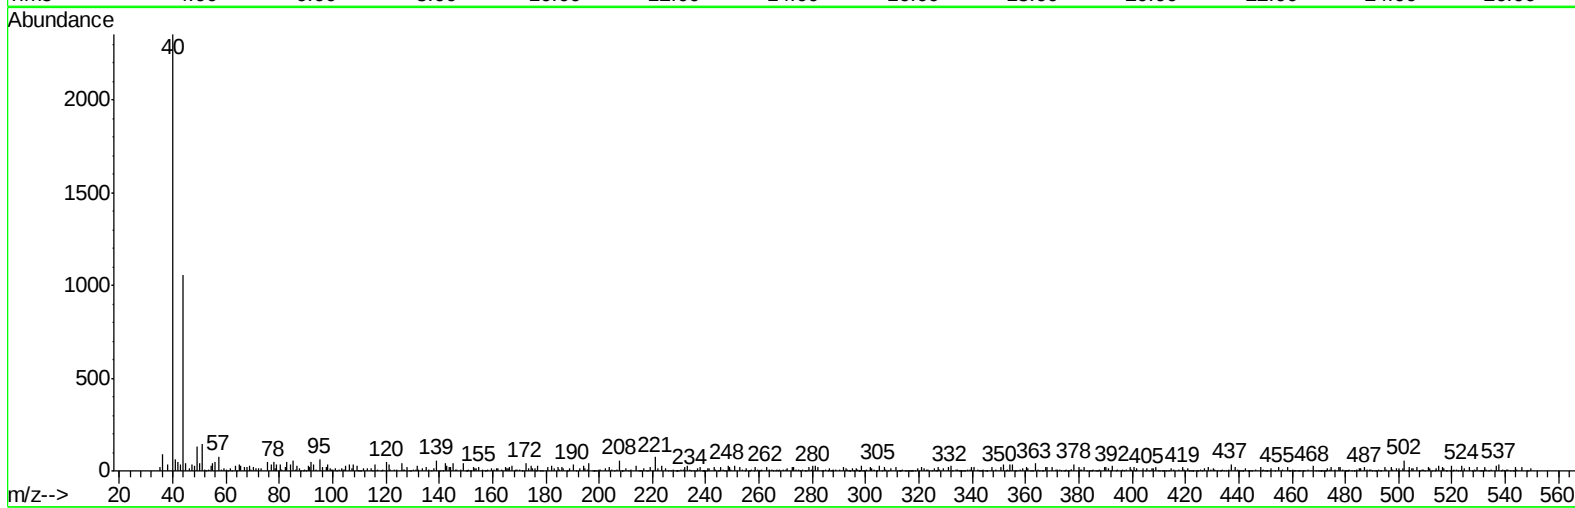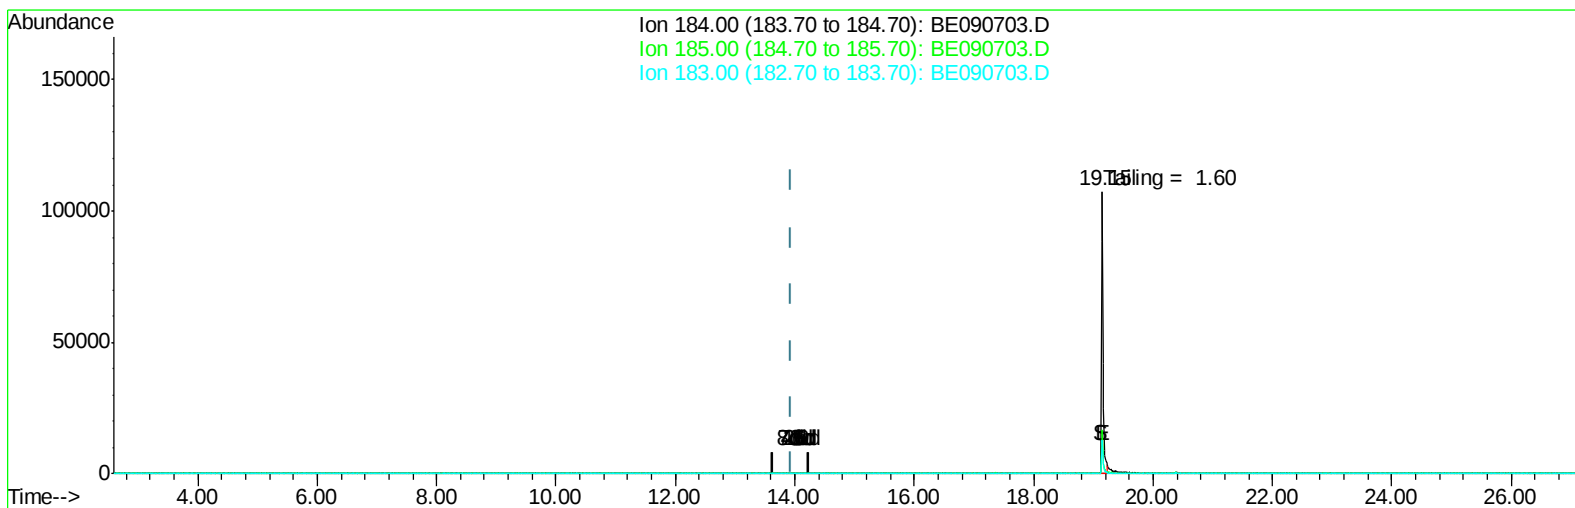

TIC: BE090703.D

(76) Benzidine

14.080min (+0.130) 36.18ng

response 14

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	36.36#
183.00	10.90	72.73#
0.00	0.00	0.00