


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE090215\
Data File : BE090703.D
Acq On : 2 Sep 2015 14:19
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 02 11:40:50 2015

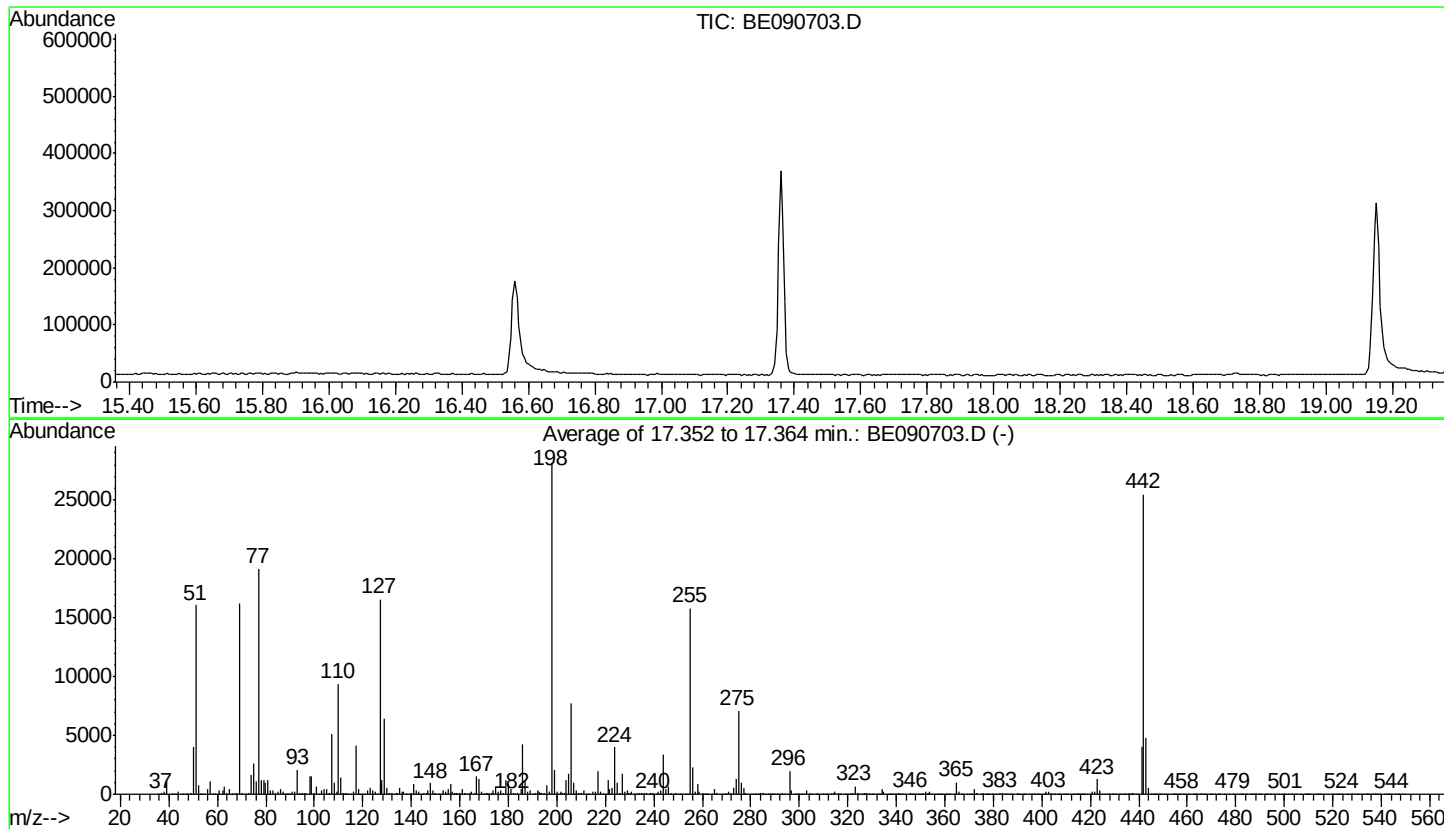

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.1	16071	PASS
68	69	0.00	2	0.4	61	PASS
69	198	0.00	100	57.4	16182	PASS
70	69	0.00	2	0.7	114	PASS
127	198	10	80	58.8	16574	PASS
197	198	0.00	2	0.7	187	PASS
198	198	100	100	100.0	28168	PASS
199	198	5	9	7.5	2102	PASS
275	198	10	60	25.1	7077	PASS
365	198	1	100	3.7	1029	PASS
441	442	0.01	24	16.0	4072	PASS
442	198	50	100	90.4	25462	PASS
443	442	15	24	18.8	4790	PASS