
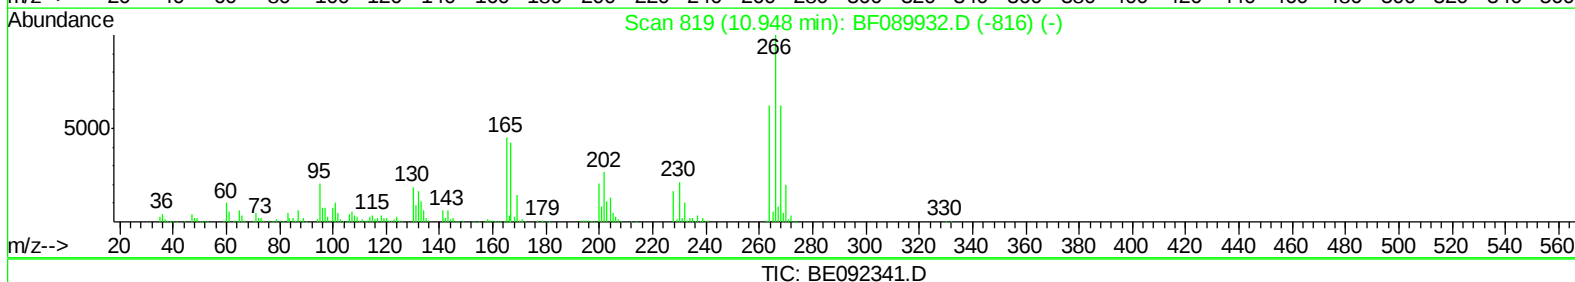
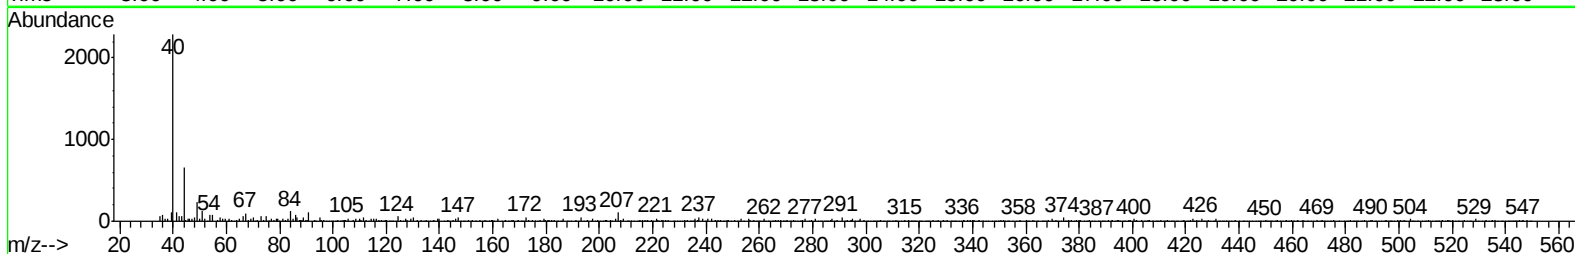


Data Path : Z:\HPCHEM1\BNA_E\Data\BE090216\
Data File : BE092341.D
Acq On : 2 Sep 2016 9:53
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 00:07:56 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 13:29:08 2016
Response via : Initial Calibration

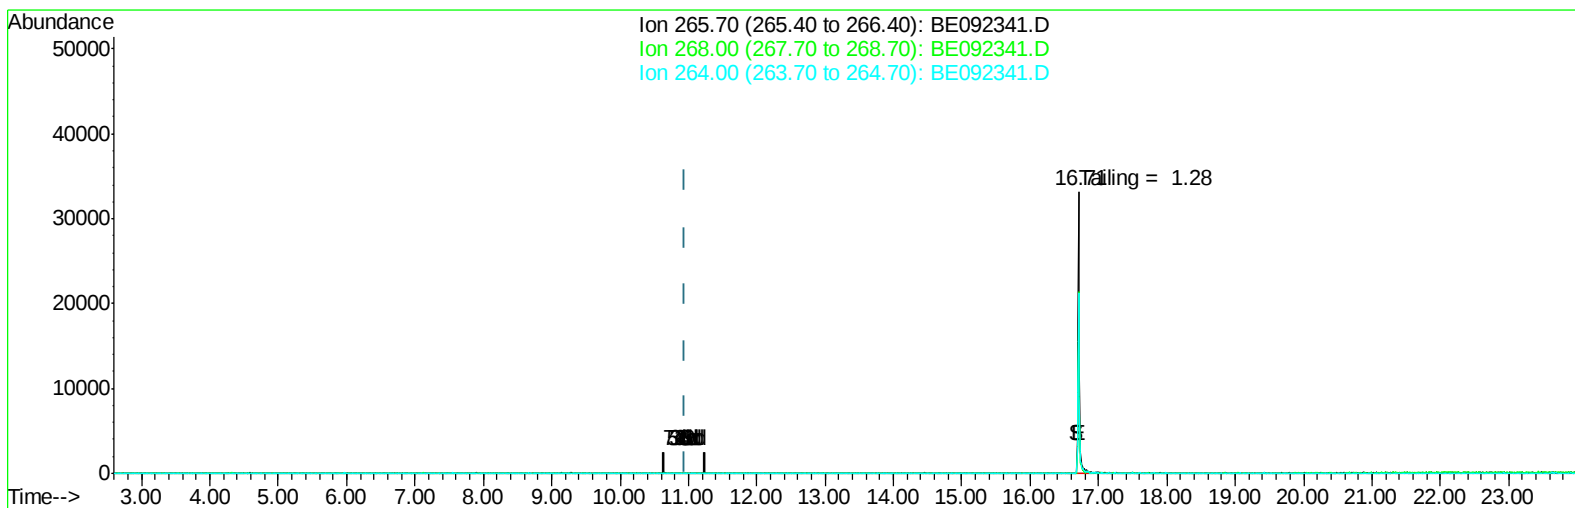

TIC: BE092341.D

(69) Pentachlorophenol (C)




10.925min (-0.022) 92.79ng

response 31

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	73.08
264.00	63.20	3.85#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE090216\
 Data File : BE092341.D
 Acq On : 2 Sep 2016 9:53
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 00:07:56 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 02 13:29:08 2016
 Response via : Initial Calibration

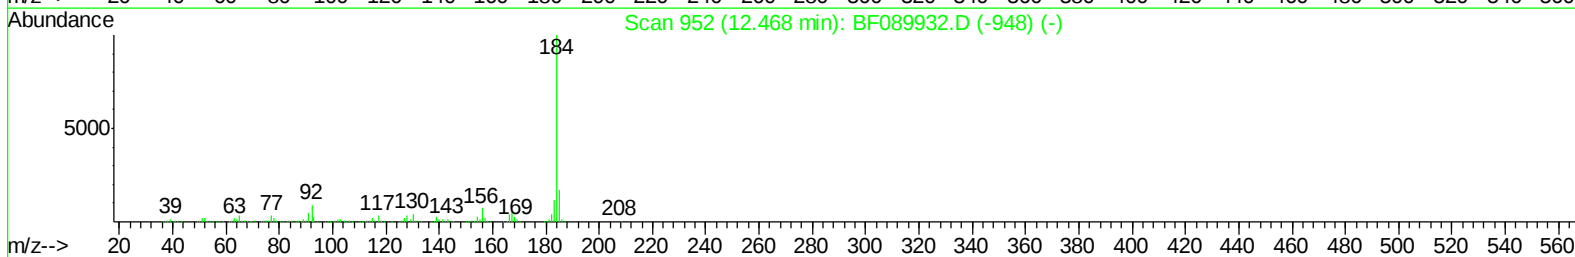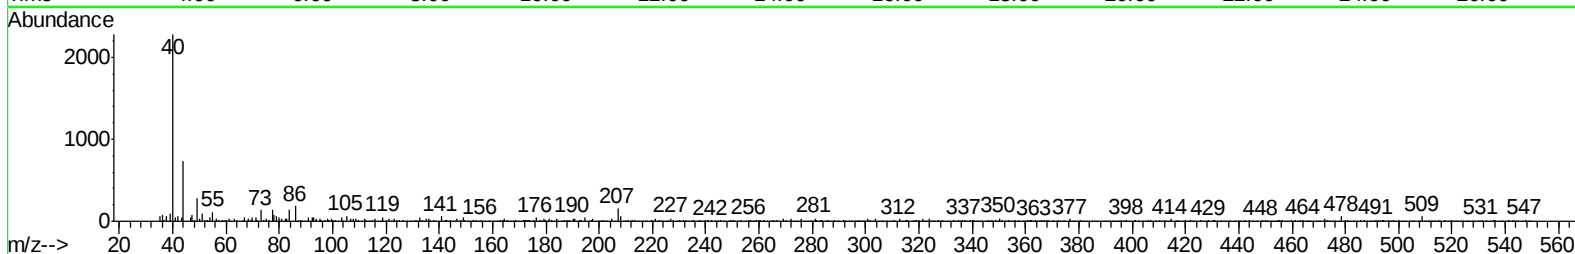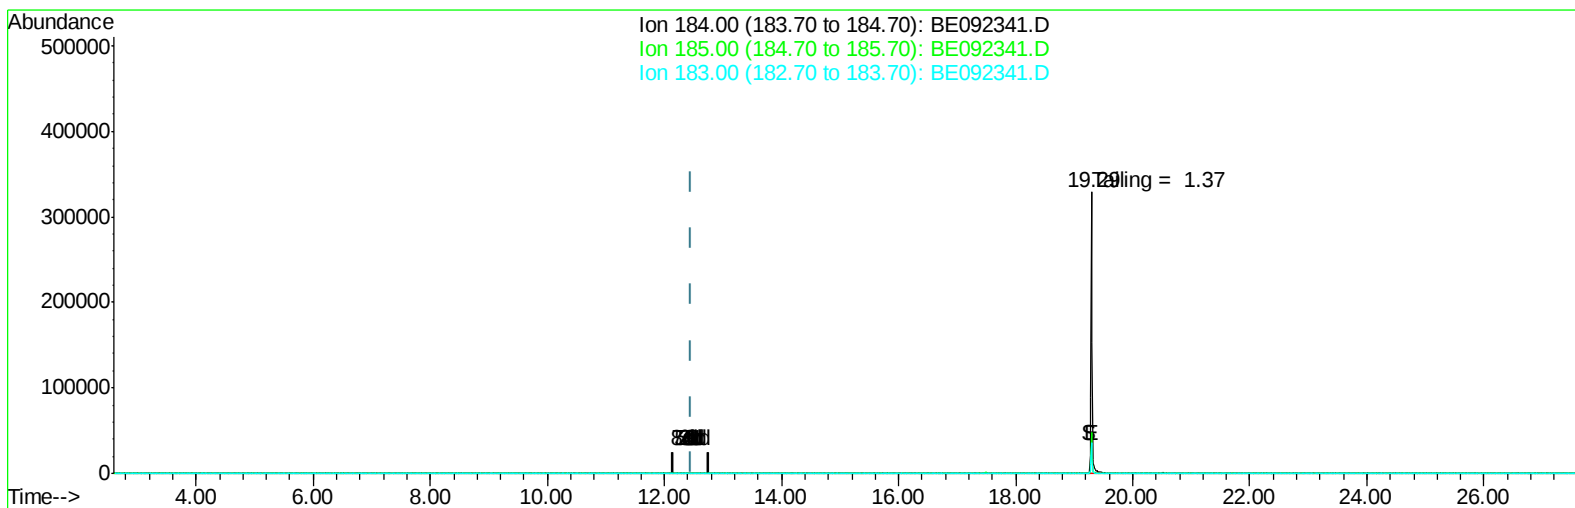

TIC: BE092341.D

(76) Benzidine

12.570min (+0.103) 12.97ng

response 29

Ion	Exp%	Act%
184.00	100	100
185.00	17.30	17.65
183.00	12.00	11.76
0.00	0.00	0.00