


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA E\Data\BE090517\
 Data File : BE093927.D
 Acq On : 5 Sep 2017 8:52
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 05 13:34:56 2017

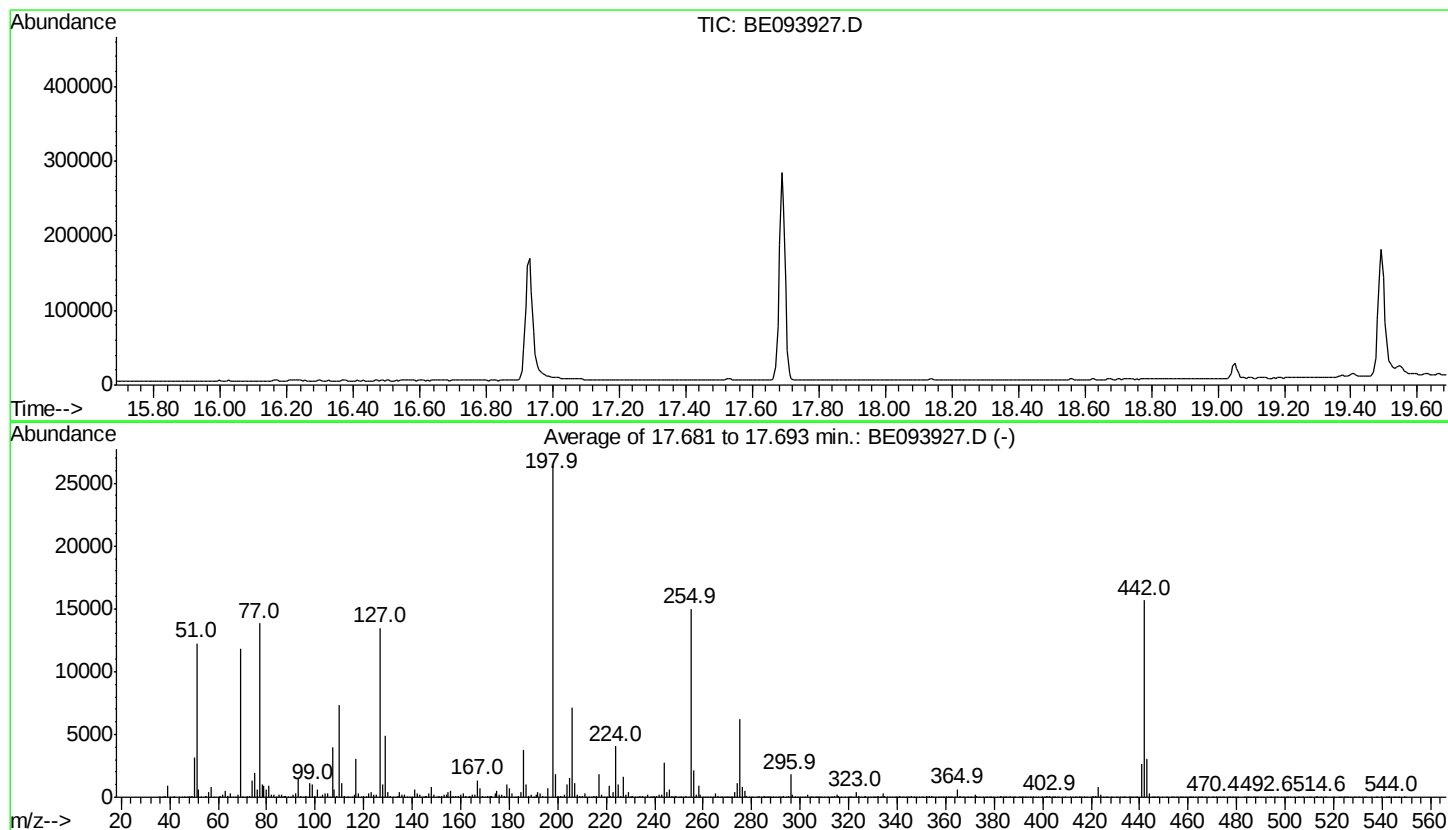

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2562

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.5	12272	PASS
68	69	0.00	2	1.5	183	PASS
69	198	0.00	100	44.8	11820	PASS
70	69	0.00	2	0.3	35	PASS
127	198	10	80	51.1	13489	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26396	PASS
199	198	5	9	7.1	1884	PASS
275	198	10	60	23.4	6174	PASS
365	198	1	100	2.5	662	PASS
441	442	0.01	24	17.0	2661	PASS
442	198	50	100	59.3	15659	PASS
443	442	15	24	19.9	3109	PASS