


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA E\Data\BE090517\
 Data File : BE093935.D
 Acq On : 5 Sep 2017 14:00
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 05 13:34:56 2017

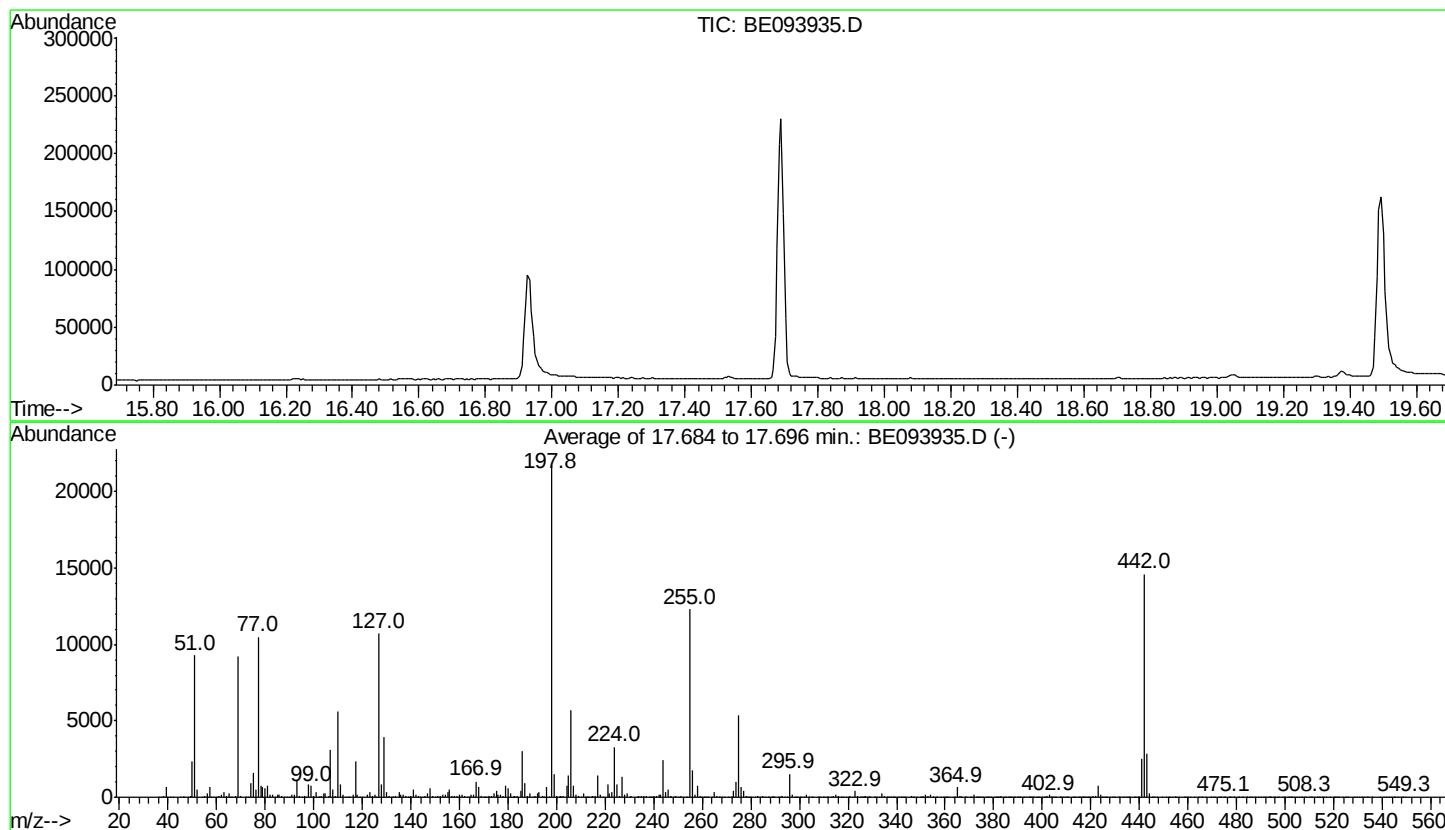

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	9259	PASS
68	69	0.00	2	0.9	81	PASS
69	198	0.00	100	42.6	9241	PASS
70	69	0.00	2	0.5	45	PASS
127	198	10	80	49.3	10701	PASS
197	198	0.00	2	0.1	30	PASS
198	198	100	100	100.0	21694	PASS
199	198	5	9	6.9	1492	PASS
275	198	10	60	24.7	5364	PASS
365	198	1	100	3.0	645	PASS
441	442	0.01	24	17.1	2493	PASS
442	198	50	100	67.2	14589	PASS
443	442	15	24	19.7	2875	PASS