
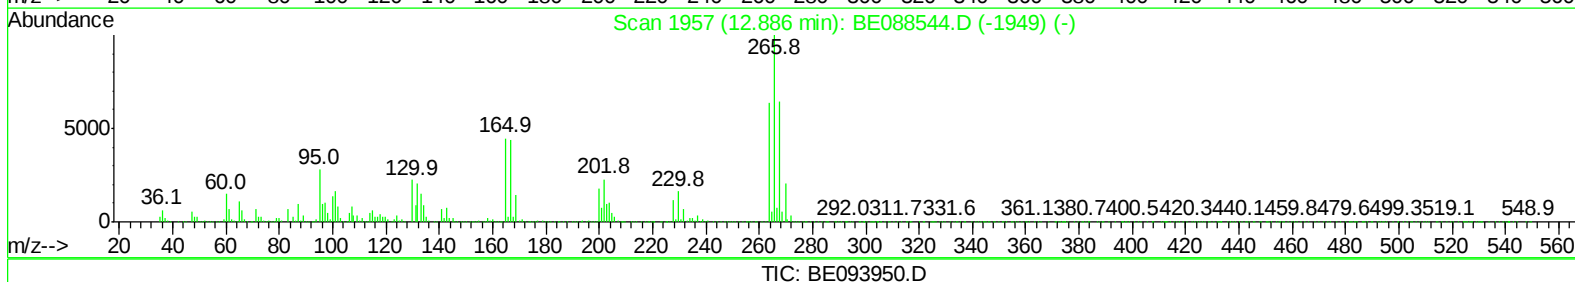
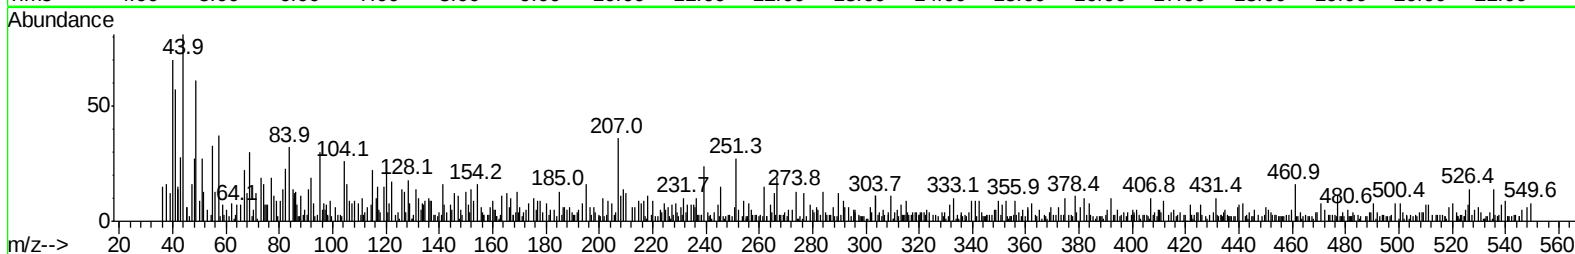


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE090617\
Data File : BE093950.D
Acq On : 6 Sep 2017 9:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 11:53:29 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-BE110514.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 06 14:19:16 2014
Response via : Initial Calibration

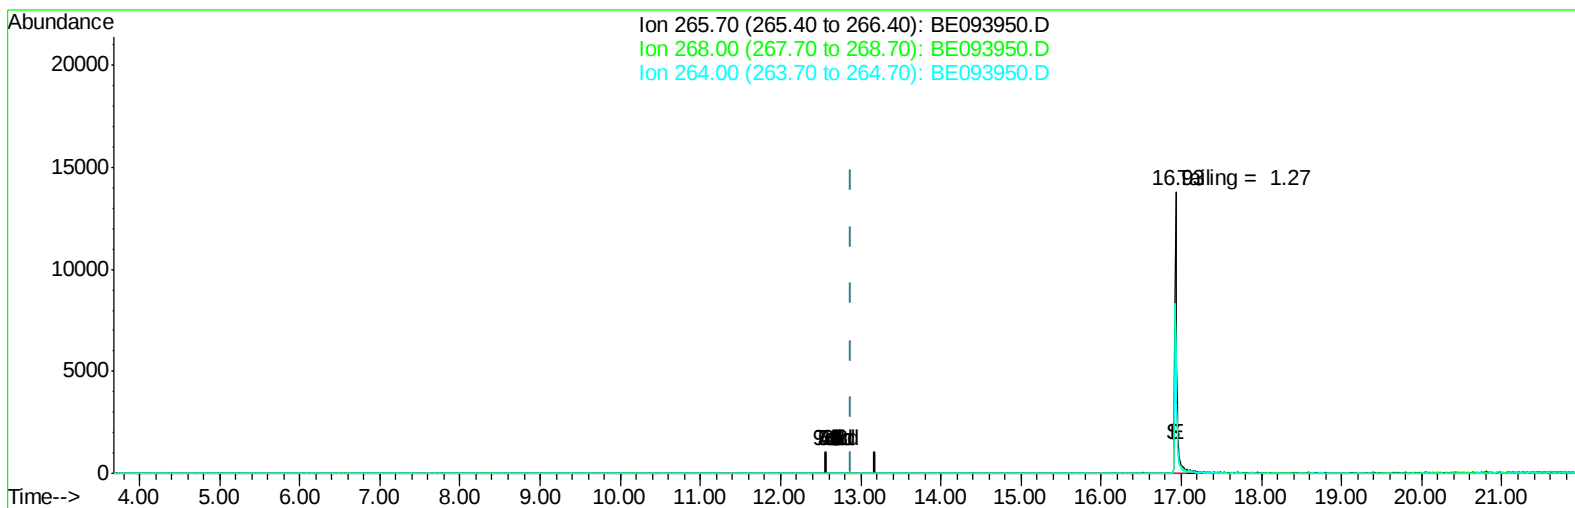

TIC: BE093950.D

(69) Pentachlorophenol (C)




12.711min (-0.175) 541.12ng

response 17

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	40.00#
264.00	63.70	73.33
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE090617\
 Data File : BE093950.D
 Acq On : 6 Sep 2017 9:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 11:53:29 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-BE110514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 06 14:19:16 2014
 Response via : Initial Calibration

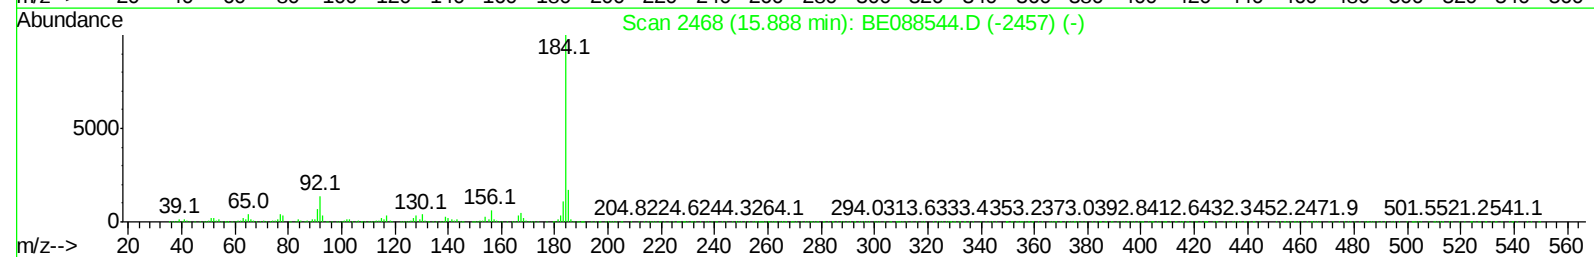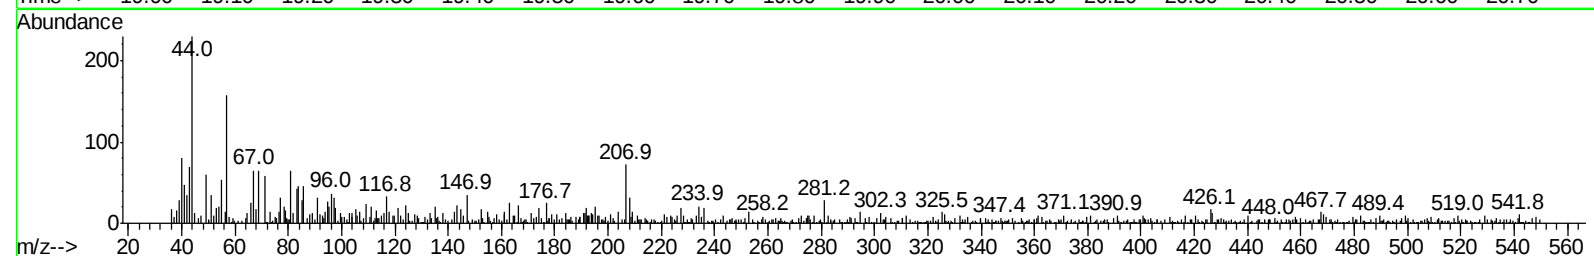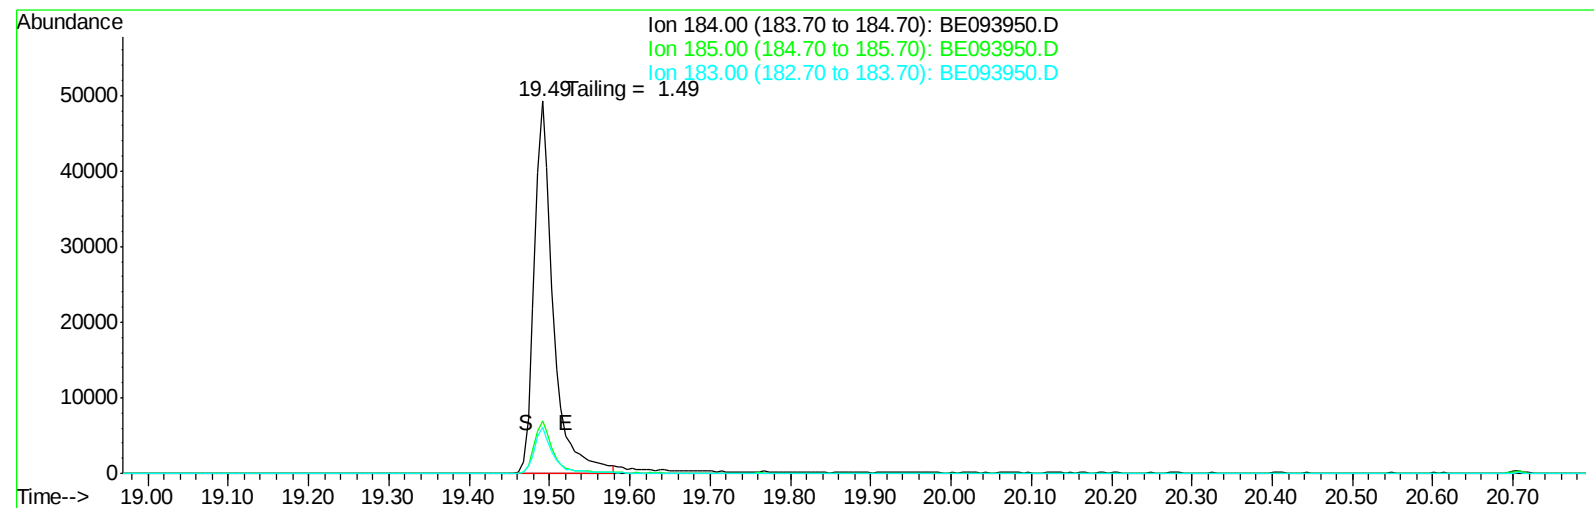

TIC: BE093950.D

(76) Benzidine




15.660min (-0.228) 86.02ng

response 17

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	77.78#
183.00	10.70	0.00#
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE090617\
 Data File : BE093950.D
 Acq On : 6 Sep 2017 9:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 11:53:29 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-BE110514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 06 14:19:16 2014
 Response via : Initial Calibration

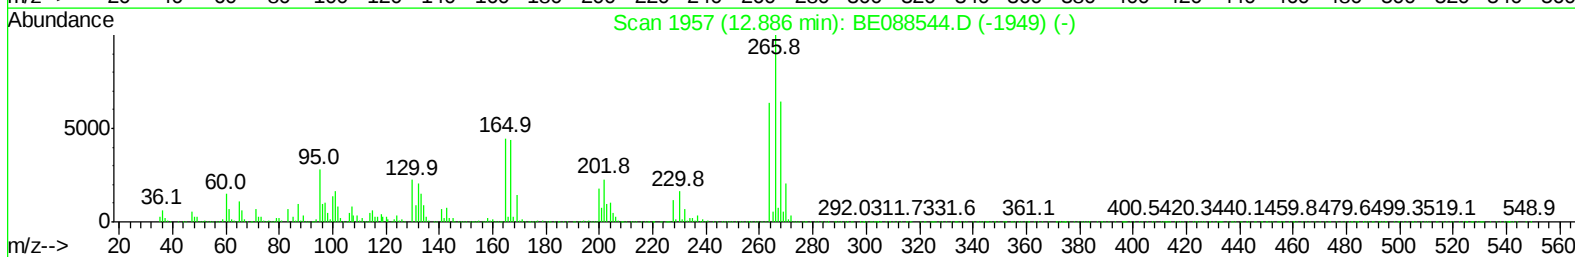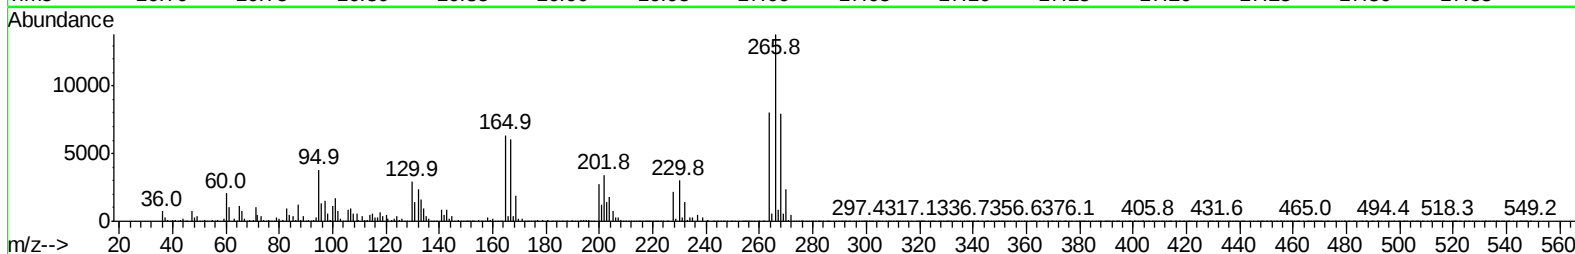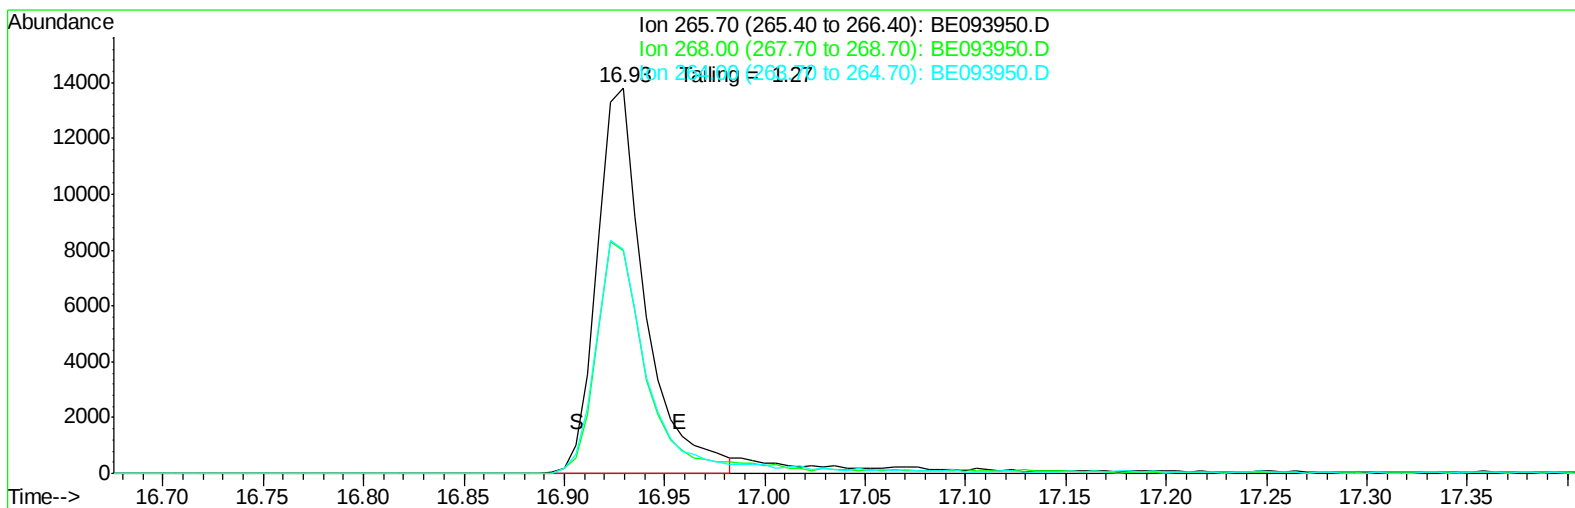

TIC: BE093950.D

(69) Pentachlorophenol (C)




16.929min (+4.044) 730156.59ng m

response 22939

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	57.66
264.00	63.70	58.08
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE090617\
 Data File : BE093950.D
 Acq On : 6 Sep 2017 9:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 11:53:29 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-BE110514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 06 14:19:16 2014
 Response via : Initial Calibration

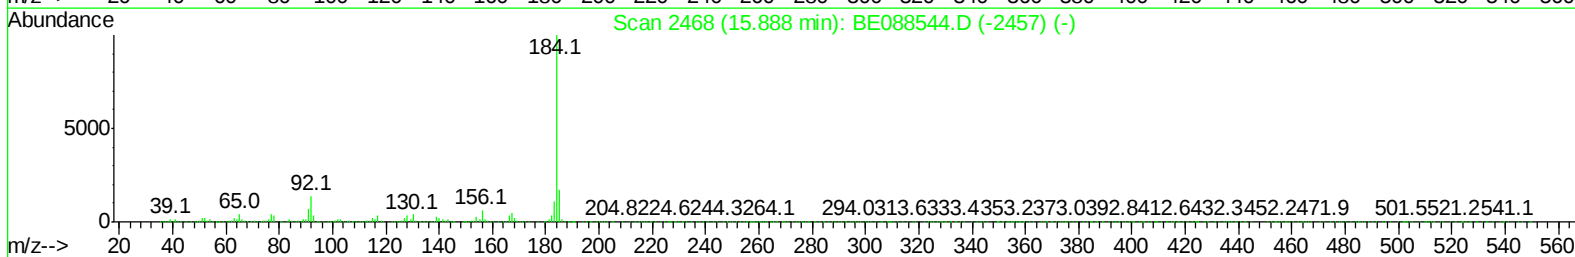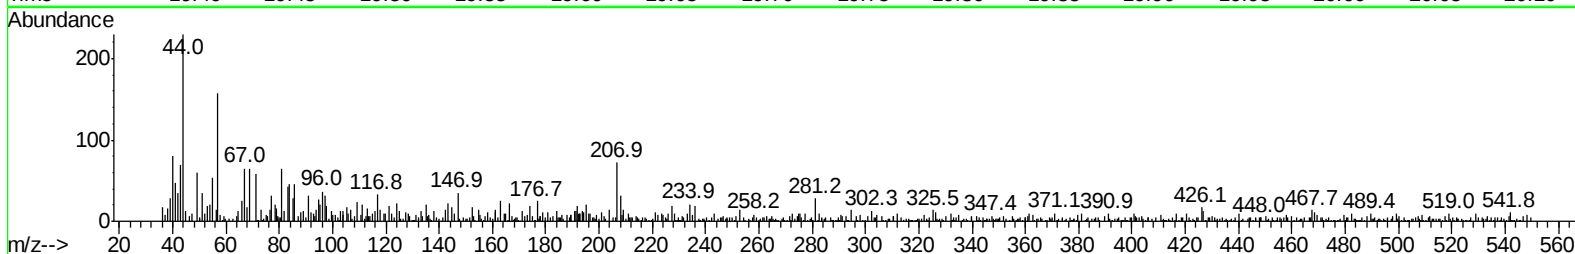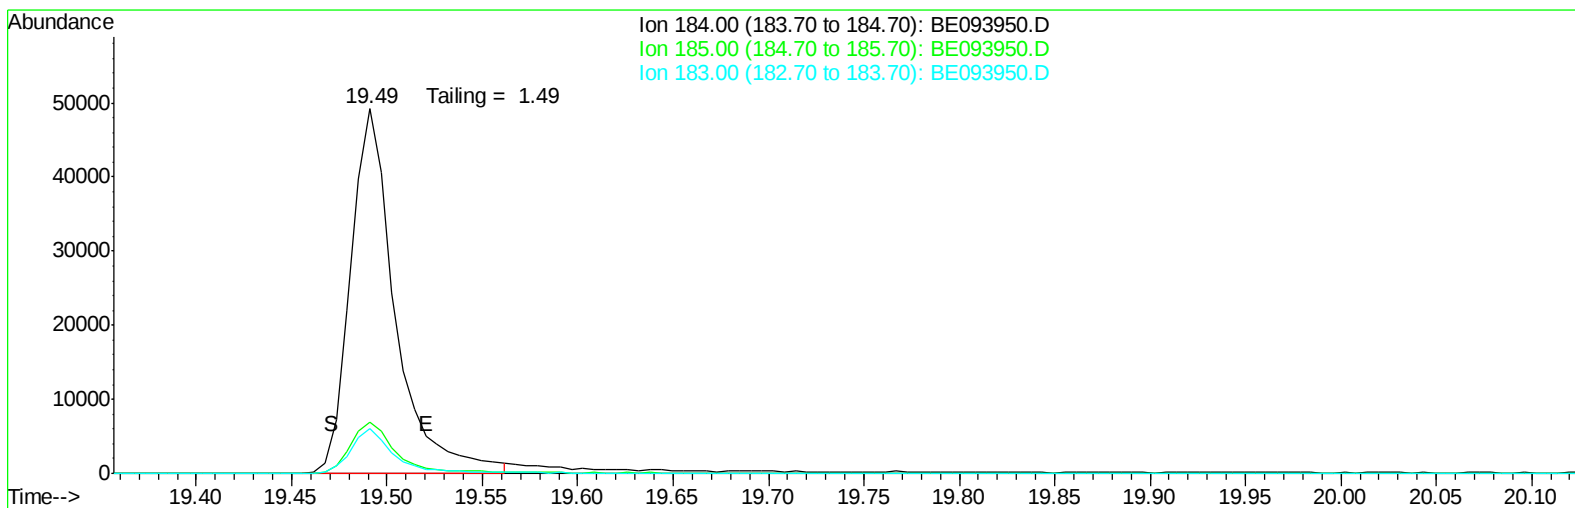

TIC: BE093950.D

(76) Benzidine

15.660min (-0.228) 86.02ng

response 17

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	77.78#
183.00	10.70	0.00#
0.00	0.00	0.00