


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE090617\
 Data File : BE093950.D
 Acq On : 6 Sep 2017 9:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 05 13:34:56 2017

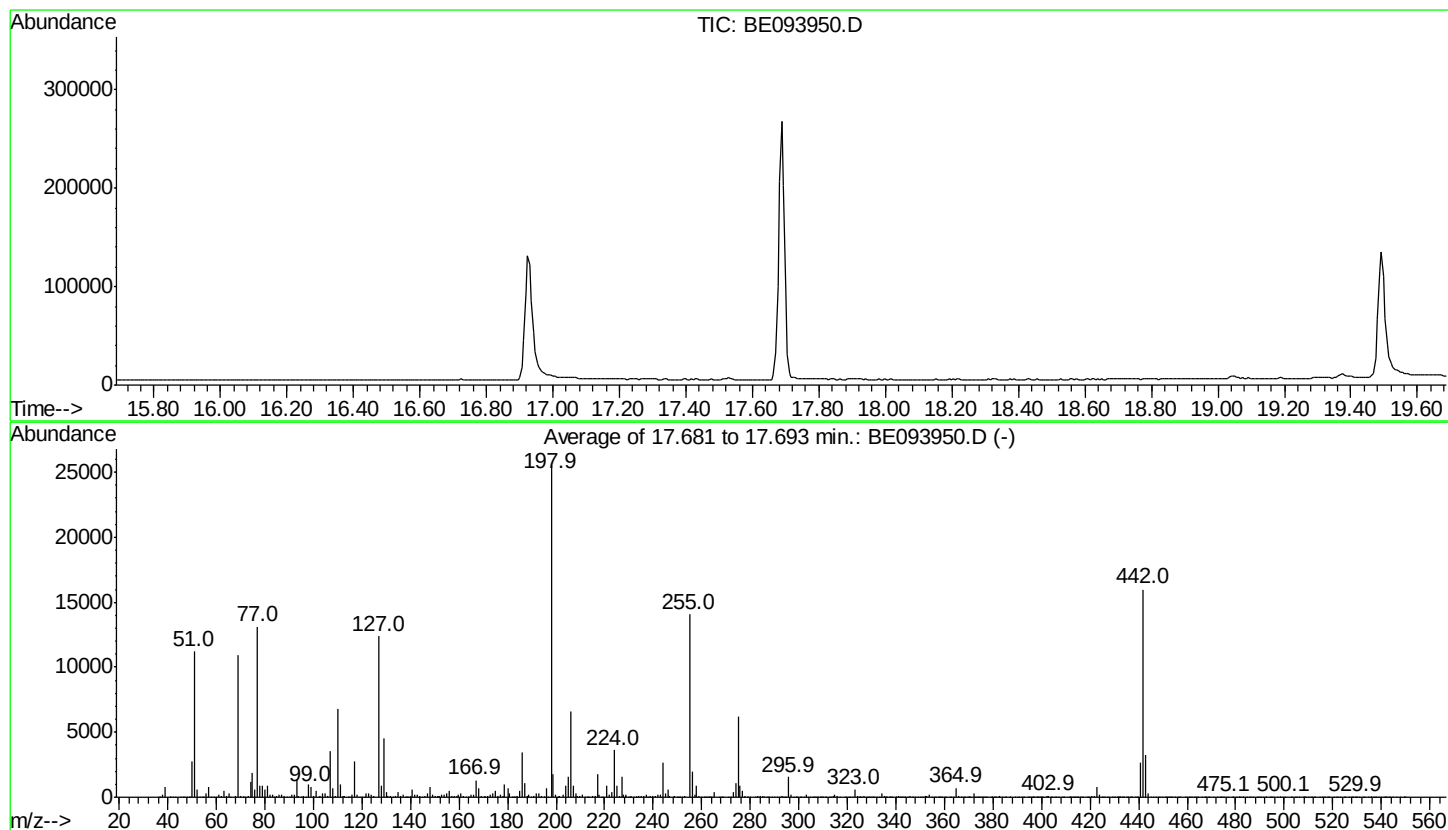

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2560

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	11188	PASS
68	69	0.00	2	0.7	78	PASS
69	198	0.00	100	42.7	10887	PASS
70	69	0.00	2	0.8	83	PASS
127	198	10	80	48.5	12384	PASS
197	198	0.00	2	0.2	40	PASS
198	198	100	100	100.0	25510	PASS
199	198	5	9	6.9	1771	PASS
275	198	10	60	24.3	6201	PASS
365	198	1	100	2.7	696	PASS
441	442	0.01	24	16.5	2641	PASS
442	198	50	100	62.7	15987	PASS
443	442	15	24	20.2	3231	PASS