
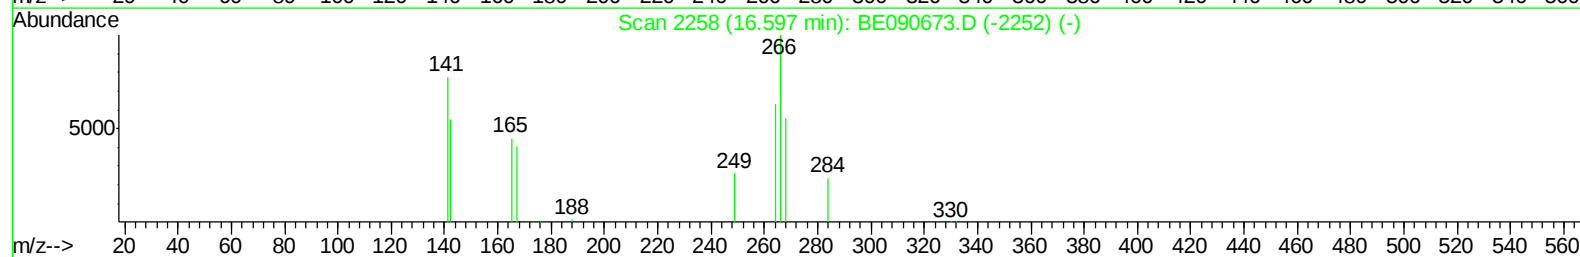
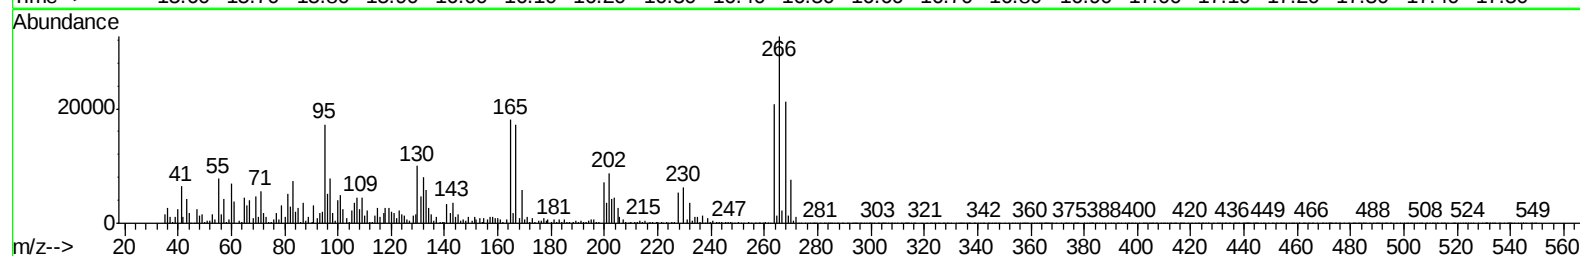


Data Path : Z:\HPCHEM1\BNA E\Data\BE090815\
Data File : BE090746.D
Acq On : 8 Sep 2015 9:12
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 01:19:04 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 11:40:50 2015
Response via : Initial Calibration

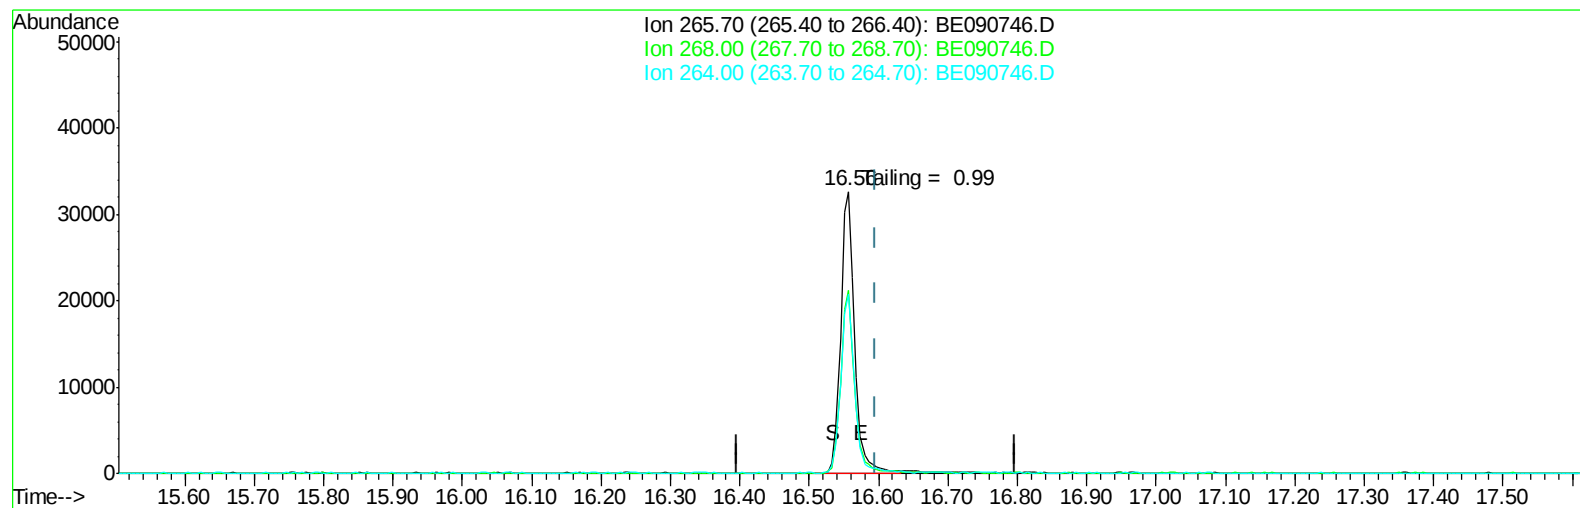

TIC: BE090746.D

(21) Pentachlorophenol

16.556min (-0.041) 30745.41ng

response 45739

Ion	Exp%	Act%
265.70	100	100
268.00	62.00	65.08
264.00	67.40	63.56
0.00	0.00	0.00