


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE090815\
Data File : BE090746.D
Acq On : 8 Sep 2015 9:12
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 02 11:40:50 2015

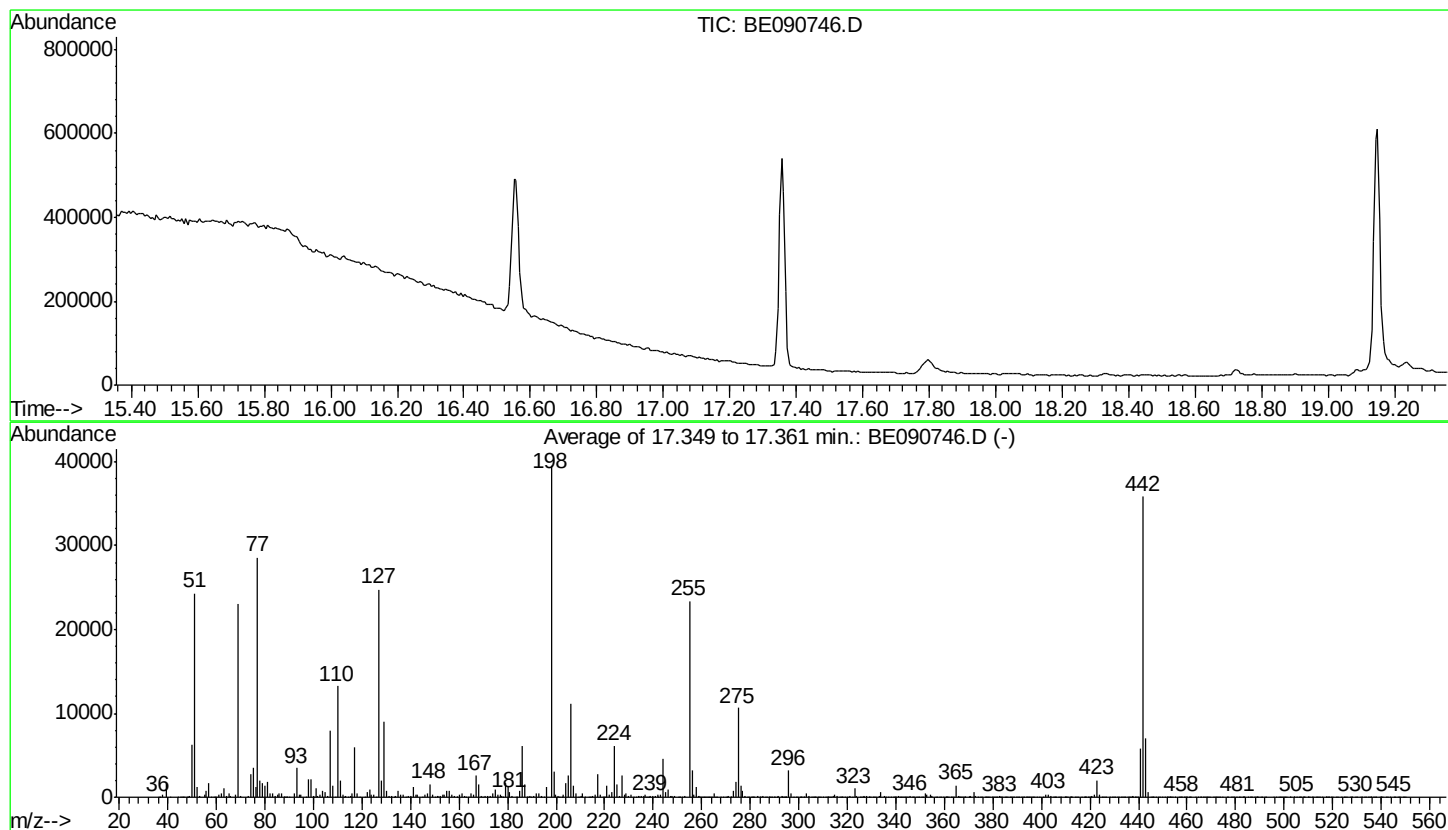

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.5	24306	PASS
68	69	0.00	2	1.1	260	PASS
69	198	0.00	100	58.5	23120	PASS
70	69	0.00	2	0.5	117	PASS
127	198	10	80	62.7	24791	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39531	PASS
199	198	5	9	7.8	3072	PASS
275	198	10	60	27.0	10682	PASS
365	198	1	100	3.6	1415	PASS
441	442	0.01	24	16.3	5822	PASS
442	198	50	100	90.6	35813	PASS
443	442	15	24	19.5	6991	PASS