


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE090916\
 Data File : BE092355.D
 Acq On : 9 Sep 2016 12:55
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 02 19:34:51 2016

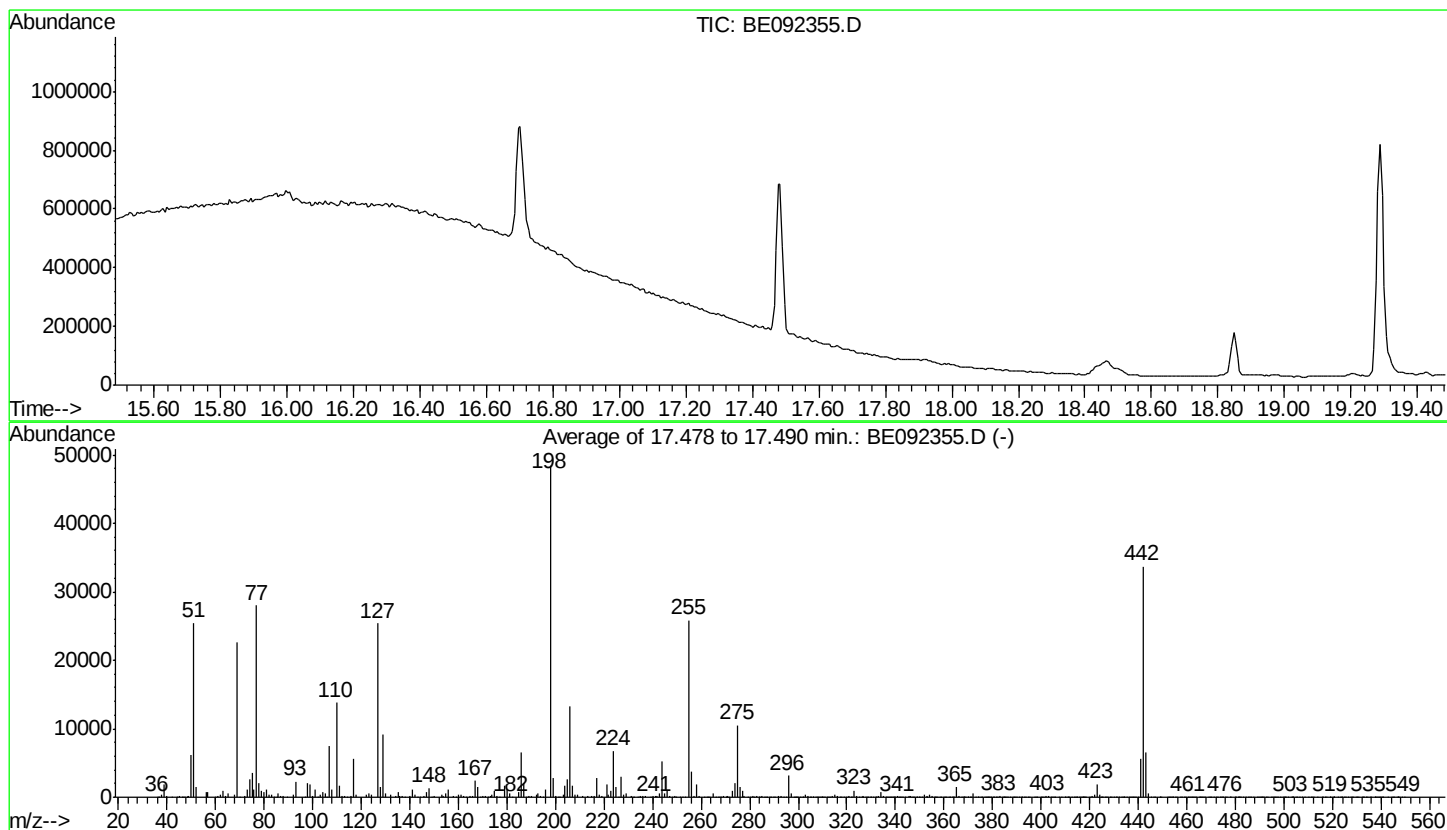

AutoFind: Scans 2534, 2535, 2536; Background Corrected with Scan 2527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.6	25477	PASS
68	69	0.00	2	1.4	318	PASS
69	198	0.00	100	46.6	22571	PASS
70	69	0.00	2	0.3	77	PASS
127	198	10	80	52.5	25411	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48416	PASS
199	198	5	9	5.9	2850	PASS
275	198	10	60	21.7	10512	PASS
365	198	1	100	3.1	1499	PASS
441	442	0.01	24	16.8	5667	PASS
442	198	50	100	69.7	33723	PASS
443	442	15	24	19.2	6467	PASS