

Data Path : Z:\HPCHEM1\BNA E\DATA\BE091015\
 Data File : BE090764.D
 Acq On : 10 Sep 2015 16:55
 Operator : UM/IZ
 Sample : G3598-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 090515-D534-F-D-B

Quant Time: Sep 11 02:52:37 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE090115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 02 11:40:50 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	43424	5.00	ng	0.00
6) Naphthalene-d8	10.31	136	194466	5.00	ng	0.00
12) Acenaphthene-d10	14.17	164	98716	5.00	ng	0.00
18) Phenanthrene-d10	16.91	188	238782	5.00	ng	0.00
25) Chrysene-d12	21.07	240	296772	5.00	ng	0.00
32) Perylene-d12	23.36	264	269050	5.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.18	112	30948	3.67	ng	0.00
5) Phenol-d6	6.75	99	27864	2.30	ng	0.00
7) Nitrobenzene-d5	8.71	82	50037	3.89	ng	0.00
13) 2,4,6-Tribromophenol	15.67	330	23527	8.12	ng	0.00
14) 2-Fluorobiphenyl	12.79	172	110751	4.05	ng	0.00
27) Terphenyl-d14	19.53	244	189551	5.77	ng	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.20	88	21	Below Cal	#	16
3) n-Nitrosodimethylamine	3.46	42	97	Below Cal	#	1
8) Nitrobenzene	8.76	77	29	0.11 ng	#	74
20) Hexachlorobenzene	16.23	284	203	Below Cal	#	56
21) Pentachlorophenol	16.60	266	33	0.47 ng	#	62
29) Chrysene	21.11	228	595	Below Cal	#	66
30) Bis(2-ethylhexyl)phthalate	21.00	149	4884	0.35 ng		97
36) Dibenzo(a,h)anthracene	25.72	278	31	0.14 ng	#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE091015\
Data File : BE090764.D
Acq On : 10 Sep 2015 16:55
Operator : UM/IZ
Sample : G3598-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
090515-D534-F-D-B

Quant Time: Sep 11 02:52:37 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 11:40:50 2015
Response via : Initial Calibration

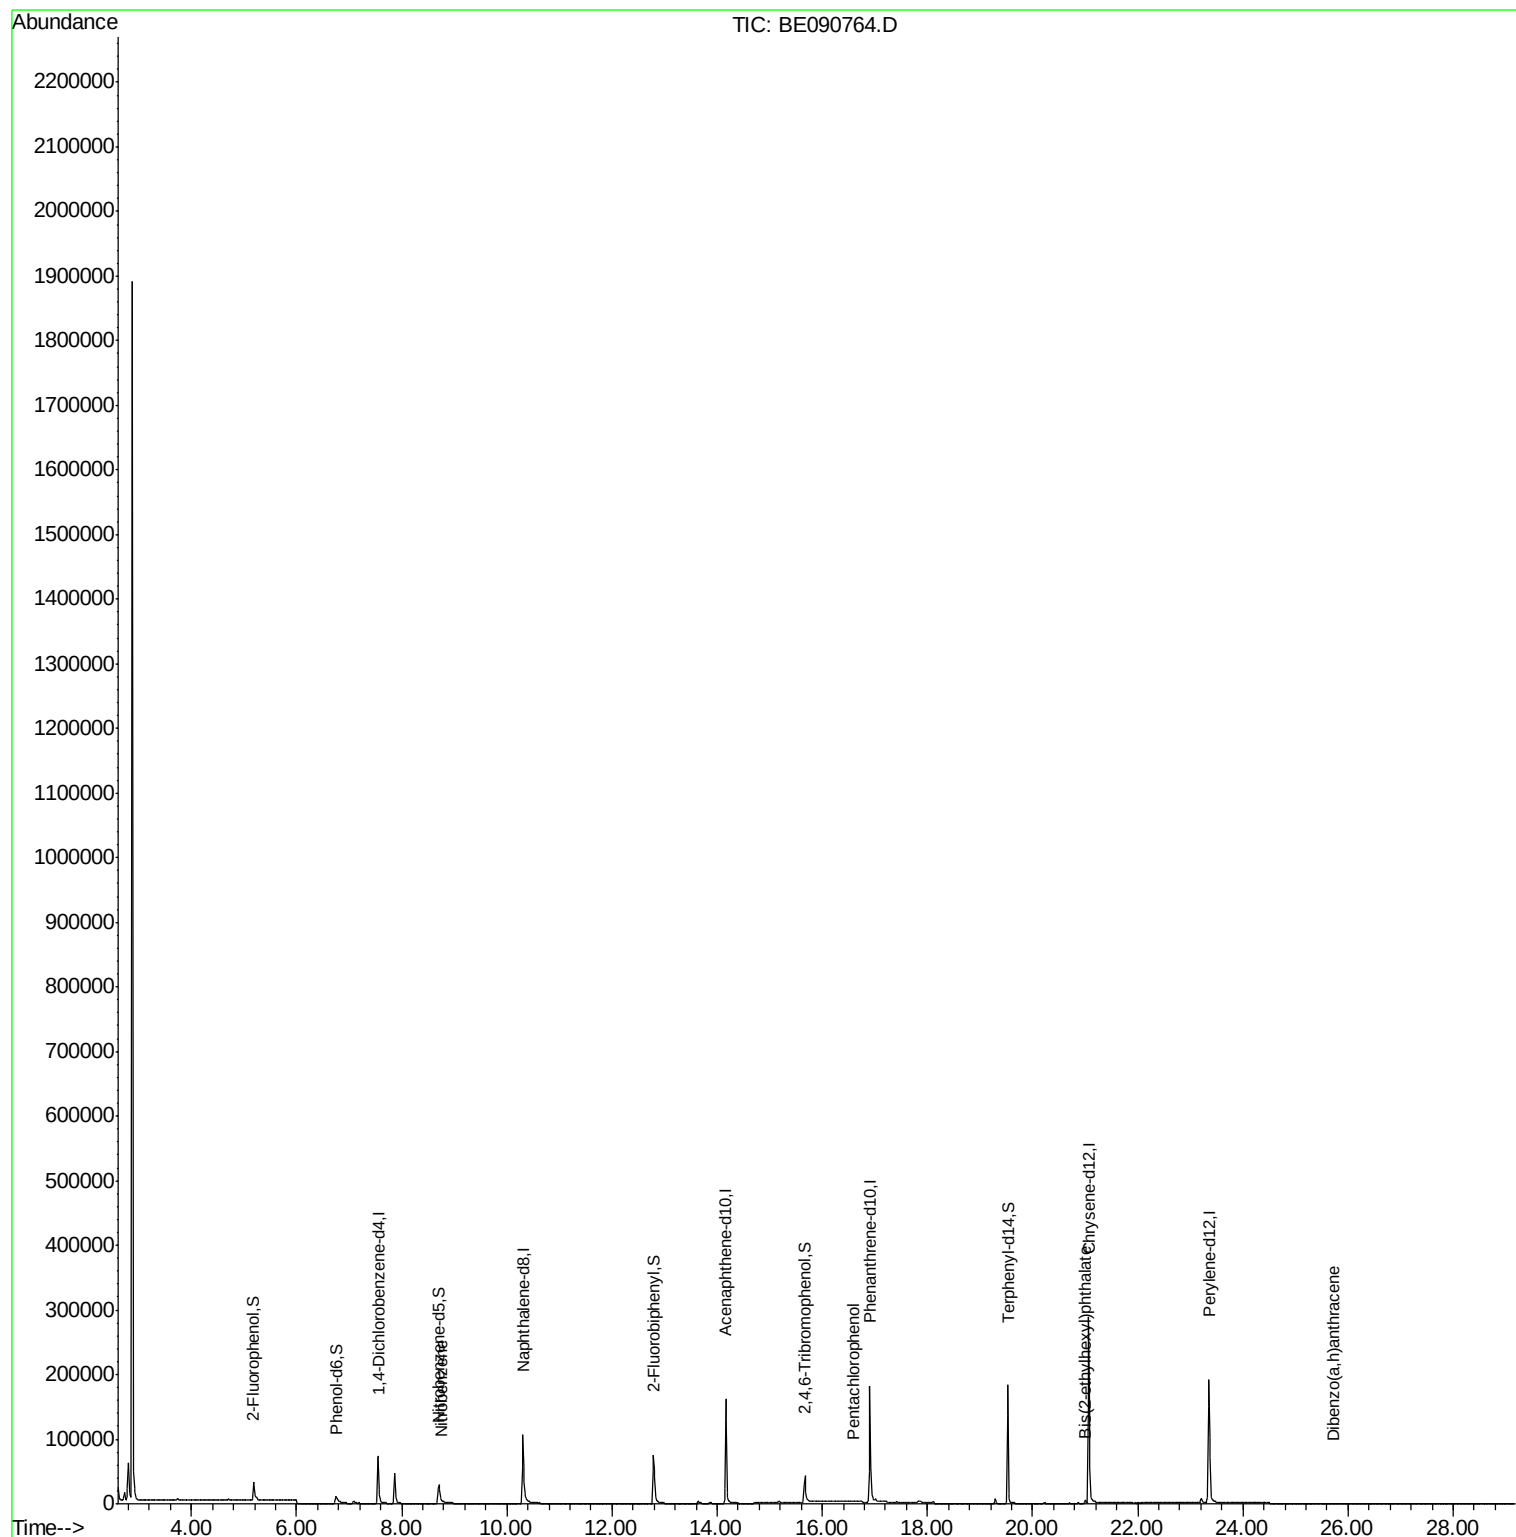



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.55 min Scan# 838

Delta R.T. -0.00 min

Lab File: BE090764.D

Acq: 10 Sep 2015 16:55

Instrument :

BNA_E

ClientSampleId :

090515-D534-F-D-B


Tot Ion:152 Resp: 43424

Ion Ratio Lower Upper

152 100

150 153.0 122.2 183.4




115 65.4 51.0 76.4

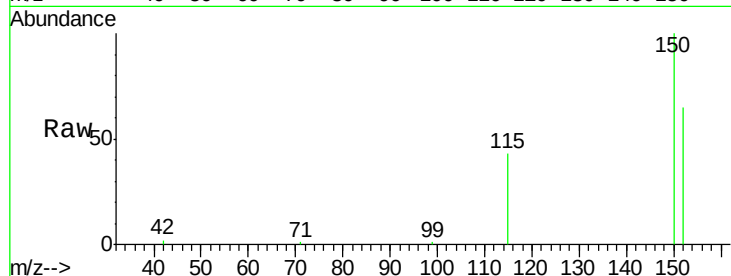

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

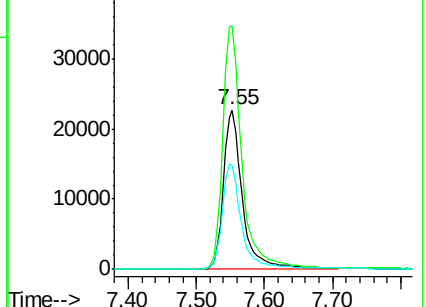

#2

1,4-Dioxane

Concen: Below Cal

RT: 3.20 min Scan# 88

Delta R.T. 0.04 min

Lab File: BE090764.D

Acq: 10 Sep 2015 16:55


Tgt Ion: 88 Resp: 21

Ion Ratio Lower Upper

88 100

58 0.0 68.4 102.6#



43 0.0 26.9 40.3#




Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

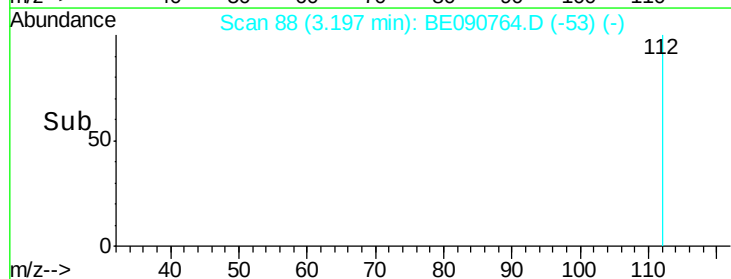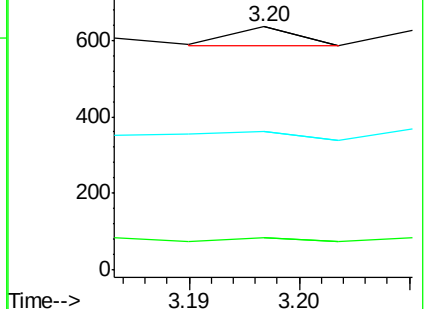




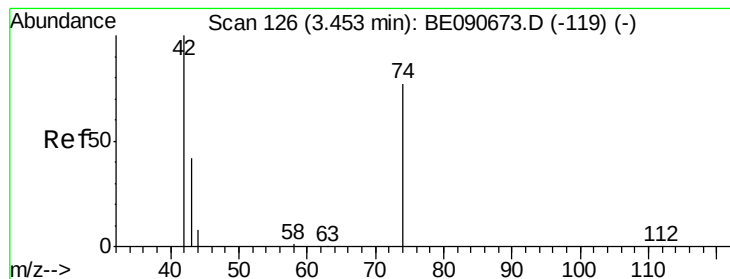


#3

n-Nitrosodimethylamine
 Concen: Below Cal
 RT: 3.46 min Scan# 127
 Delta R.T. 0.01 min
 Lab File: BE090764.D
 Acq: 10 Sep 2015 16:55

Instrument :
 BNA_E
 ClientSampleId :
 090515-D534-F-D-B




Tot Ion: 42 Resp: 97
 Ion Ratio Lower Upper
 42 100
 74 0.0 83.7 125.5#
 44 102.1 10.0 15.0#

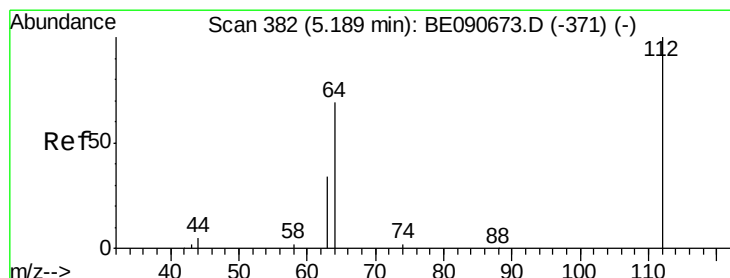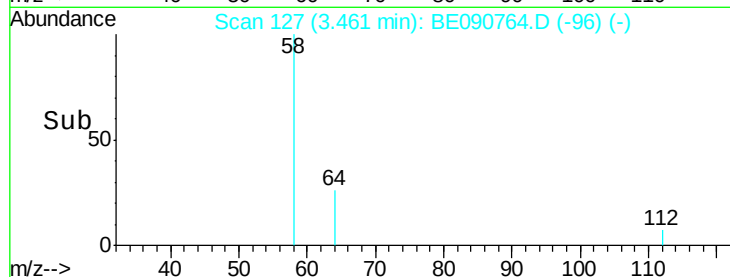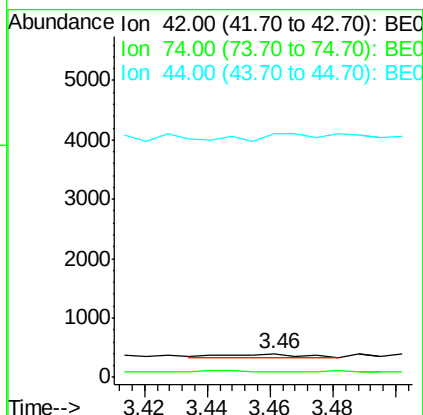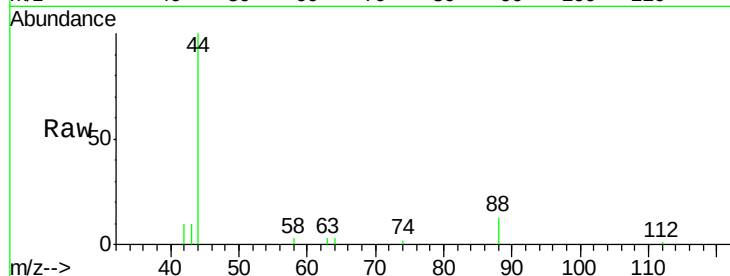


#4

2-Fluorophenol
 Concen: 3.67 ng
 RT: 5.18 min Scan# 381
 Delta R.T. -0.00 min
 Lab File: BE090764.D
 Acq: 10 Sep 2015 16:55

Tgt Ion: 112 Resp: 30948
 Ion Ratio Lower Upper
 112 100
 64 72.1 57.3 85.9
 63 37.2 29.2 43.8

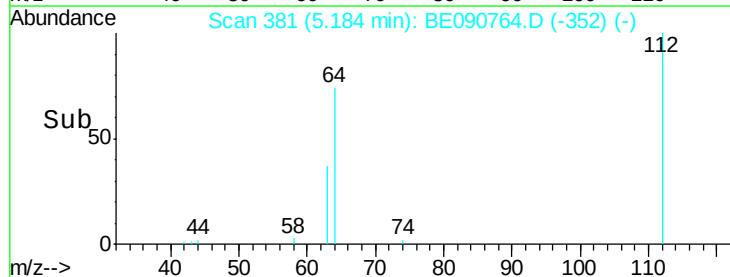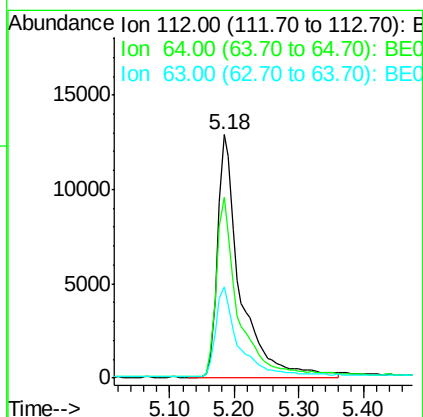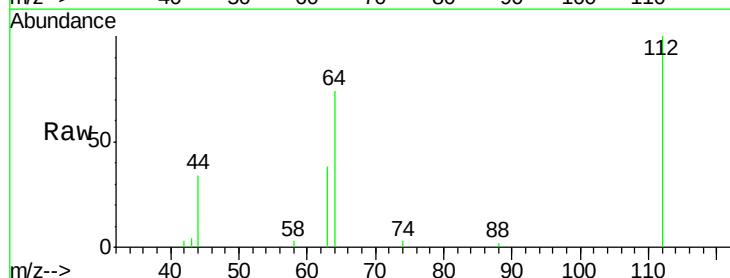

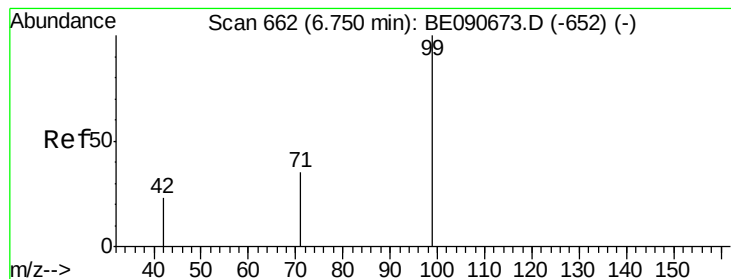

#5

Phenol-d6

Concen: 2.30 ng

RT: 6.75 min Scan# 662

Delta R.T. 0.00 min

Lab File: BE090764.D

Acq: 10 Sep 2015 16:55

Instrument :

BNA_E

ClientSampleId :

090515-D534-F-D-B


Tot Ion: 99 Resp: 27864

Ion Ratio Lower Upper




99 100

42 21.9 16.8 25.2

71 36.5 28.3 42.5



Abundance Ion 99.00 (98.70 to 99.70): BE0
Ion 42.00 (41.70 to 42.70): BE0
Ion 71.00 (70.70 to 71.70): BE0

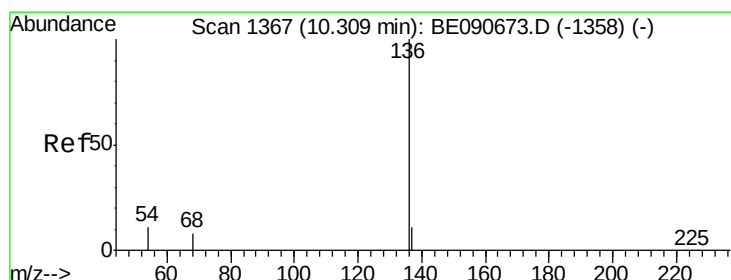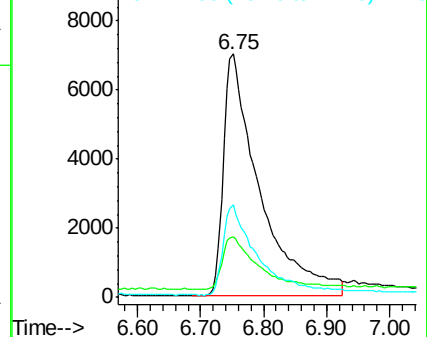

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.31 min Scan# 1367

Delta R.T. 0.00 min

Lab File: BE090764.D

Acq: 10 Sep 2015 16:55

Tgt Ion: 136 Resp: 194466


Ion Ratio Lower Upper

136 100



137 10.8 8.7 13.1


54 11.3 9.0 13.6

68 8.3 6.3 9.5



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BE0
Ion 68.00 (67.70 to 68.70): BE0

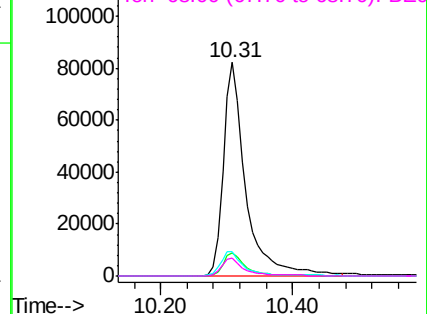

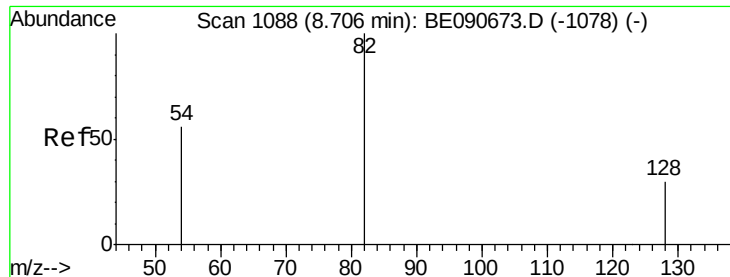

#7

Nitrobenzene-d5

Concen: 3.89 ng

RT: 8.71 min Scan# 1088

Delta R.T. 0.00 min

Lab File: BE090764.D

Acq: 10 Sep 2015 16:55

Instrument :

BNA_E

ClientSampleId :

090515-D534-F-D-B





Tot Ion: 82 Resp: 50037

Ion Ratio Lower Upper

82 100

128 29.7 25.0 37.4

54 59.3 46.3 69.5

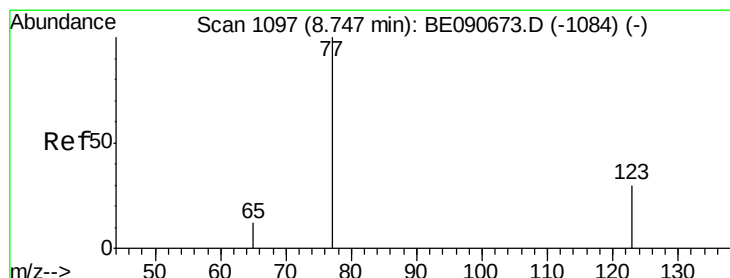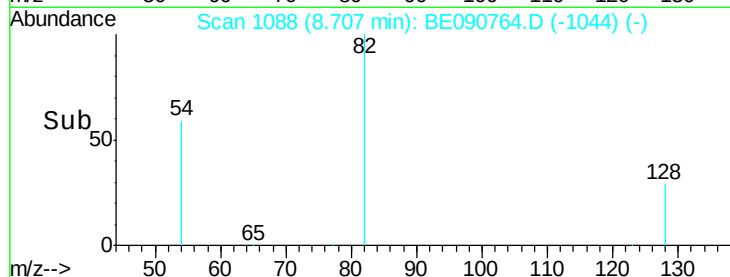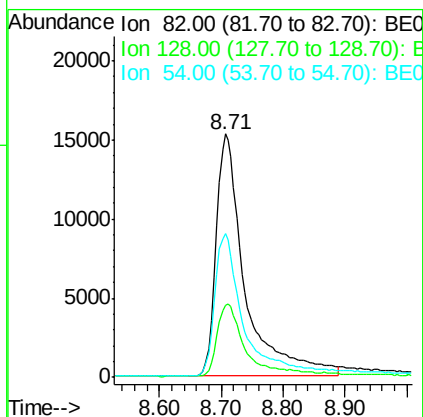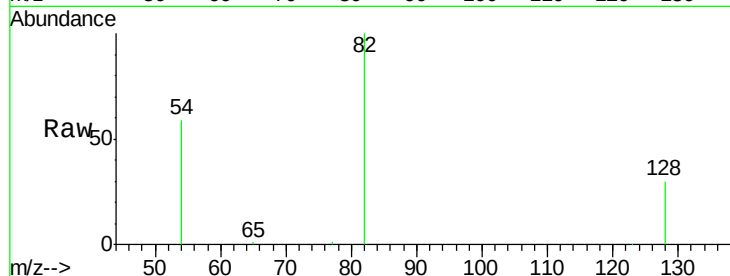

#8

Nitrobenzene

Concen: 0.11 ng

RT: 8.76 min Scan# 1099

Delta R.T. 0.01 min

Lab File: BE090764.D

Acq: 10 Sep 2015 16:55




Tgt Ion: 77 Resp: 29


Ion Ratio Lower Upper

77 100

123 44.8 25.1 37.7#

65 0.0 9.9 14.9#

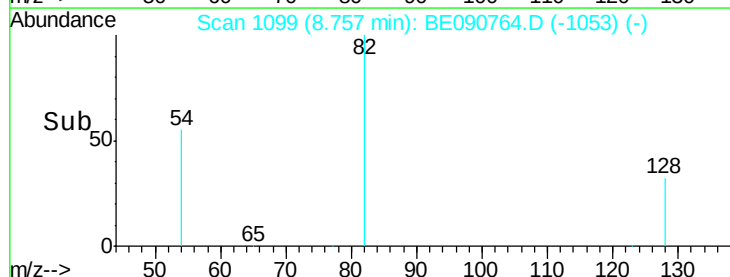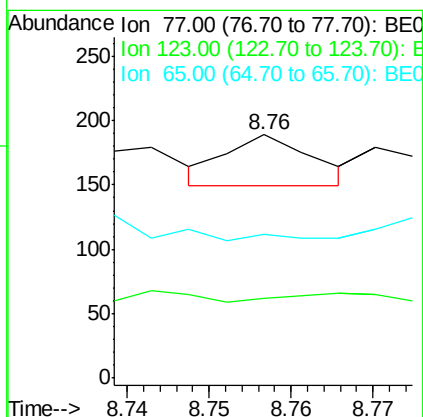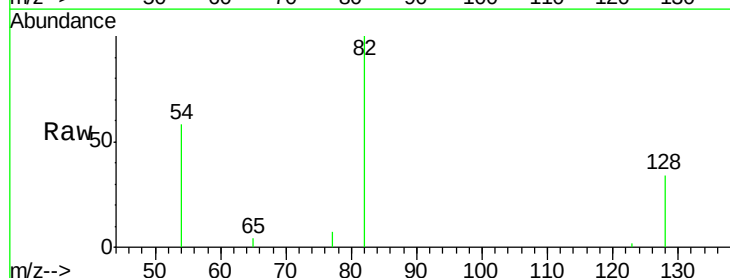

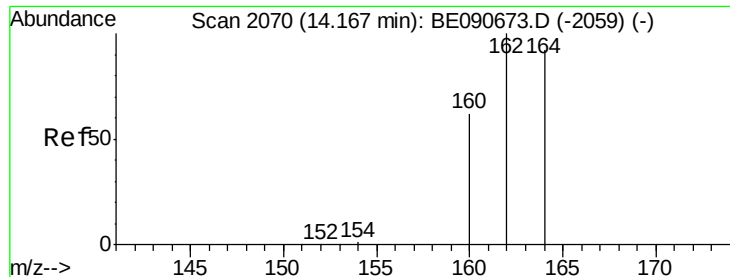

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.17 min Scan# 2070

Delta R.T. 0.00 min

Lab File: BE090764.D

Acq: 10 Sep 2015 16:55

Instrument :

BNA_E

ClientSampleId :

090515-D534-F-D-B


Tot Ion:164 Resp: 98716

Ion Ratio Lower Upper

164 100

162 107.2 86.8 130.2




160 59.6 53.9 80.9

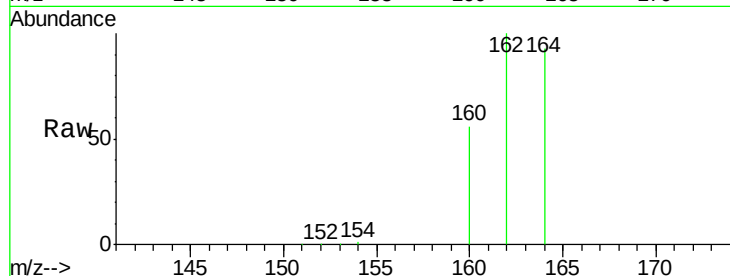

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

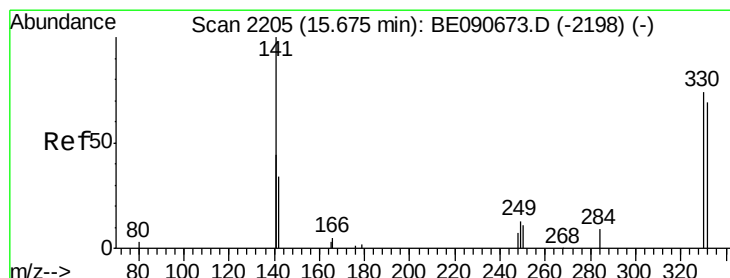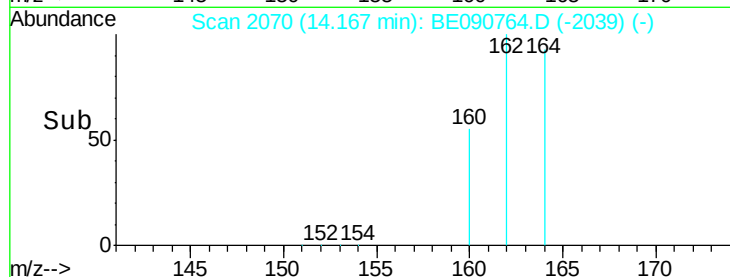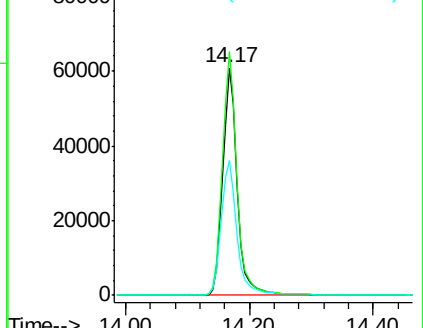

#13

2,4,6-Tribromophenol

Concen: 8.12 ng

RT: 15.67 min Scan# 2204

Delta R.T. -0.00 min

Lab File: BE090764.D

Acq: 10 Sep 2015 16:55


Tgt Ion:330 Resp: 23527

Ion Ratio Lower Upper

330 100

332 96.5 74.9 112.3



141 177.2 145.2 217.8

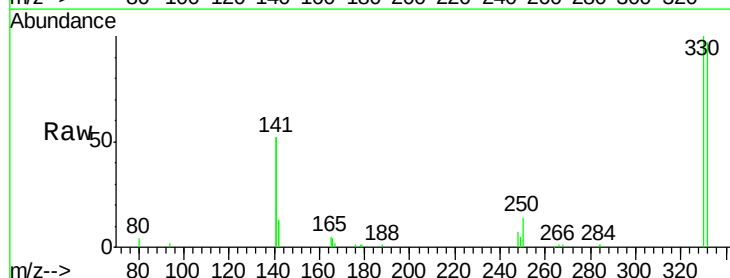


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



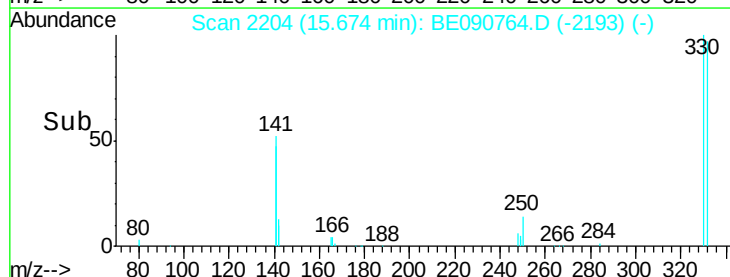
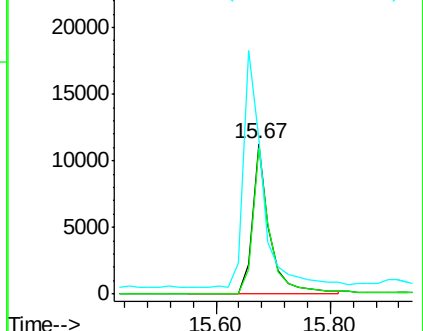


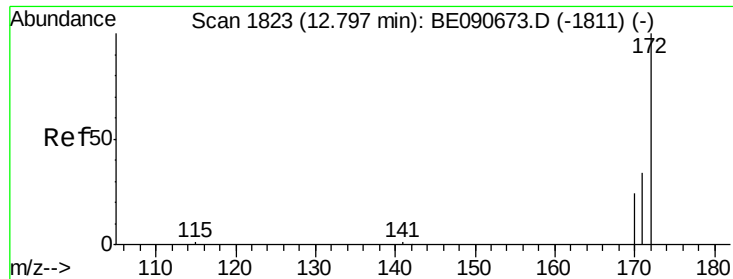

#14
2-Fluorobiphenyl
Concen: 4.05 ng
RT: 12.79 min Scan# 1822
Delta R.T. -0.01 min
Lab File: BE090764.D
Acq: 10 Sep 2015 16:55




Instrument :
BNA_E
ClientSampleId :
090515-D534-F-D-B


Tot Ion:172 Resp: 110751
Ion Ratio Lower Upper
172 100
171 35.3 27.8 41.8
170 24.1 19.8 29.6

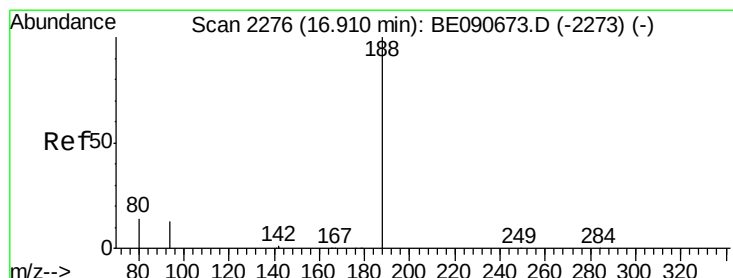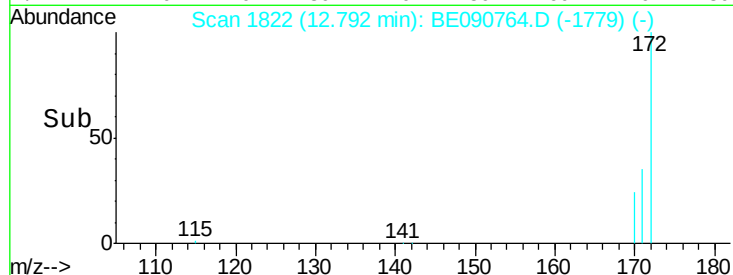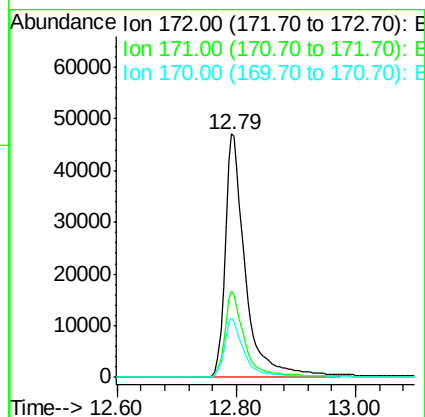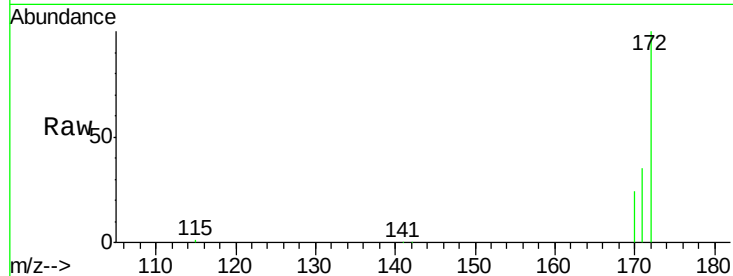

#18
Phenanthrene-d10
Concen: 5.00 ng
RT: 16.91 min Scan# 2275
Delta R.T. -0.00 min
Lab File: BE090764.D
Acq: 10 Sep 2015 16:55

Tgt Ion:188 Resp: 238782
Ion Ratio Lower Upper
188 100
94 11.1 10.3 15.5
80 12.0 11.0 16.6

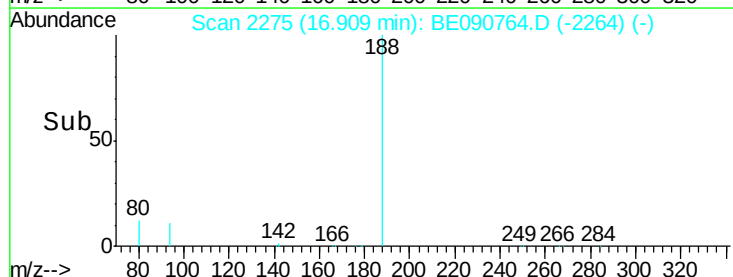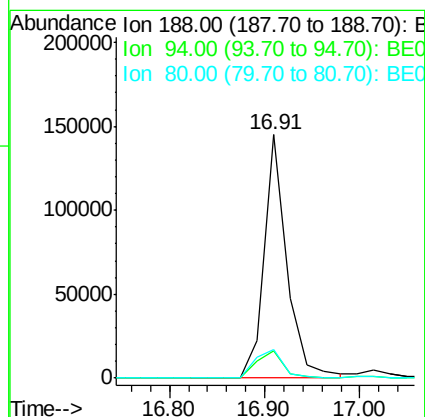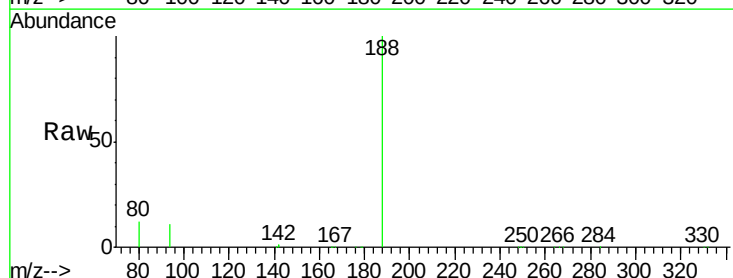



#20

Hexachlorobenzene

Concen: Below Cal

RT: 16.23 min Scan# 2236

Delta R.T. -0.00 min

Lab File: BE090764.D

Acq: 10 Sep 2015 16:55

Instrument :

BNA_E

ClientSampleId :

090515-D534-F-D-B


Tot Ion:284 Resp: 203

Ion Ratio Lower Upper

284 100

142 0.0 35.0 52.4#




249 37.9 25.5 38.3

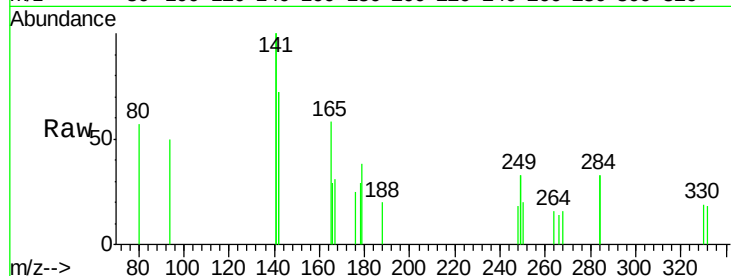

Abundance Ion 283.80 (283.50 to 284.50): E

Ion 142.00 (141.70 to 142.70): E

Ion 249.00 (248.70 to 249.70): E

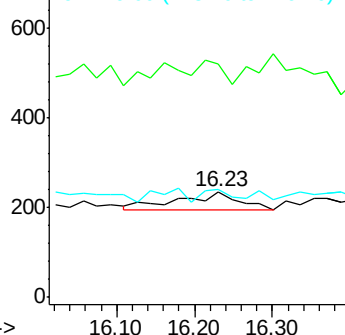

#21

Pentachlorophenol

Concen: 0.47 ng

RT: 16.60 min Scan# 2257

Delta R.T. -0.00 min

Lab File: BE090764.D

Acq: 10 Sep 2015 16:55


Tgt Ion:266 Resp: 33

Ion Ratio Lower Upper

266 100

268 101.7 49.6 74.4#



264 87.9 53.9 80.9#




Abundance Ion 265.70 (265.40 to 266.40): E

Ion 268.00 (267.70 to 268.70): E

Ion 264.00 (263.70 to 264.70): E

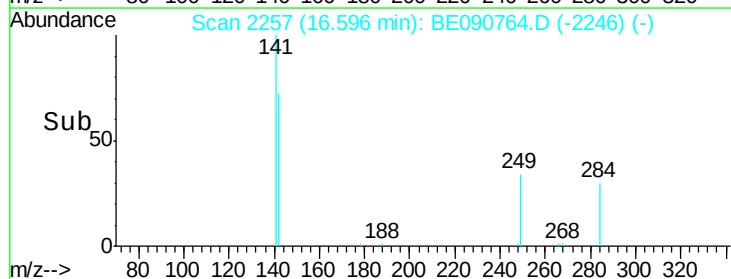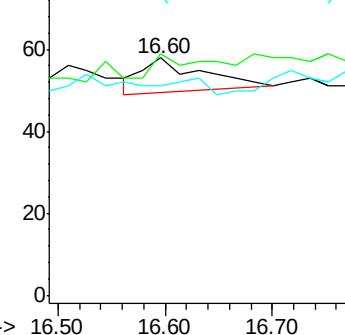



#25

Chrysene-d12

Concen: 5.00 ng

RT: 21.07 min Scan# 2860

Delta R.T. -0.01 min

Lab File: BE090764.D

Acq: 10 Sep 2015 16:55

Instrument :

BNA_E

ClientSampleId :

090515-D534-F-D-B


Tot Ion:240 Resp: 296772

Ion Ratio Lower Upper

240 100

120 15.9 10.1 15.1#


236 28.2 21.9 32.9





Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

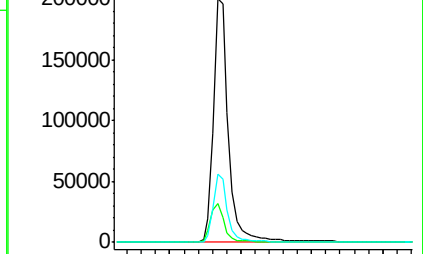

Time-->



#27

Terphenyl-d14

Concen: 5.77 ng

RT: 19.53 min Scan# 2608

Delta R.T. -0.01 min

Lab File: BE090764.D

Acq: 10 Sep 2015 16:55


Tgt Ion:244 Resp: 189551

Ion Ratio Lower Upper

244 100

212 8.2 6.9 10.3


122 15.4 12.9 19.3




Abundance Ion 244.00 (243.70 to 244.70): E


Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

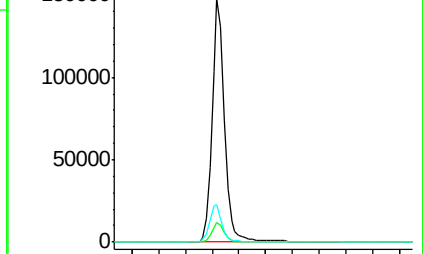

Time-->

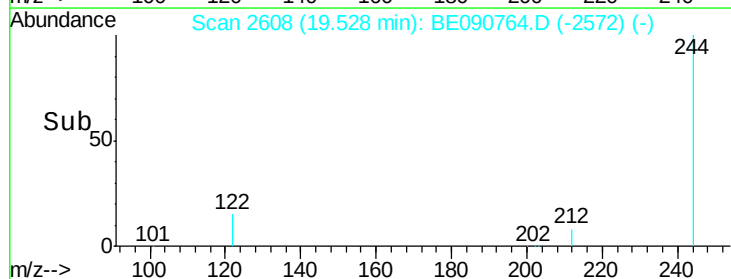



#29

Chrysene

Concen: Below Cal

RT: 21.11 min Scan# 2866

Delta R.T. 0.00 min

Lab File: BE090764.D

Acq: 10 Sep 2015 16:55

Instrument :

BNA_E

ClientSampleId :

090515-D534-F-D-B


Tot Ion:228 Resp: 595

Ion Ratio Lower Upper

228 100

226 44.7 24.2 36.4#




229 40.2 15.3 22.9#



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

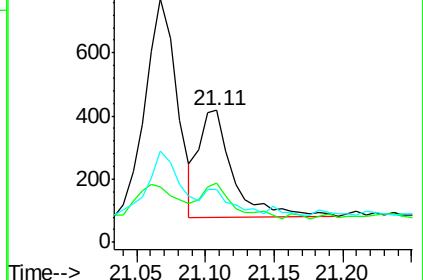

#30

Bis(2-ethylhexyl)phthalate

Concen: 0.35 ng

RT: 21.00 min Scan# 2850

Delta R.T. -0.01 min

Lab File: BE090764.D

Acq: 10 Sep 2015 16:55


Tgt Ion:149 Resp: 4884

Ion Ratio Lower Upper

149 100

167 23.3 20.1 30.1



279 3.3 2.3 3.5




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E



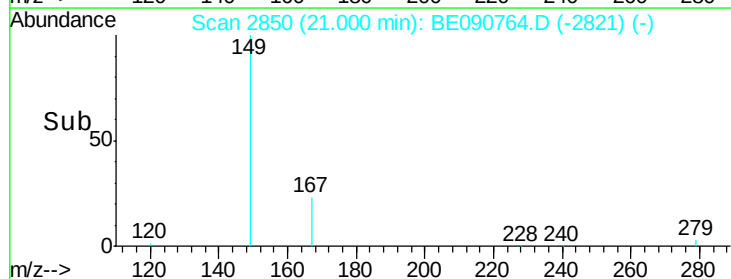
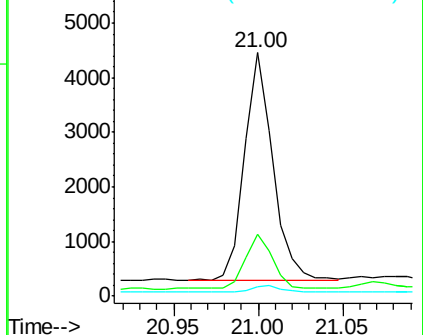


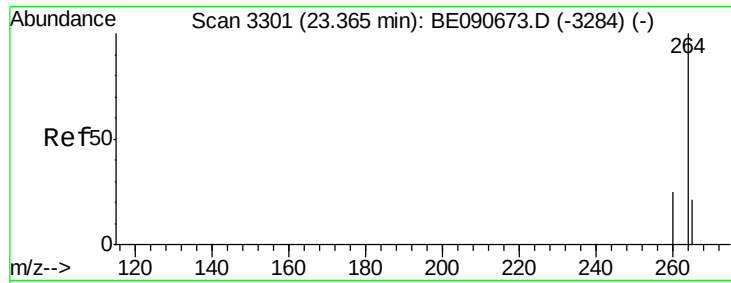

#32
Pervlene-d12
Concen: 5.00 ng
RT: 23.36 min Scan# 3298
Delta R.T. -0.01 min
Lab File: BE090764.D
Acq: 10 Sep 2015 16:55

Instrument :
BNA_E
ClientSampleId :
090515-D534-F-D-B

Tot Ion:264 Resp: 269050
Ion Ratio Lower Upper
264 100
260 24.9 19.7 29.5
265 21.4 17.5 26.3

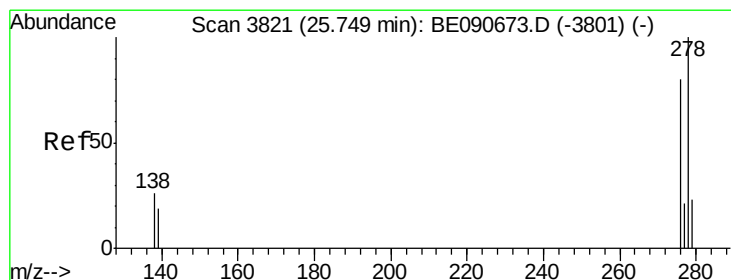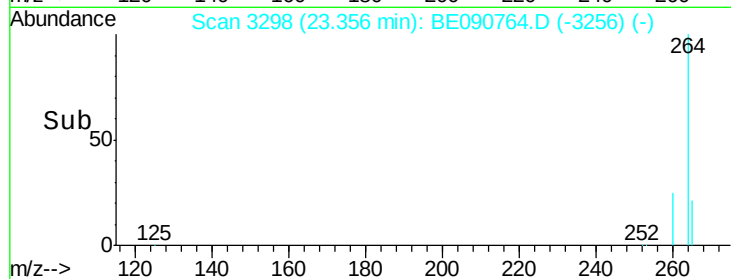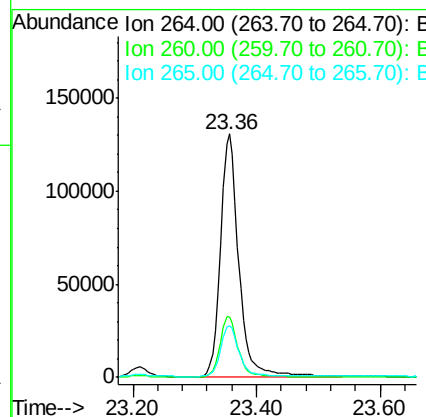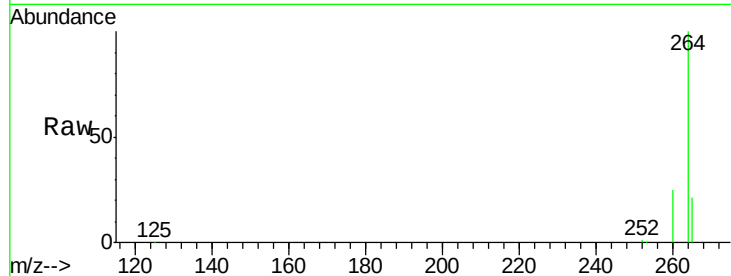

#36
Dibenzo(a,h)anthracene
Concen: 0.14 ng
RT: 25.72 min Scan# 3814
Delta R.T. -0.03 min
Lab File: BE090764.D
Acq: 10 Sep 2015 16:55

Tgt Ion:278 Resp: 31
Ion Ratio Lower Upper
278 100
139 147.5 15.4 23.0#
279 118.8 18.8 28.2#

